


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020123\
Data File : BF132261.D
Acq On : 01 Feb 2023 15:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 02 01:30:34 2023

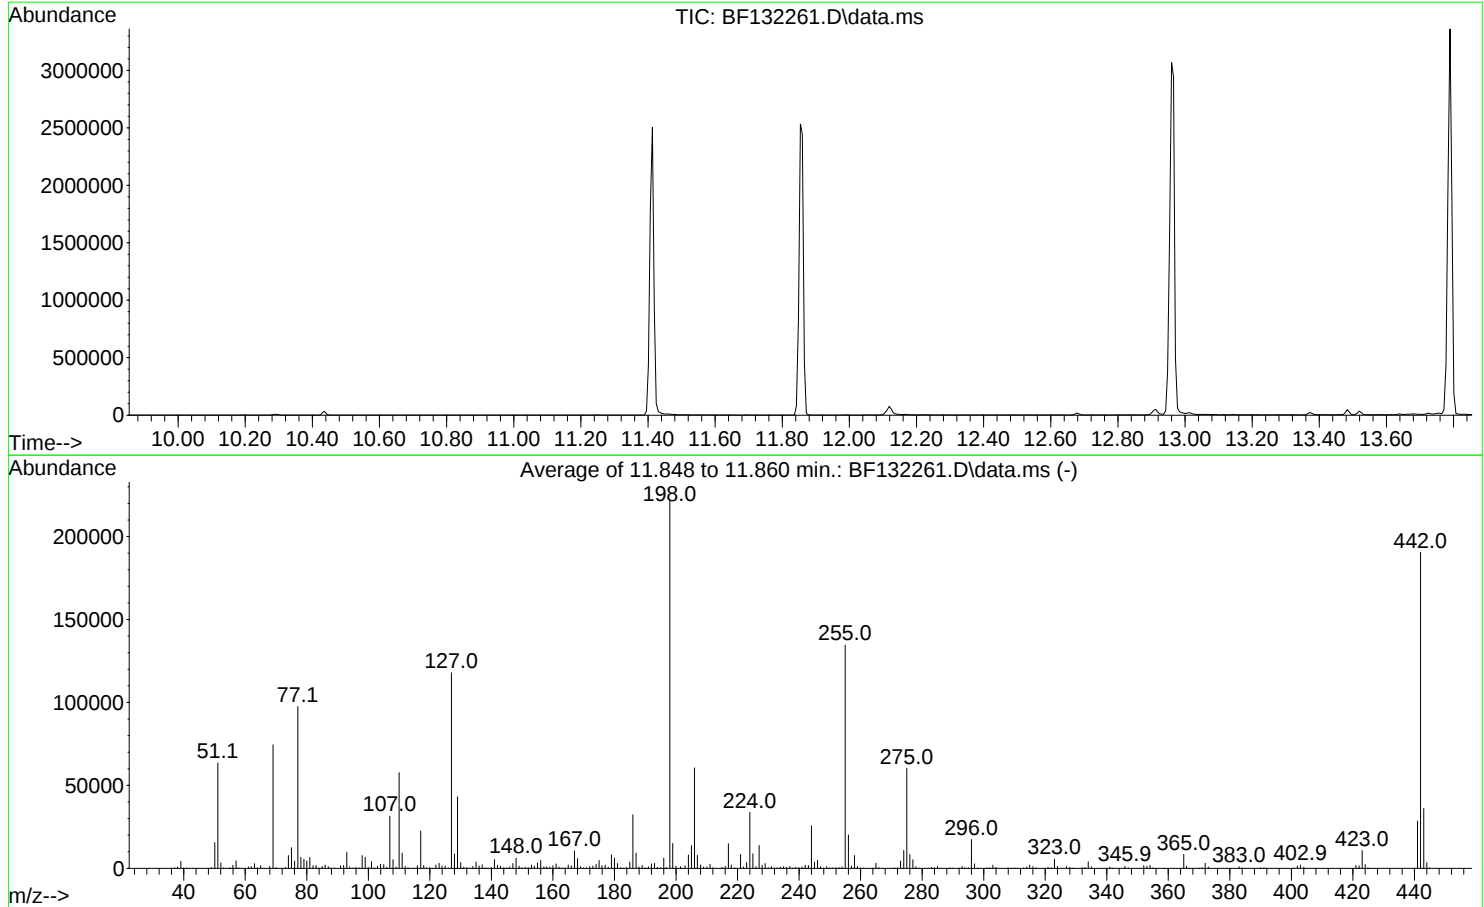




AutoFind: Scans 1532, 1533, 1534; Background Corrected with Scan 1527

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.7	63565	PASS
68	69	0.00	2	1.5	1130	PASS
69	198	0.00	100	33.6	74440	PASS
70	69	0.00	2	0.5	402	PASS
127	198	10	80	53.1	117856	PASS
197	198	0.00	2	0.2	411	PASS
198	198	100	100	100.0	221781	PASS
199	198	5	9	6.7	14960	PASS
275	198	10	60	27.1	60200	PASS
365	198	1	100	3.7	8308	PASS
441	198	0.01	100	12.8	28482	PASS
442	442	50	100	100.0	190477	PASS
443	442	15	24	18.9	36038	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020123\
 Data File : BF132261.D
 Acq On : 01 Feb 2023 15:38
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 02 05:16:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 02 01:30:34 2023
 Response via : Initial Calibration

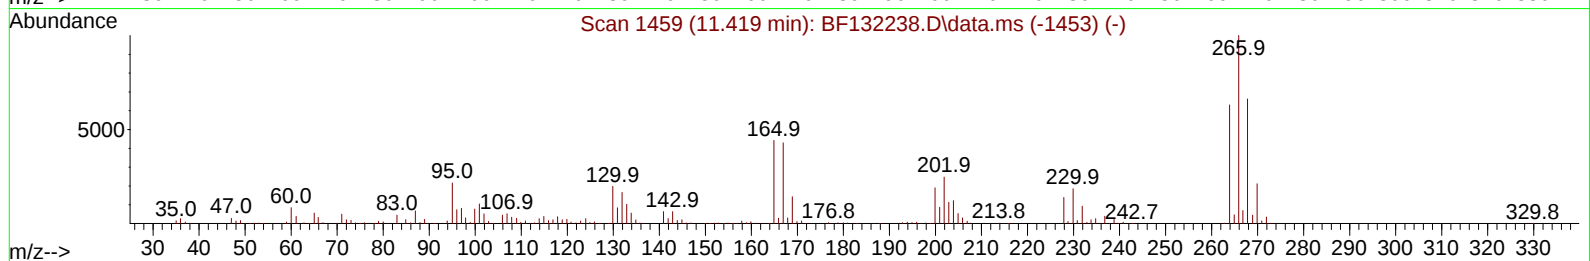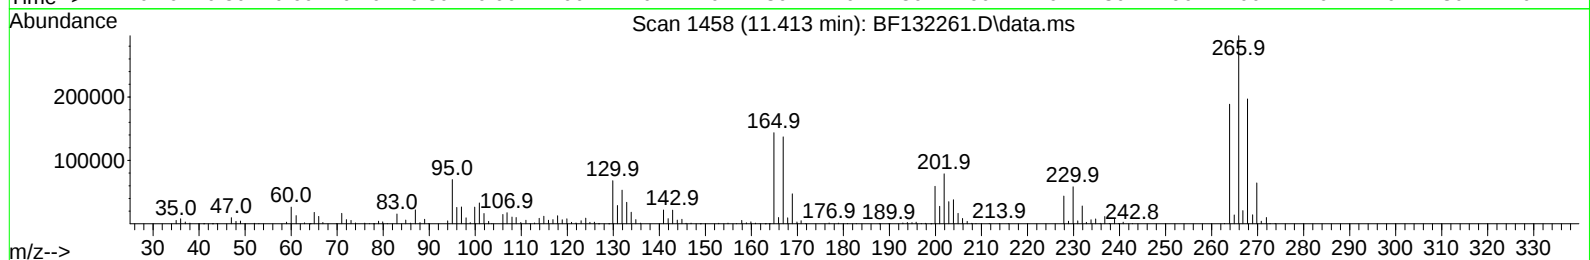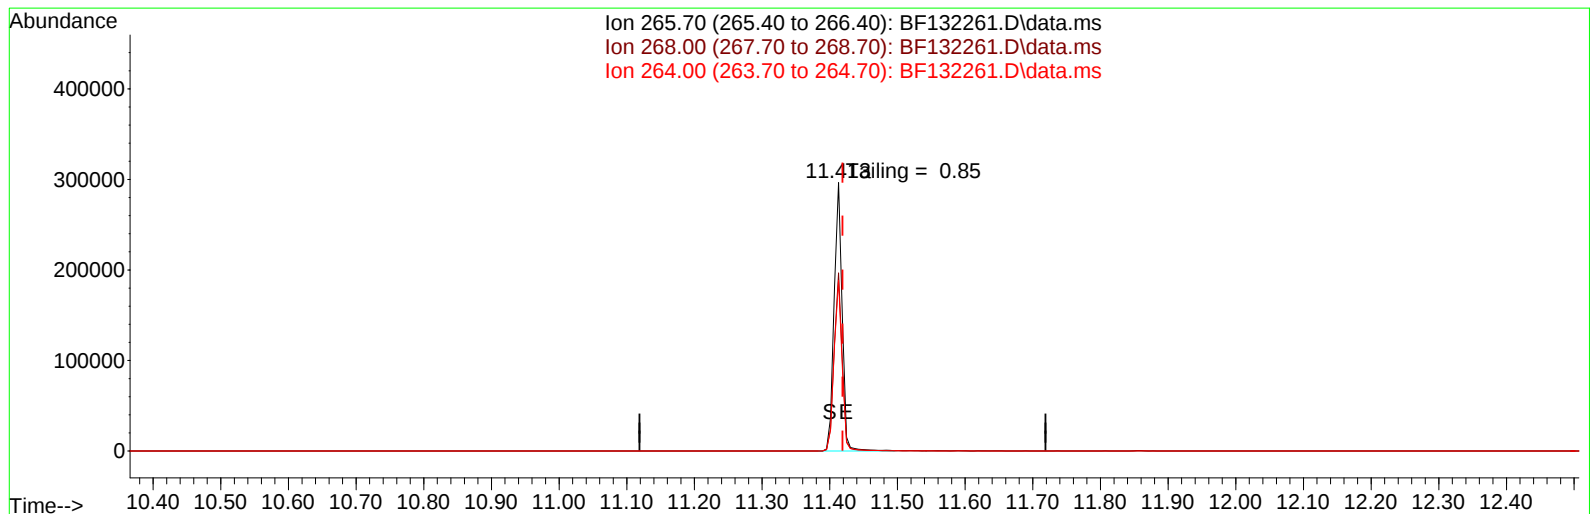

TIC: BF132261.D\data.ms

(70) Pentachlorophenol (C)

11.413min (-0.006) 569426.91 ng




response 244082

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	66.36
264.00	63.10	63.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020123\
Data File : BF132261.D
Acq On : 01 Feb 2023 15:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 02 05:16:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 02 01:30:34 2023
Response via : Initial Calibration

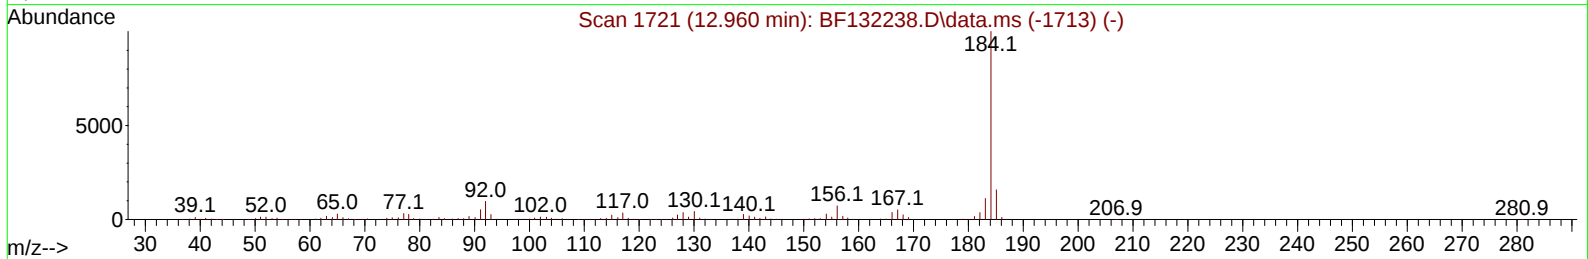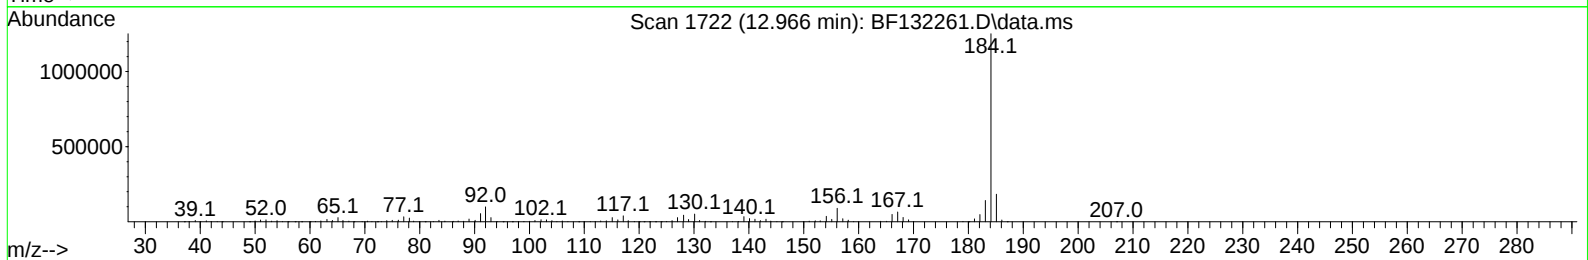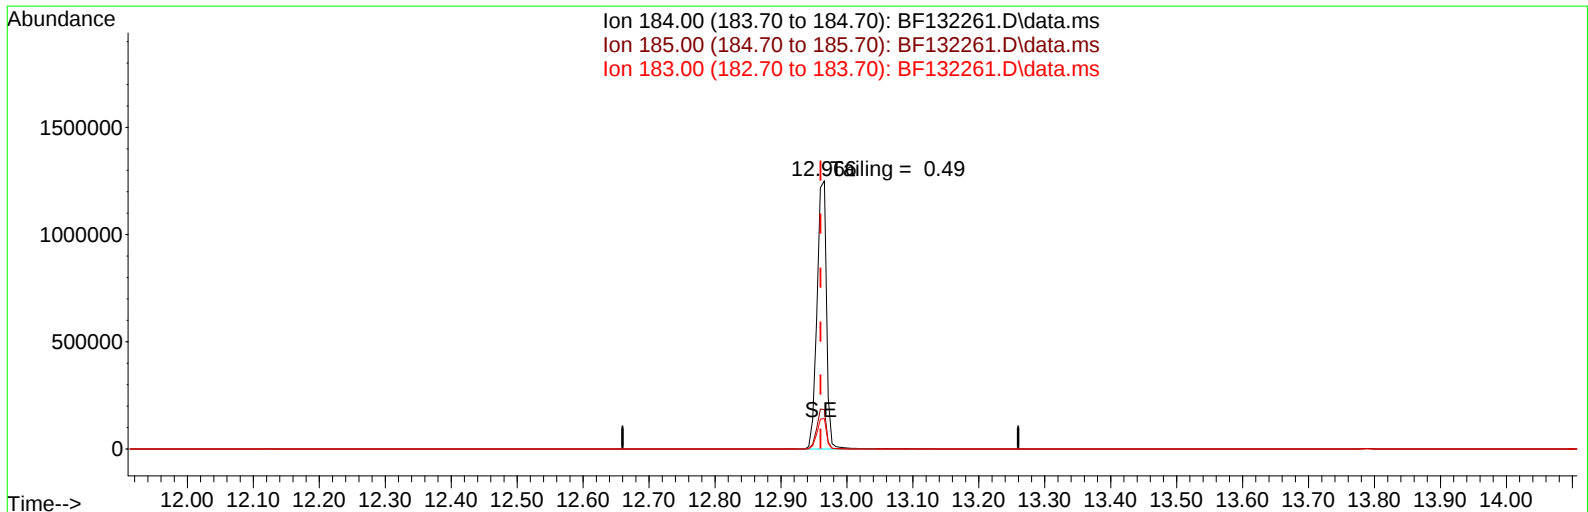

TIC: BF132261.D\data.ms

(77) Benzidine

12.966min (+ 0.006) 281278.87 ng

response 1248895

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.65
183.00	11.10	11.32
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/1/2023	BNA_F	<u>BF132261.D</u>
Compound Name	Response	Retention Time
DDT	542173	13.789
DDD	12224	13.483
DDE	548	13.148
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12772	554945	2.30

Instrument :
BNA_F
ClientSampleId :
DFTPP