
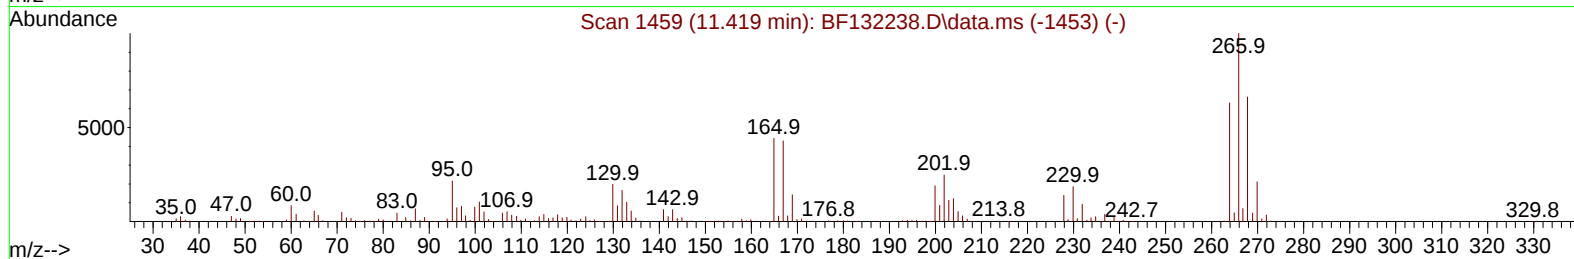
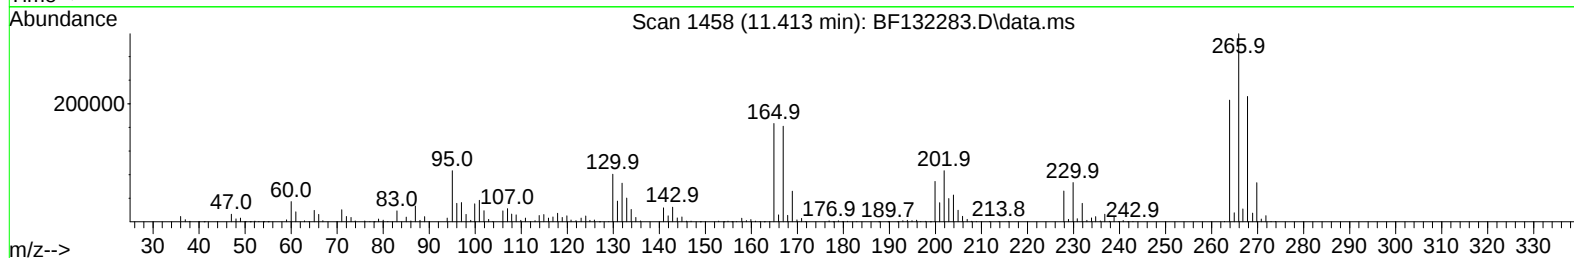


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020223\
Data File : BF132283.D
Acq On : 02 Feb 2023 10:07
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 03:17:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 02 01:30:34 2023
Response via : Initial Calibration

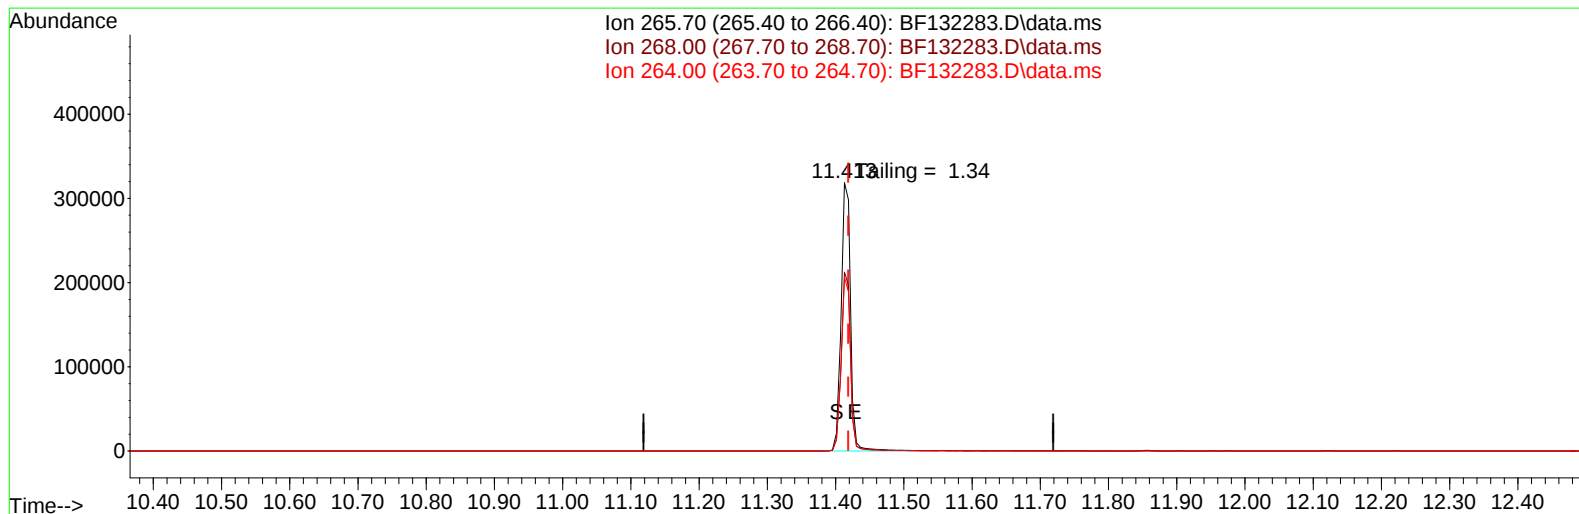

TIC: BF132283.D\data.ms

(70) Pentachlorophenol (C)




11.413min (-0.006) 163031.61 ng

response 305277

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	66.67
264.00	63.10	64.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020223\
Data File : BF132283.D
Acq On : 02 Feb 2023 10:07
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 03:17:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 02 01:30:34 2023
Response via : Initial Calibration

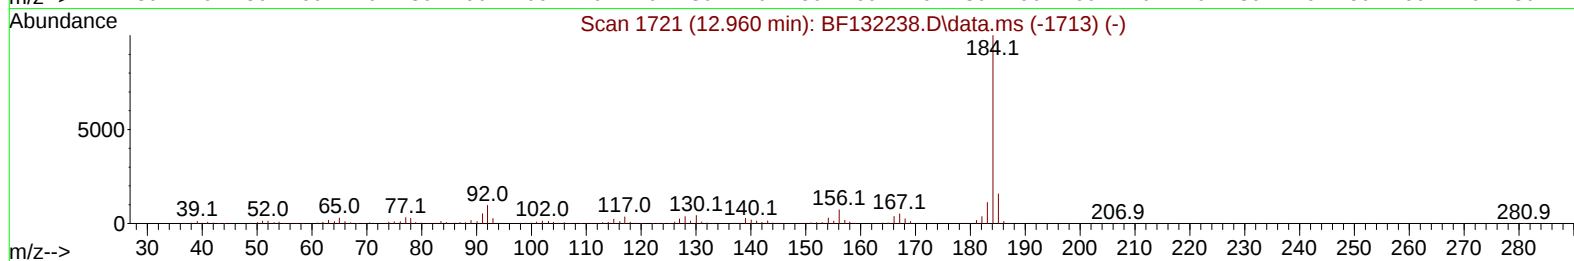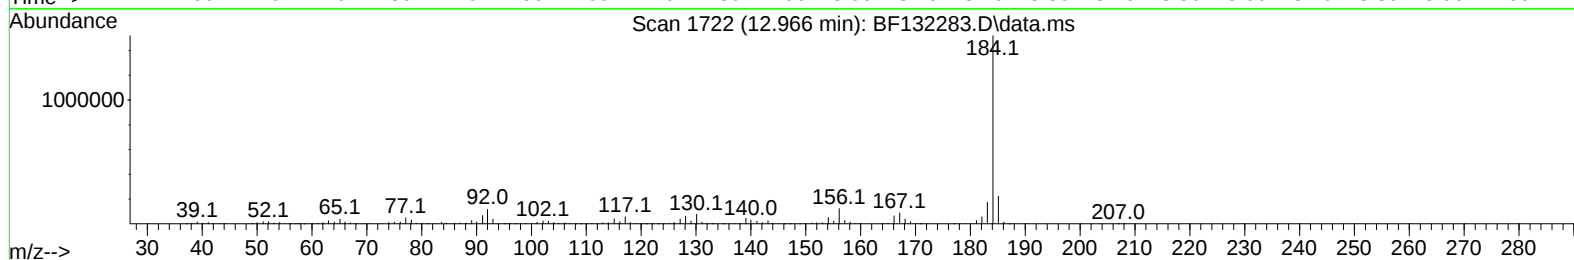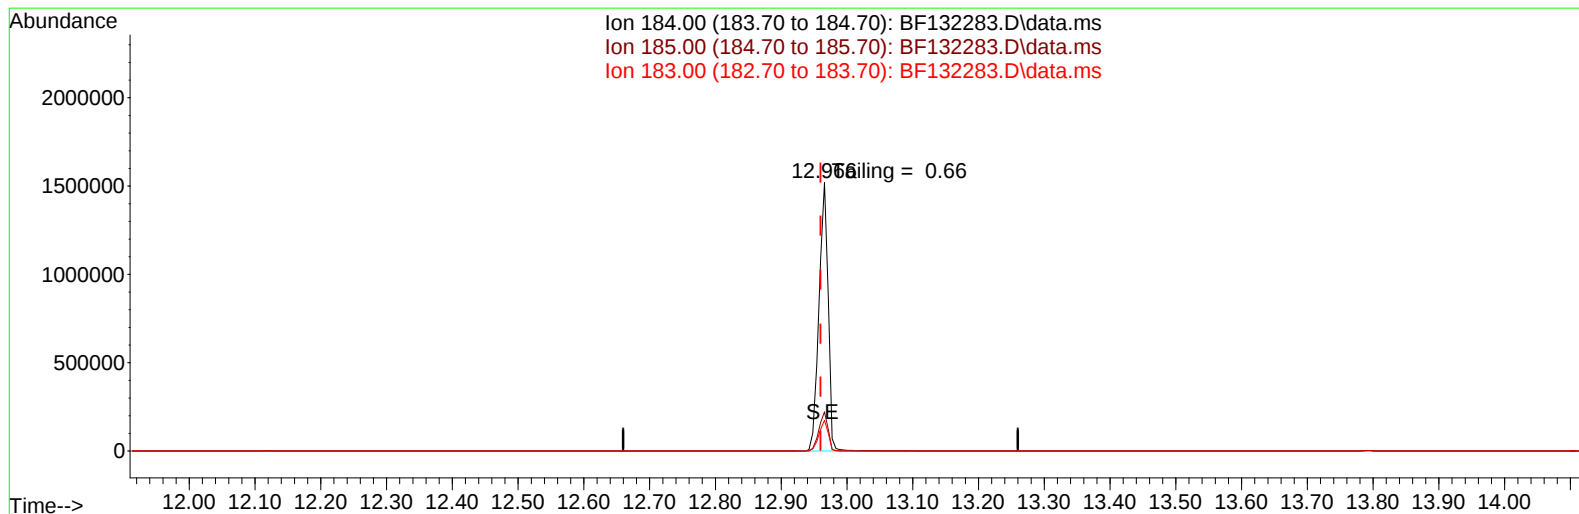

TIC: BF132283.D\data.ms

(77) Benzidine

12.966min (+ 0.006) 23205.74 ng

response 1484676

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.65
183.00	11.10	11.44
0.00	0.00	0.00