
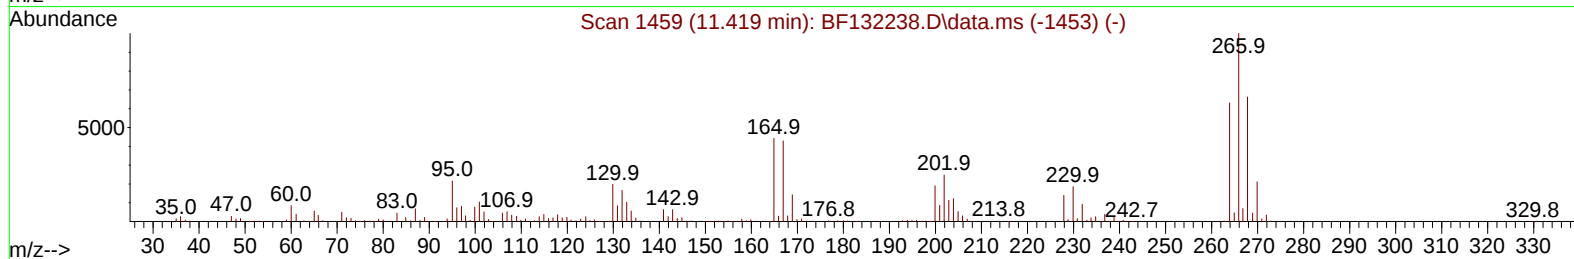
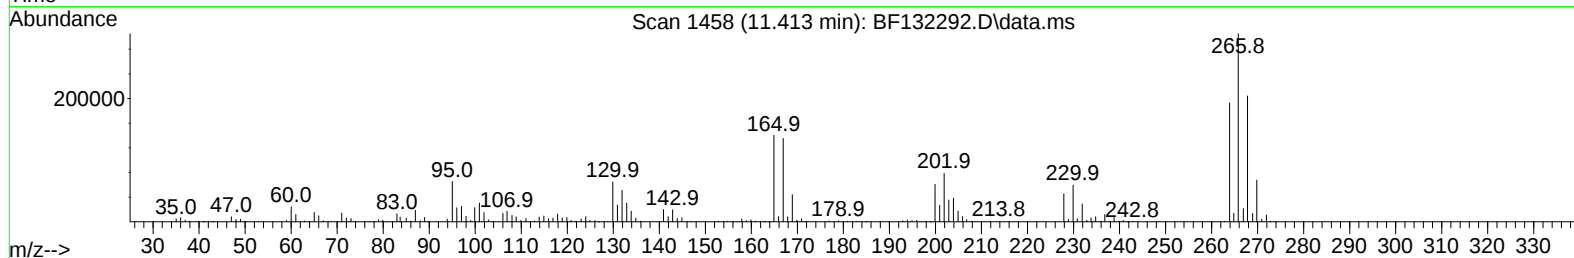


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020223\
Data File : BF132292.D
Acq On : 02 Feb 2023 15:08
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 04:15:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 02 01:30:34 2023
Response via : Initial Calibration

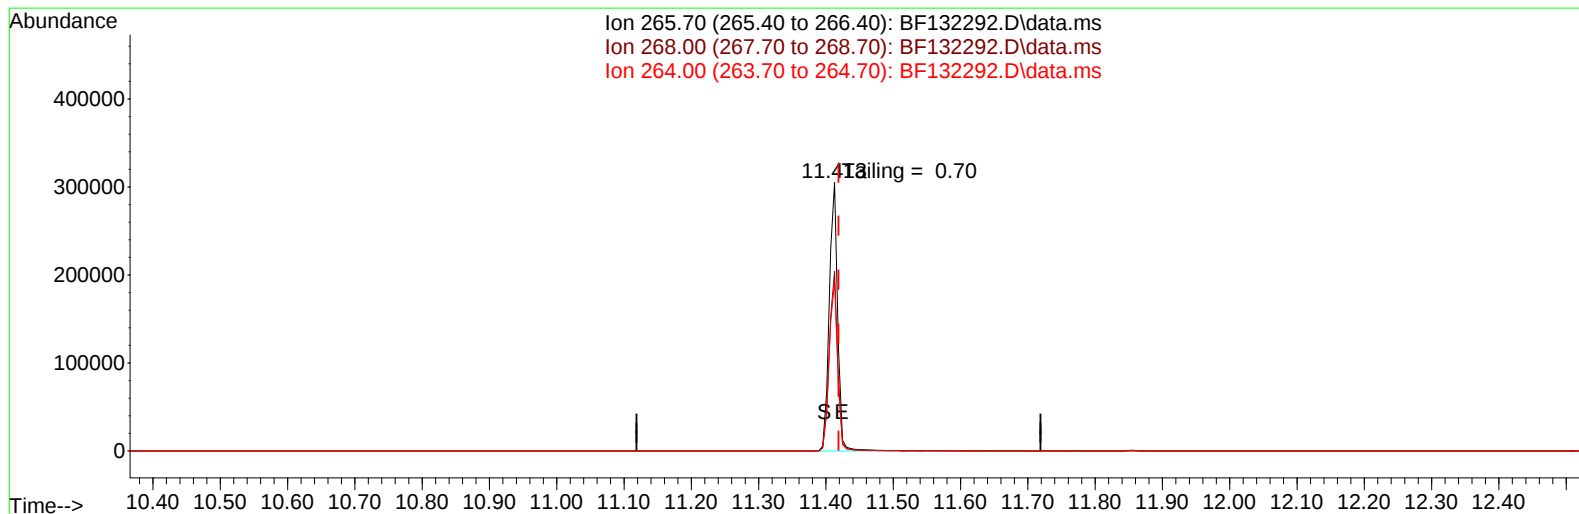

TIC: BF132292.D\data.ms

(70) Pentachlorophenol (C)




11.413min (-0.006) 219843.48 ng

response 266172

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	66.91
264.00	63.10	63.28
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020223\  
Data File : BF132292.D  
Acq On    : 02 Feb 2023  15:08  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Feb 03 04:15:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 02 01:30:34 2023
Response via : Initial Calibration

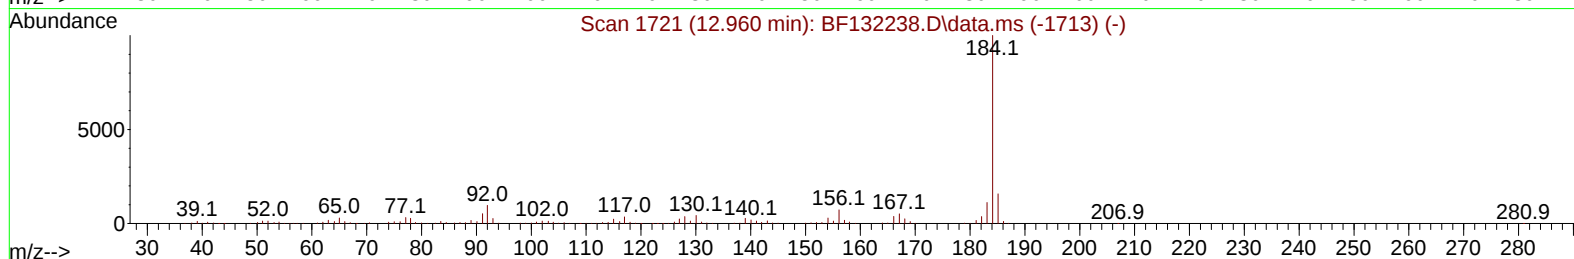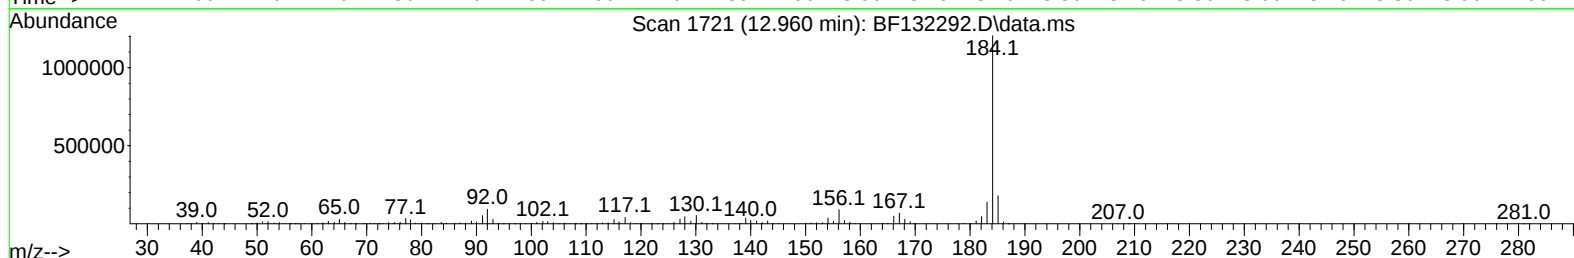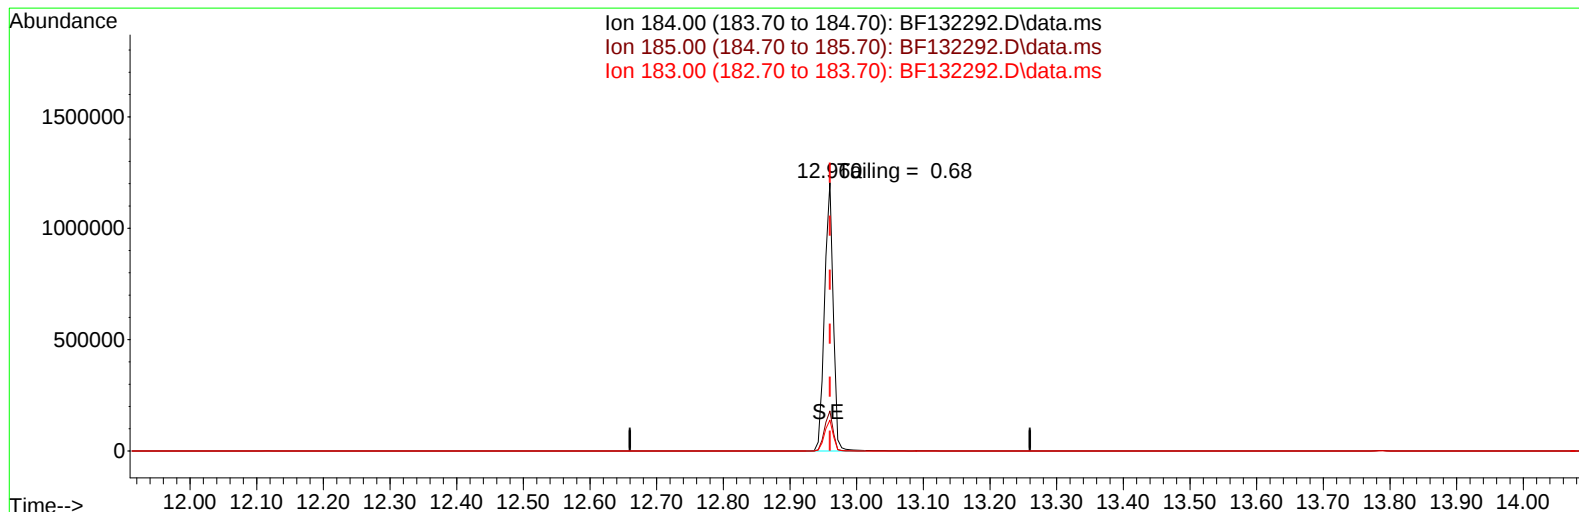

TIC: BF132292.D\data.ms

(77) Benzidine

12.960min (-0.000) 223462.34 ng

response **1085936**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.92
183.00	11.10	11.51
0.00	0.00	0.00