

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020223\
 Data File : BF132285.D
 Acq On : 02 Feb 2023 11:11
 Operator : CG\JU
 Sample : PB150609BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB150609BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF132285.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.331	417	424	435	rVB	1449617	2044797	28.23%	4.702%
2	5.707	482	488	491	rBV	4145851	4792131	66.16%	11.019%
3	6.684	647	654	657	rBV	3672791	4923617	67.98%	11.321%
4	7.066	715	719	722	rBV	1514502	1206330	16.65%	2.774%
5	7.631	808	815	818	rBV	2961110	3416373	47.17%	7.855%
6	8.354	932	938	941	rBV	2012658	1670197	23.06%	3.840%
7	9.437	1115	1122	1125	rBV	6364517	6560829	90.58%	15.086%
8	10.119	1232	1238	1241	rBV	2429865	1993642	27.52%	4.584%
9	10.919	1367	1374	1377	rBV	4687134	4767026	65.81%	10.961%
10	11.619	1489	1493	1496	rBV	2547656	2135511	29.48%	4.910%
11	13.219	1759	1765	1768	rBV	7075947	7243240	100.00%	16.655%
12	14.136	1913	1921	1931	rBV3	24308	75460	1.04%	0.174%
13	14.283	1941	1946	1949	rBV	1583975	1516820	20.94%	3.488%
14	15.866	2210	2215	2224	rBV	842788	1144492	15.80%	2.632%




Sum of corrected areas: 43490465

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020223\
Data File : BF132285.D
Acq On : 02 Feb 2023 11:11
Operator : CG\JU
Sample : PB150609BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB150609BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

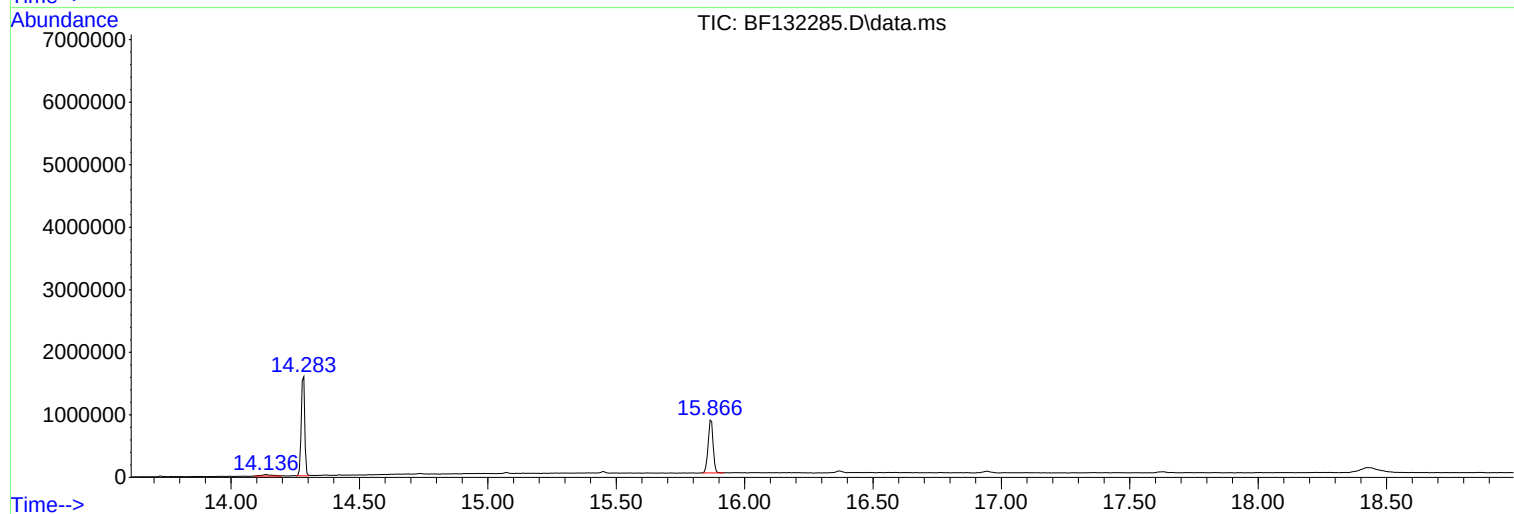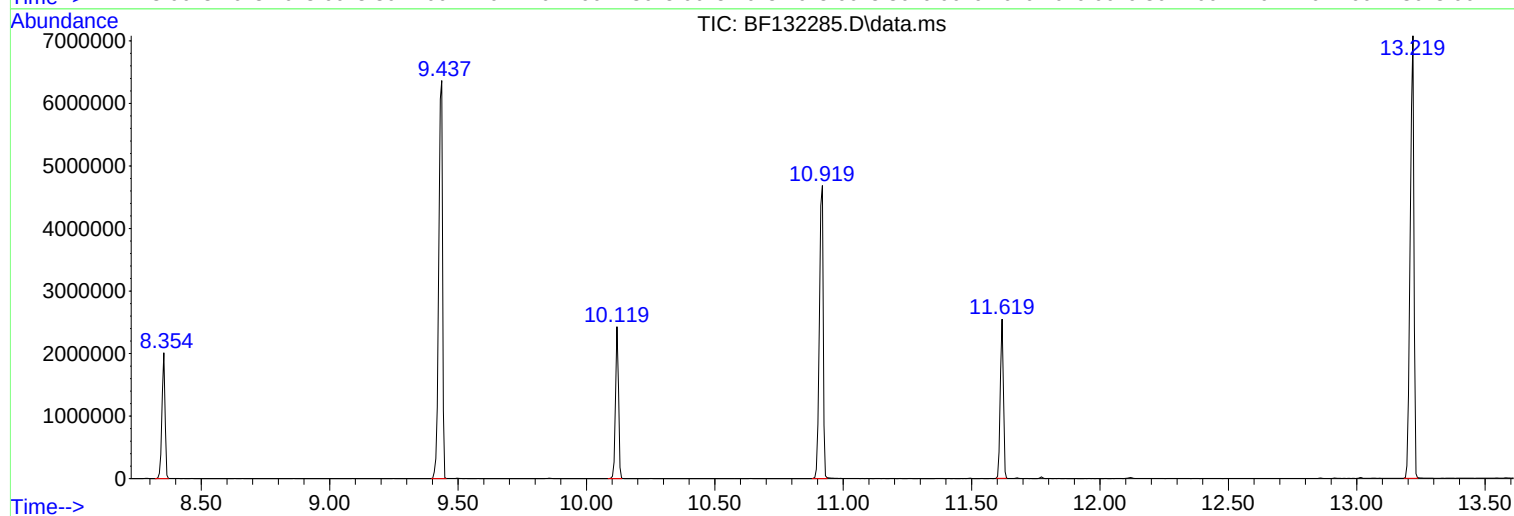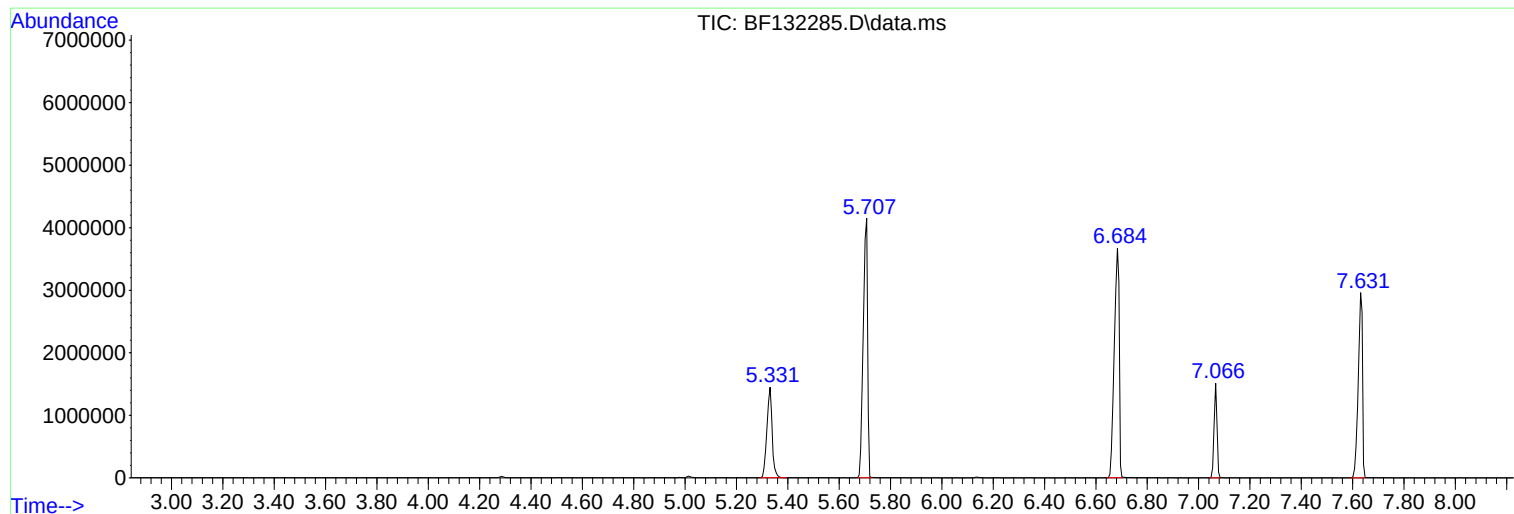

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020223\
Data File : BF132285.D
Acq On : 02 Feb 2023 11:11
Operator : CG\JU
Sample : PB150609BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB150609BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
5.331	33.90 ng	2044800	1,4-Dichlorobenzene-d4	7.066	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2	(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	47
3	Guanidine	59	CH5N3	000113-00-8	43
4	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17
5	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10

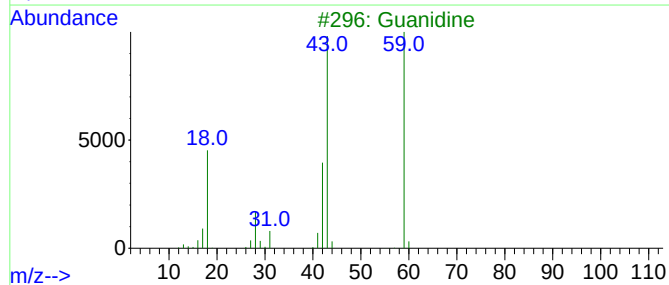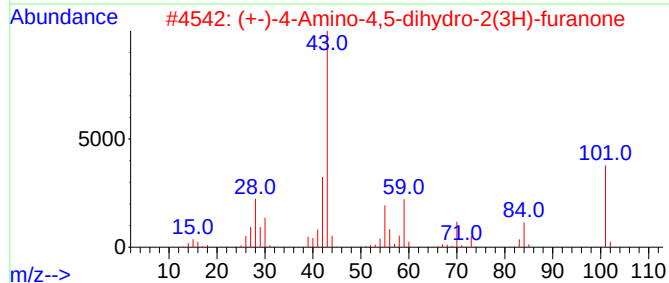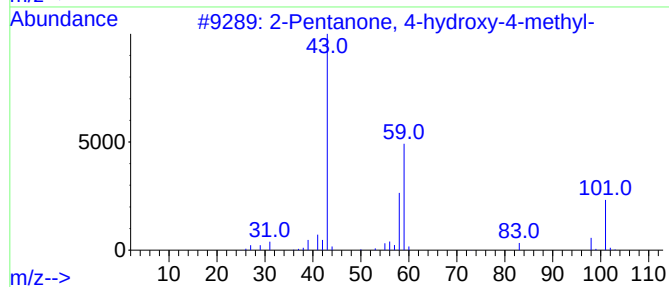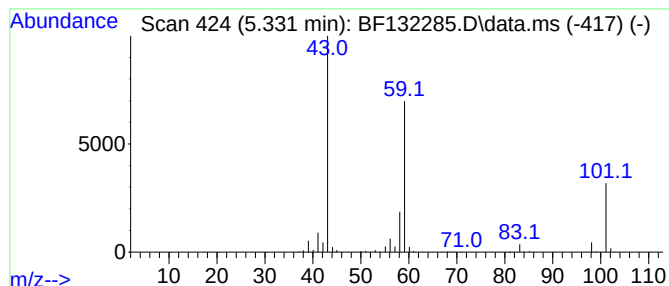

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020223\
Data File : BF132285.D
Acq On : 02 Feb 2023 11:11
Operator : CG\JU
Sample : PB150609BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB150609BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.331	33.9	ng	2044800	1	7.066	1206330	20.0