
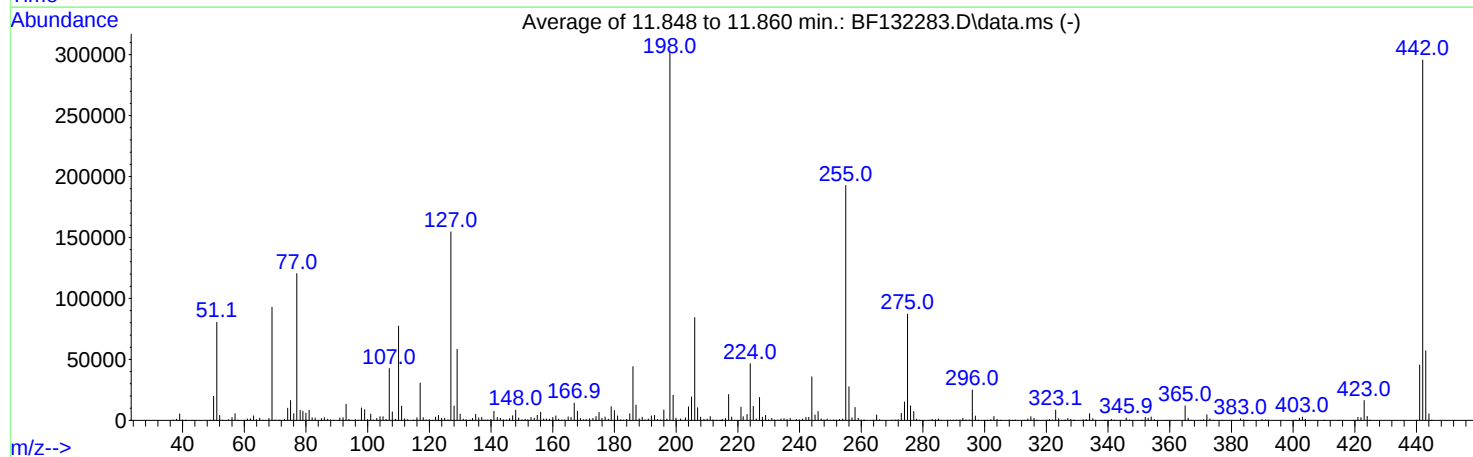


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020223\
 Data File : BF132283.D
 Acq On : 02 Feb 2023 10:07
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Feb 04 01:32:42 2023

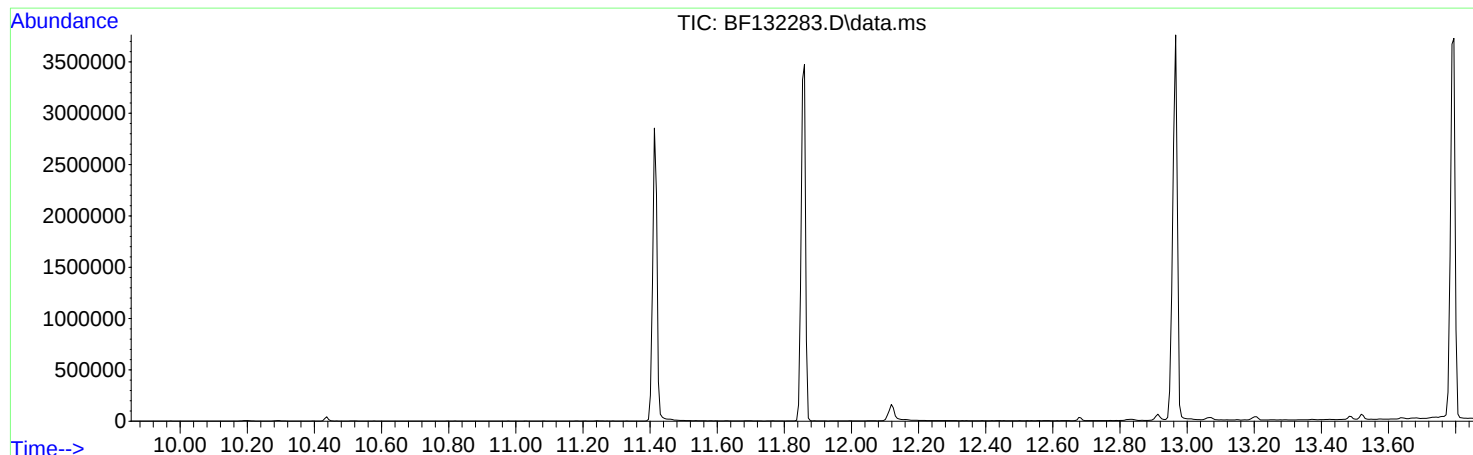




AutoFind: Scans 1532, 1533, 1534; Background Corrected with Scan 1527

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.7	80467	PASS
68	69	0.00	2	1.7	1541	PASS
69	198	0.00	100	30.7	92763	PASS
70	69	0.00	2	0.5	453	PASS
127	198	10	80	51.2	154603	PASS
197	198	0.00	2	0.4	1083	PASS
198	198	100	100	100.0	301717	PASS
199	198	5	9	6.9	20680	PASS
275	198	10	60	28.9	87165	PASS
365	198	1	100	4.0	11980	PASS
441	198	0.01	100	15.0	45398	PASS
442	442	50	100	100.0	295573	PASS
443	442	15	24	19.3	57164	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020223\
Data File : BF132283.D
Acq On : 02 Feb 2023 10:07
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 03 03:17:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 02 01:30:34 2023
Response via : Initial Calibration

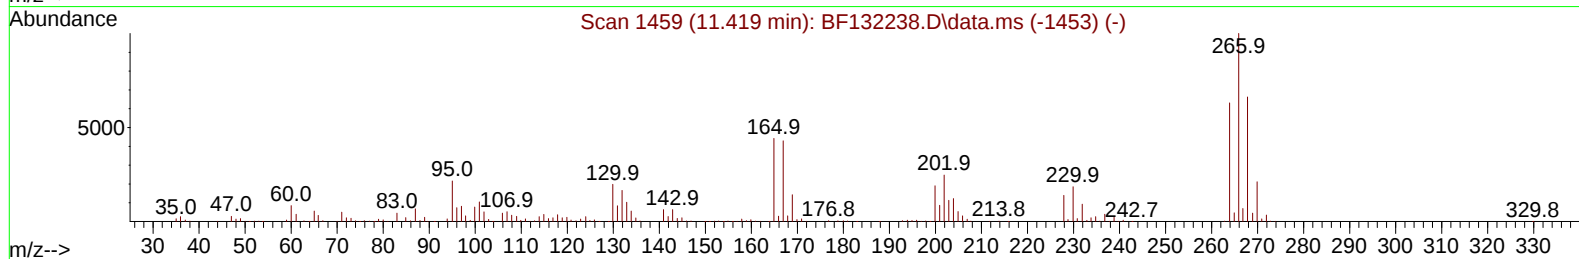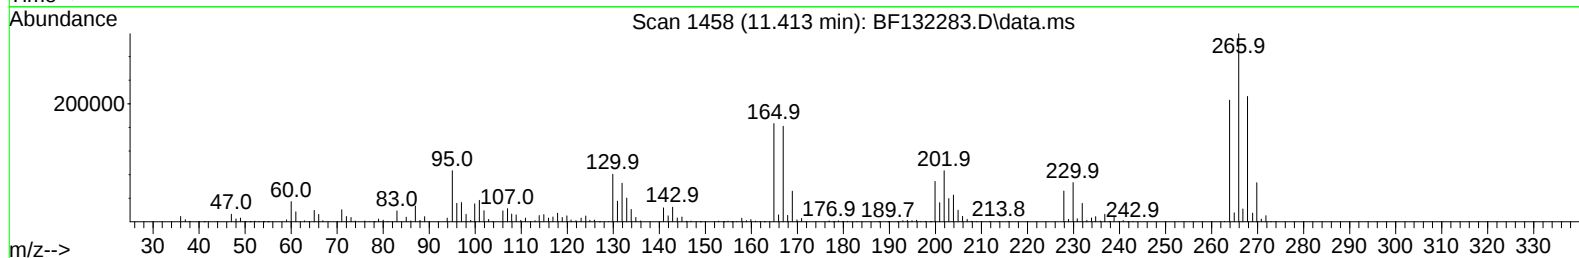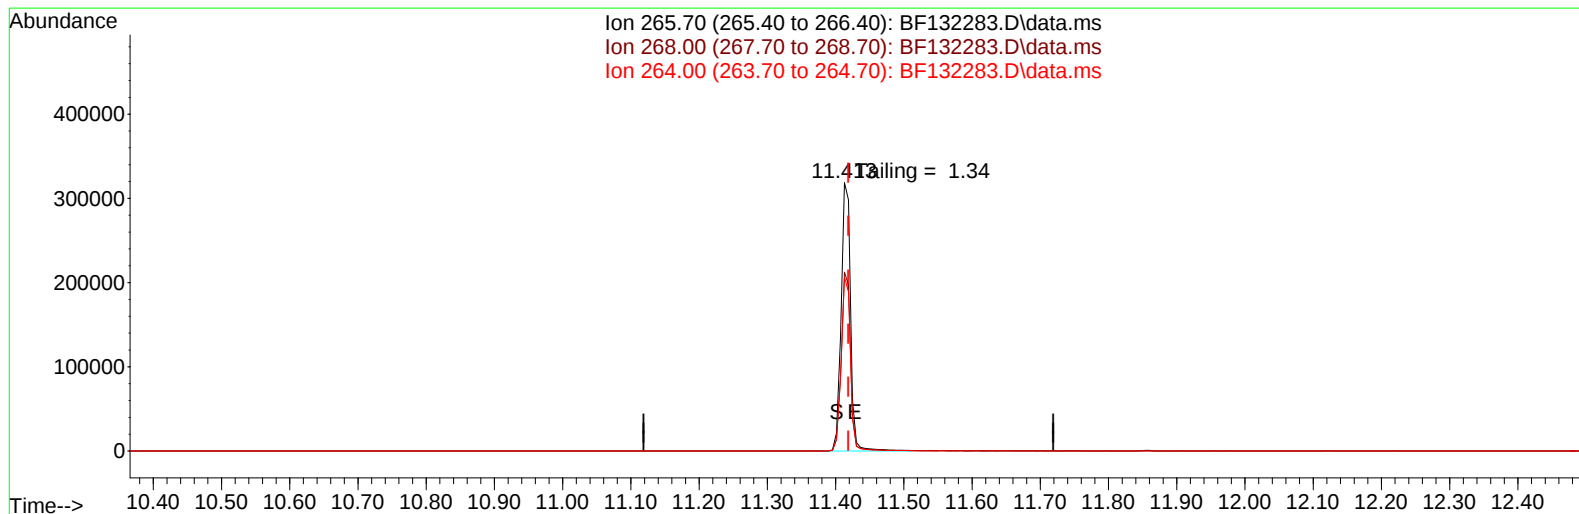

TIC: BF132283.D\data.ms

(70) Pentachlorophenol (C)

11.413min (-0.006) 163031.61 ng


response 305277

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	66.67
264.00	63.10	64.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020223\
Data File : BF132283.D
Acq On : 02 Feb 2023 10:07
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 03 03:17:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 02 01:30:34 2023
Response via : Initial Calibration

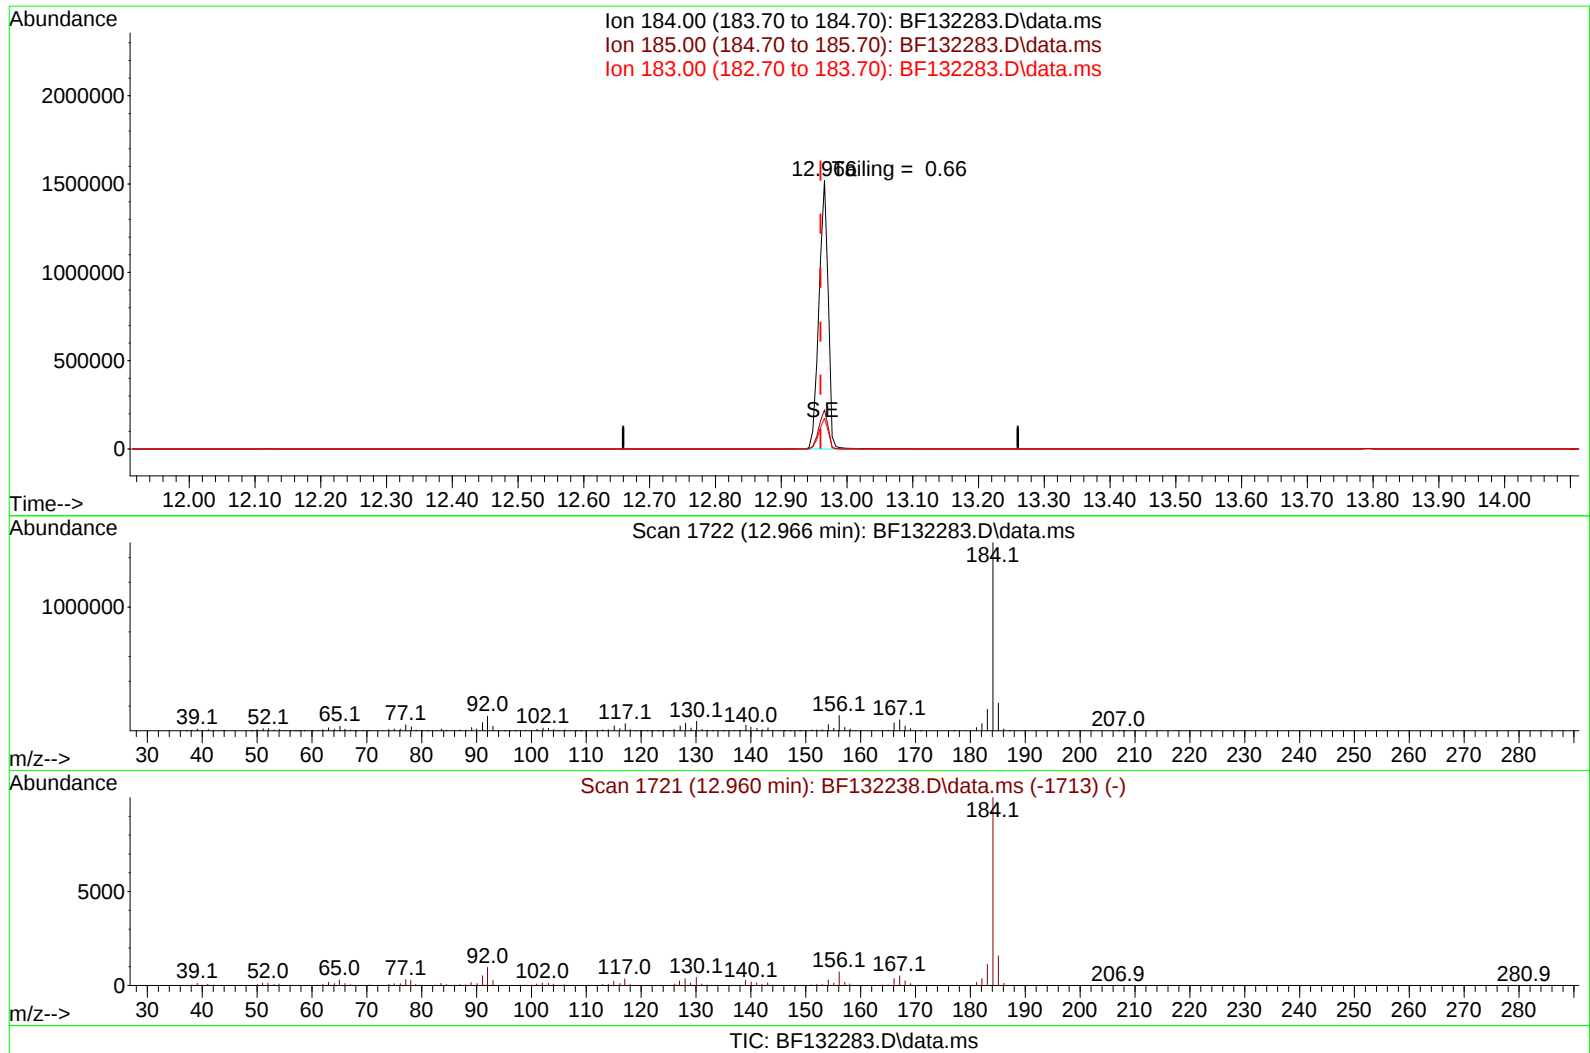

(77) Benzidine

12.966min (+ 0.006) 23205.74 ng

response 1484676

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.65
183.00	11.10	11.44
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/2/2023	BNA_F	<u>BF132283.D</u>
Compound Name	Response	Retention Time
DDT	696819	13.795
DDD	12806	13.519
DDE	565	13.148
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13371	710190	1.88

Instrument :
BNA_F
ClientSampleId :
DFTPP