
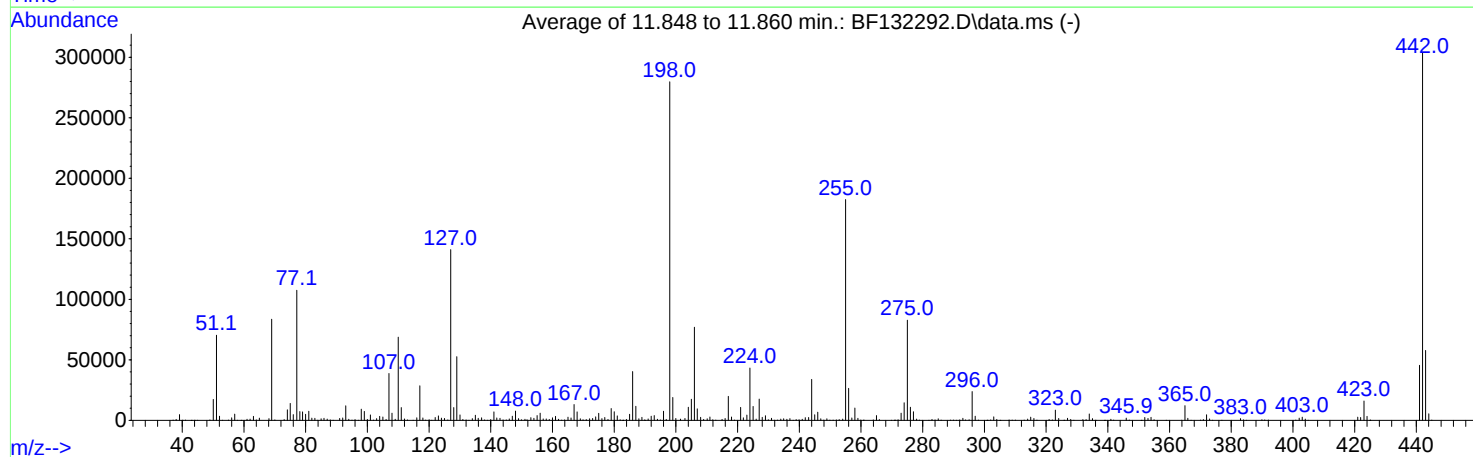


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020223\
 Data File : BF132292.D
 Acq On : 02 Feb 2023 15:08
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Feb 04 01:32:42 2023

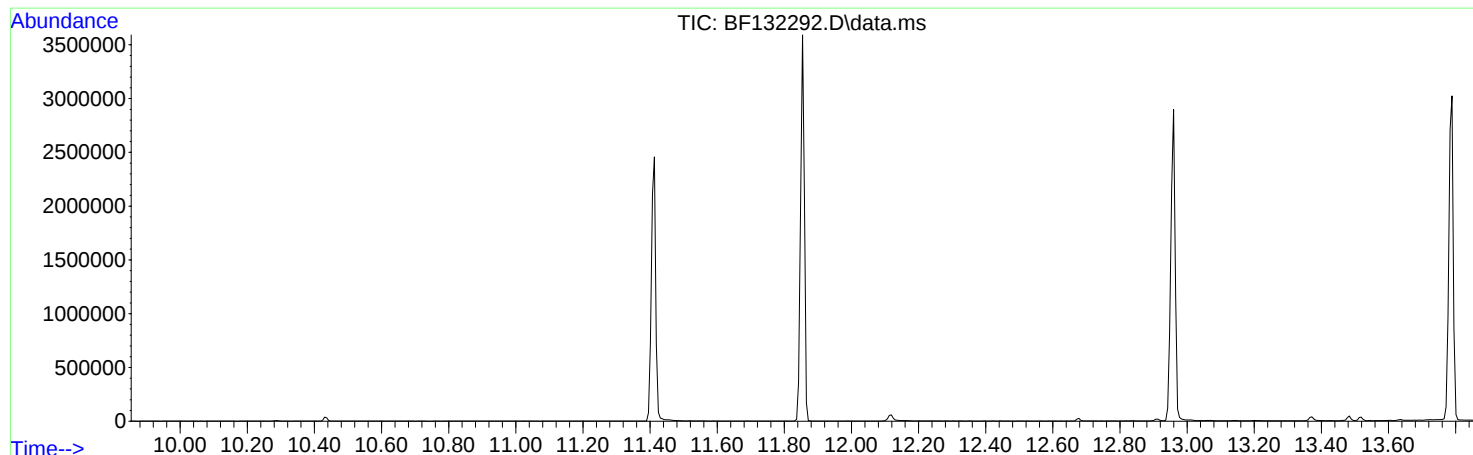




AutoFind: Scans 1532, 1533, 1534; Background Corrected with Scan 1527

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.1	70325	PASS
68	69	0.00	2	1.7	1428	PASS
69	198	0.00	100	29.9	83611	PASS
70	69	0.00	2	0.5	434	PASS
127	198	10	80	50.4	141037	PASS
197	198	0.00	2	0.3	839	PASS
198	198	100	100	100.0	279680	PASS
199	198	5	9	6.8	18889	PASS
275	198	10	60	29.6	82712	PASS
365	198	1	100	4.4	12169	PASS
441	198	0.01	100	16.3	45544	PASS
442	442	50	100	100.0	303944	PASS
443	442	15	24	19.0	57749	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020223\
 Data File : BF132292.D
 Acq On : 02 Feb 2023 15:08
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 03 04:15:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 02 01:30:34 2023
 Response via : Initial Calibration

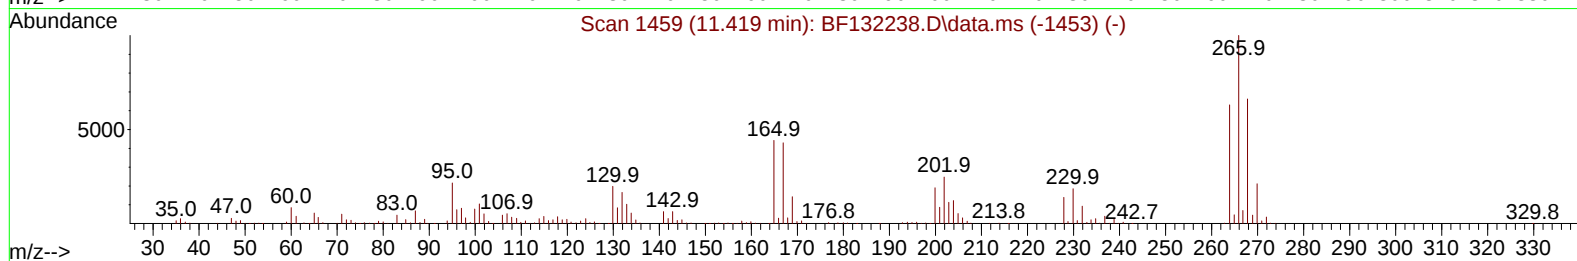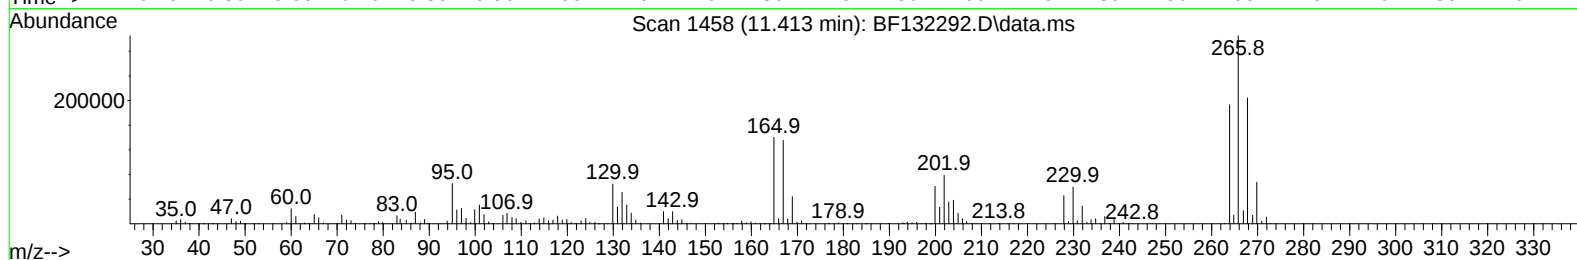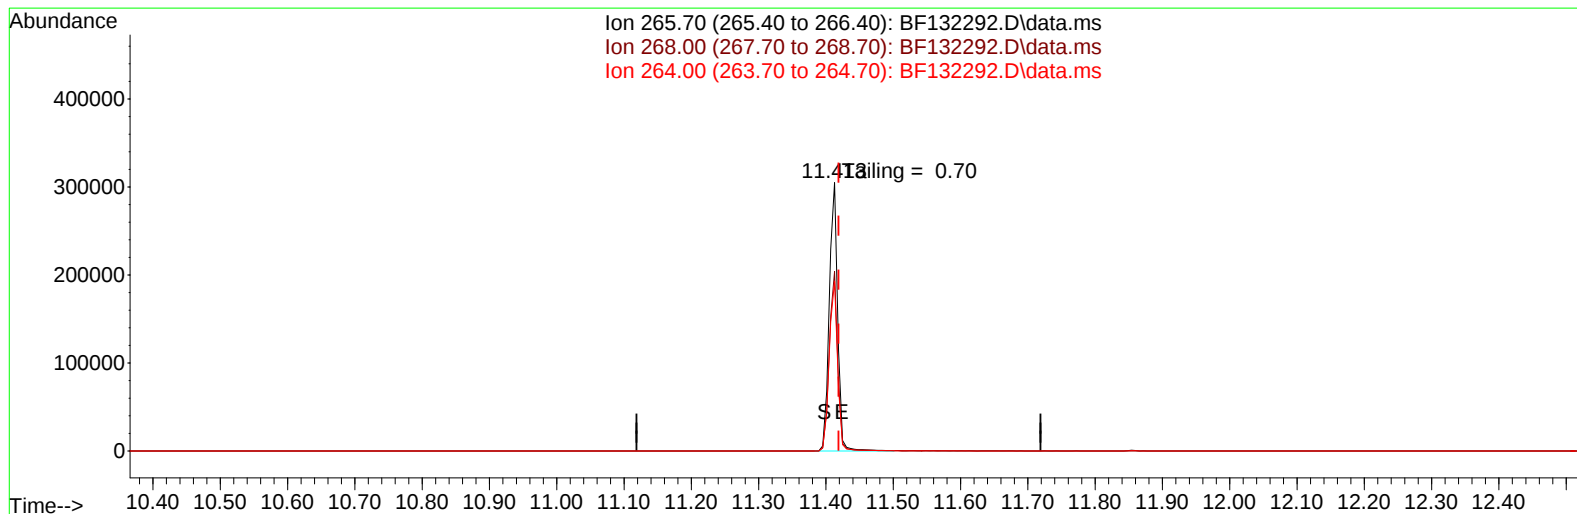

TIC: BF132292.D\data.ms

(70) Pentachlorophenol (C)

11.413min (-0.006) 219843.48 ng




response 266172

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	66.91
264.00	63.10	63.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020223\
Data File : BF132292.D
Acq On : 02 Feb 2023 15:08
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 03 04:15:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 02 01:30:34 2023
Response via : Initial Calibration

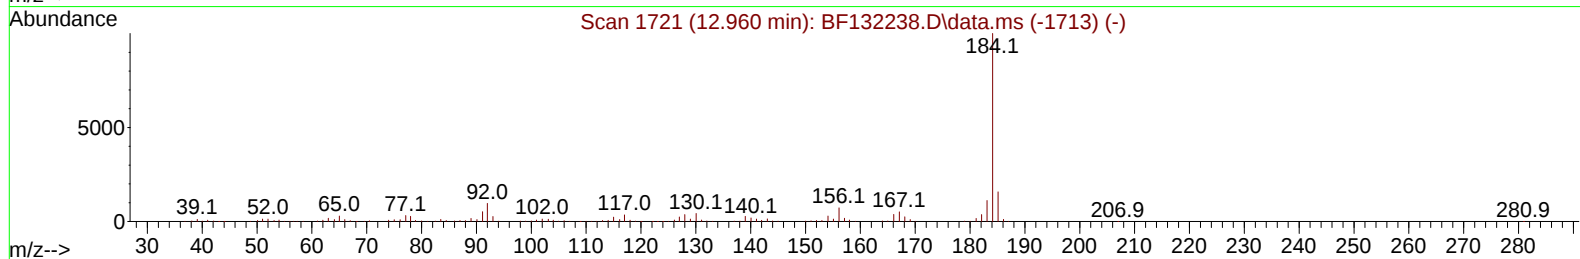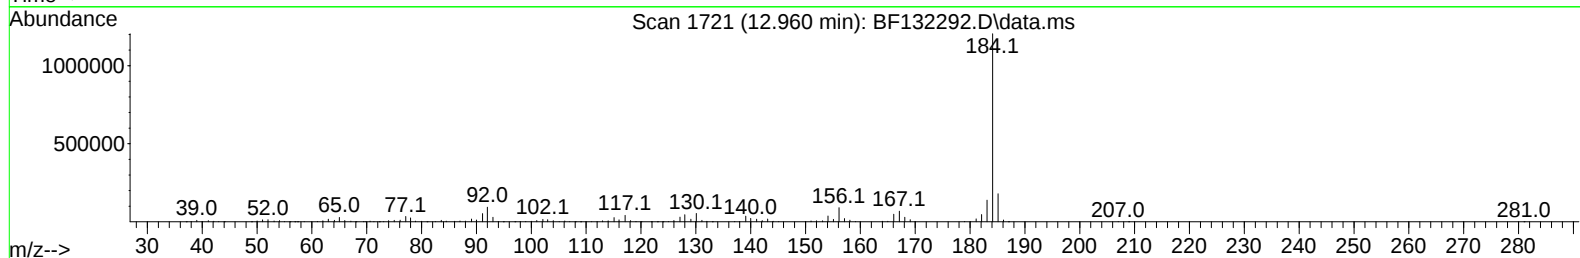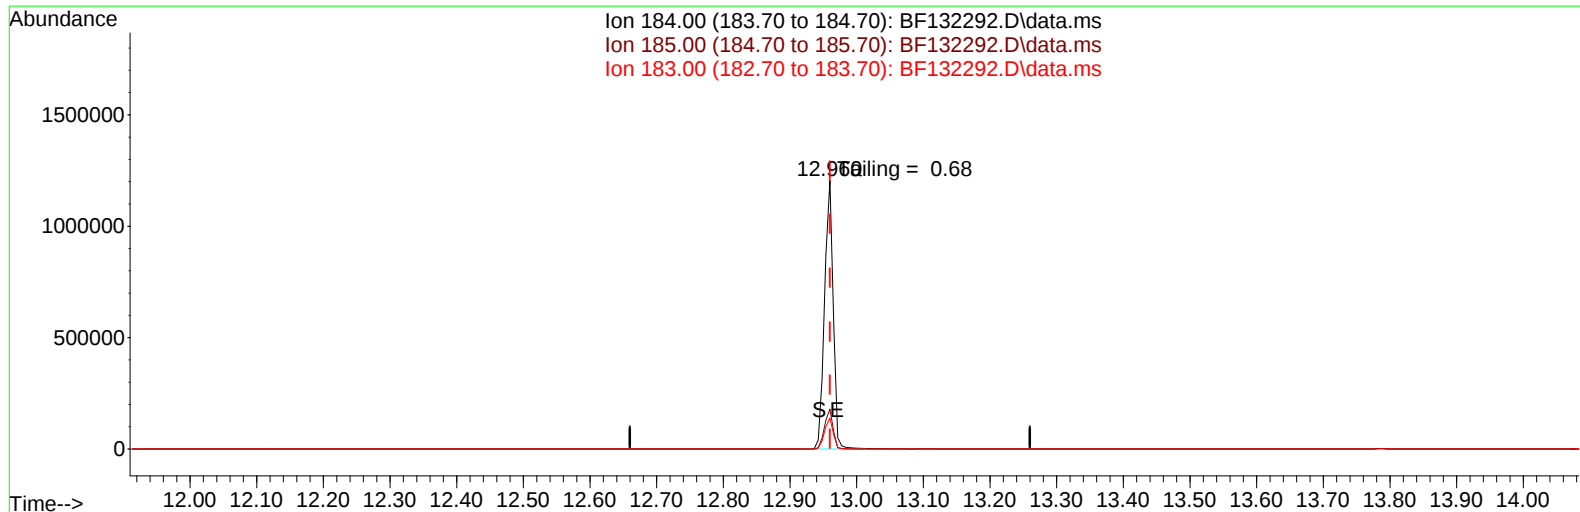

TIC: BF132292.D\data.ms

(77) Benzidine

12.960min (-0.000) 223462.34 ng

response 1085936

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.92
183.00	11.10	11.51
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/2/2023	BNA_F	<u>BF132292.D</u>
Compound Name	Response	Retention Time
DDT	538726	13.789
DDD	12733	13.483
DDE	521	13.142
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13254	551980	2.40

Instrument :
BNA_F
ClientSampleId :
DFTPP