
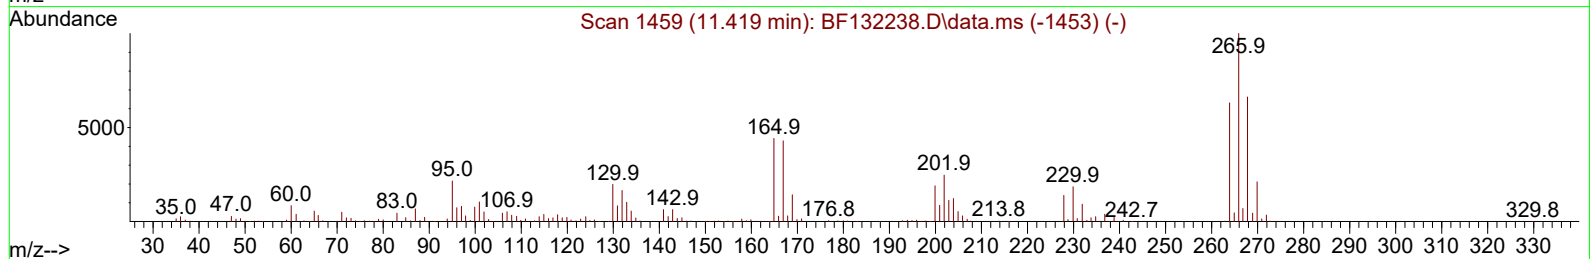
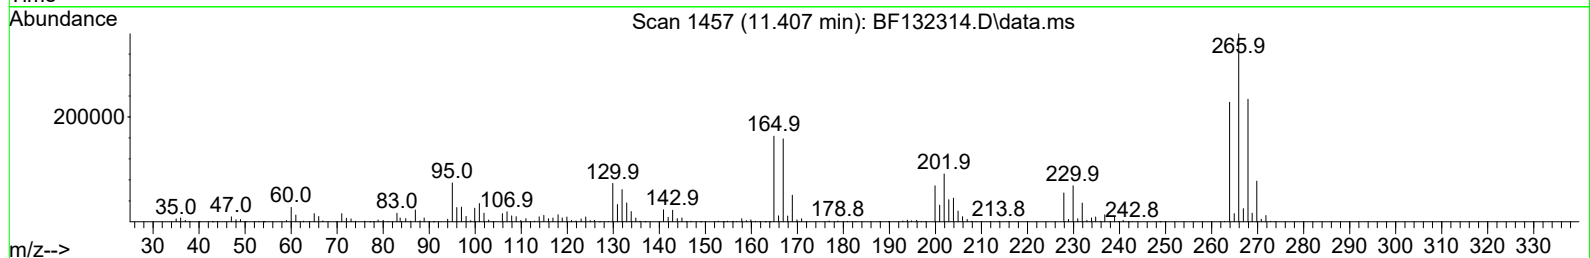


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020323\
Data File : BF132314.D
Acq On : 03 Feb 2023 10:12
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 03:59:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 04 01:32:42 2023
Response via : Initial Calibration

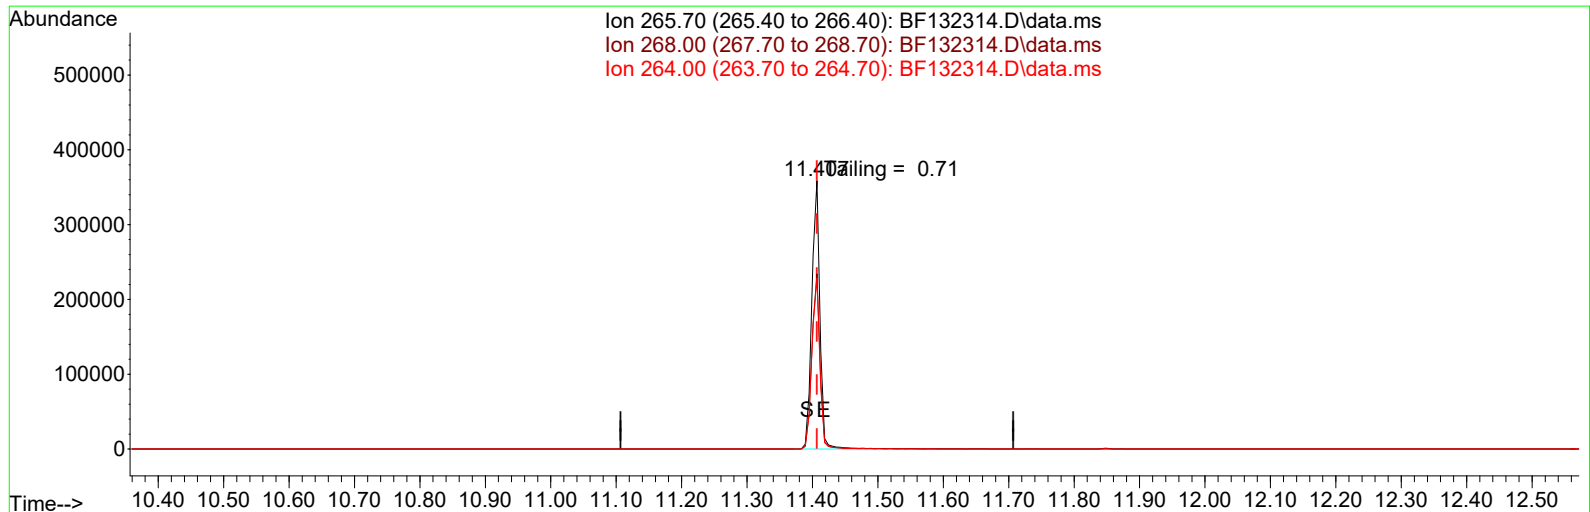

TIC: BF132314.D\data.ms

(70) Pentachlorophenol (C)




11.407min (-0.000) 745859.28 ng

response 308491

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	65.20
264.00	63.10	63.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020323\
 Data File : BF132314.D
 Acq On : 03 Feb 2023 10:12
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 03:59:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 04 01:32:42 2023
 Response via : Initial Calibration

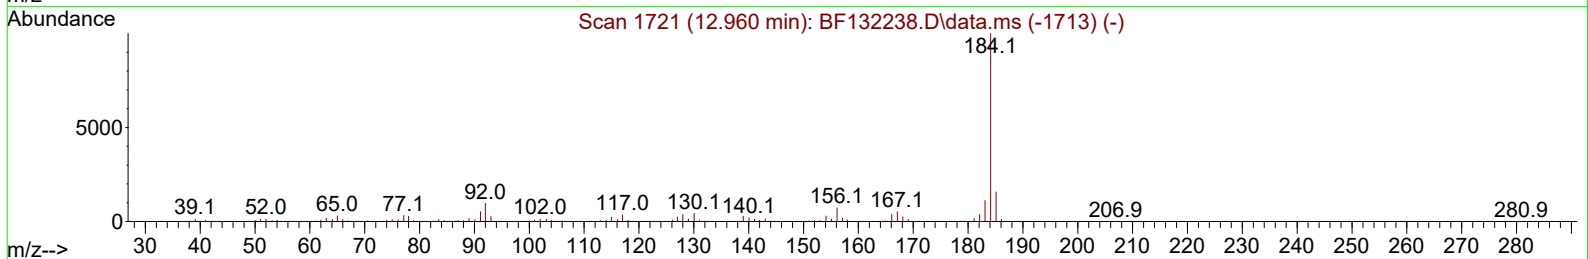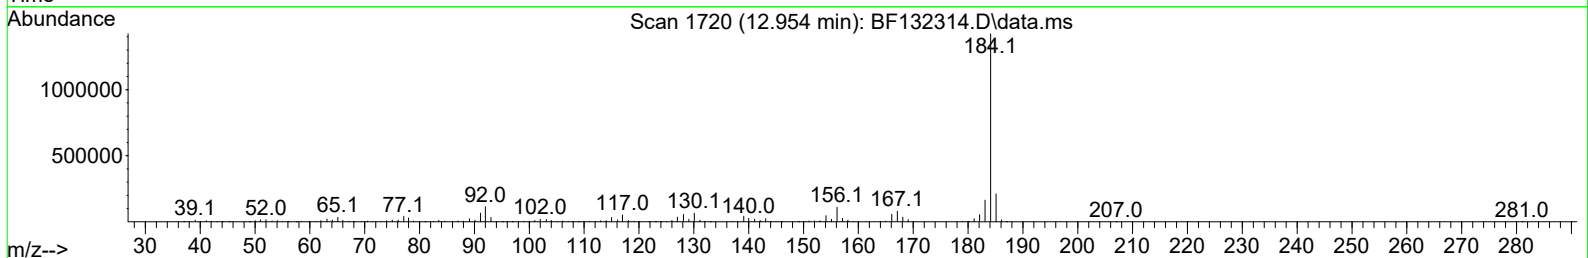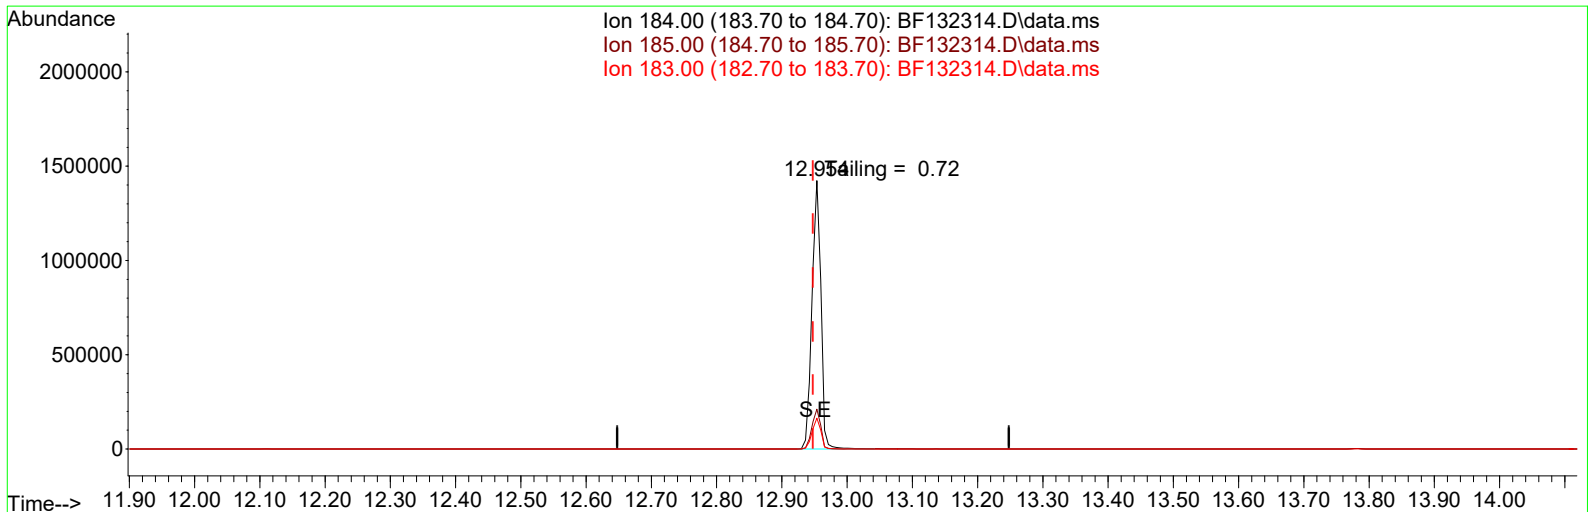

TIC: BF132314.D\data.ms

(77) Benzidine

12.954min (+ 0.006) 77737.14 ng

response 1369759

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.85
183.00	11.10	11.51
0.00	0.00	0.00