

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020323\
 Data File : BF132325.D
 Acq On : 03 Feb 2023 16:59
 Operator : CG\JU
 Sample : 01371-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 4-RAMP-E

Quant Time: Feb 04 01:39:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 04 01:32:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.054	152	230702	20.000	ng	0.00
21) Naphthalene-d8	8.342	136	886983	20.000	ng	0.00
39) Acenaphthene-d10	10.107	164	460643	20.000	ng	0.00
64) Phenanthrene-d10	11.607	188	812117	20.000	ng	0.00
76) Chrysene-d12	14.265	240	454162	20.000	ng	0.00
86) Perylene-d12	15.848	264	356902	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.690	112	1428472	99.528	ng	0.01
7) Phenol-d6	6.678	99	1743646	98.541	ng	0.00
23) Nitrobenzene-d5	7.625	82	1086857	68.187	ng	0.00
42) 2,4,6-Tribromophenol	10.907	330	567099	119.715	ng	0.00
45) 2-Fluorobiphenyl	9.425	172	1893592	63.480	ng	0.00
79) Terphenyl-d14	13.201	244	1922070	81.867	ng	0.00
Target Compounds						
84) Bis(2-ethylhexyl)phtha...	14.224	149	54663	2.506	ng	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020323\
Data File : BF132325.D
Acq On : 03 Feb 2023 16:59
Operator : CG\JU
Sample : 01371-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
4-RAMP-E

Quant Time: Feb 04 01:39:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 04 01:32:42 2023
Response via : Initial Calibration




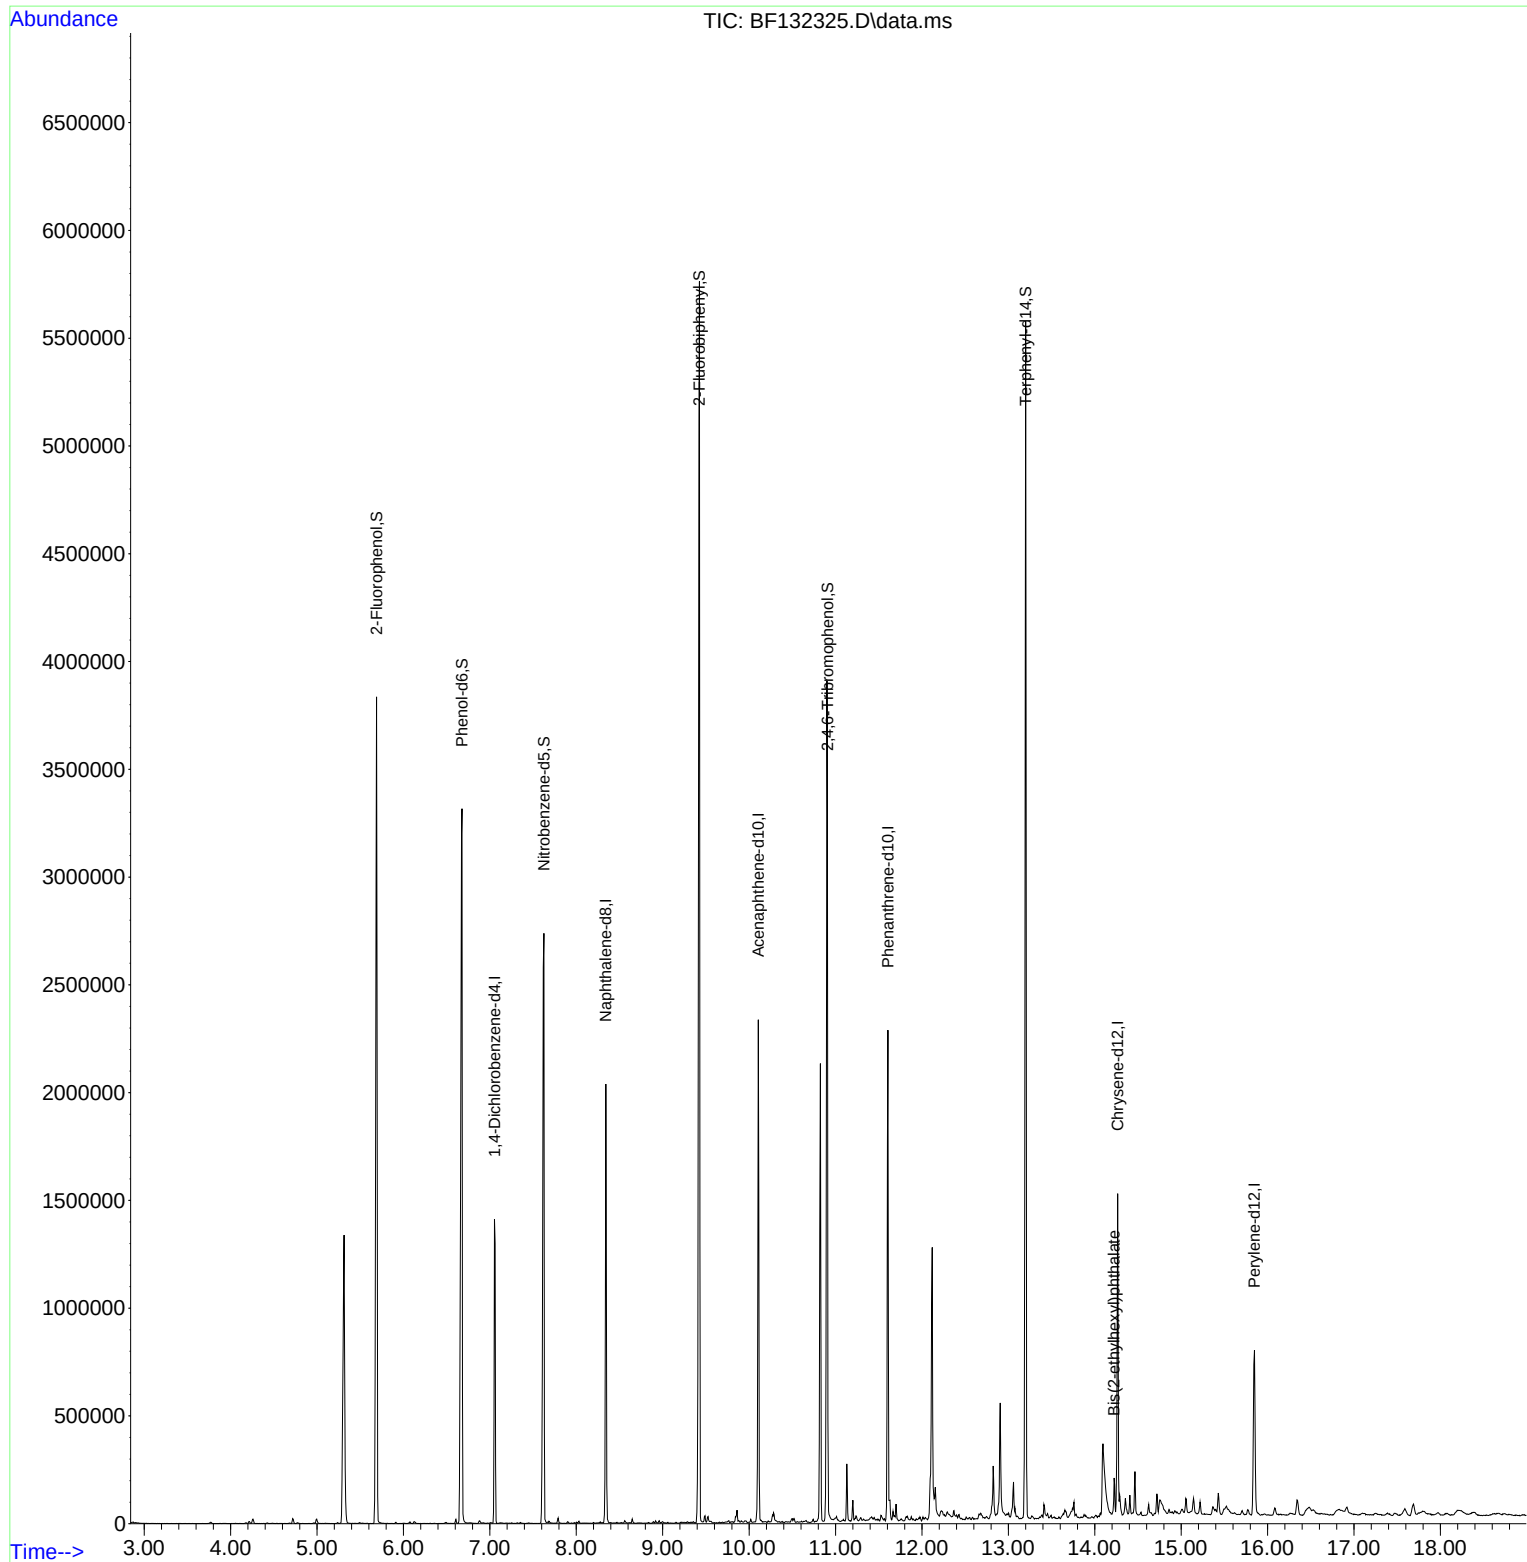


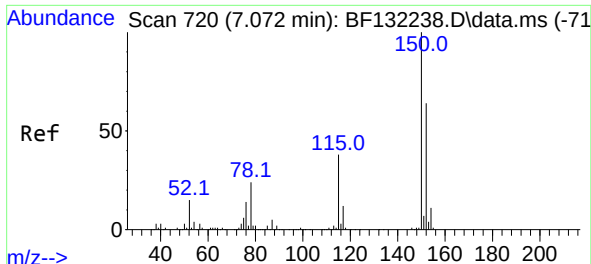

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.054 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF132325.D
Acq: 03 Feb 2023 16:59




Instrument :
BNA_F
ClientSampleId :
4-RAMP-E


Tgt Ion:152 Resp: 230702
Ion Ratio Lower Upper
152 100
150 155.2 124.2 186.2
115 62.5 47.3 70.9

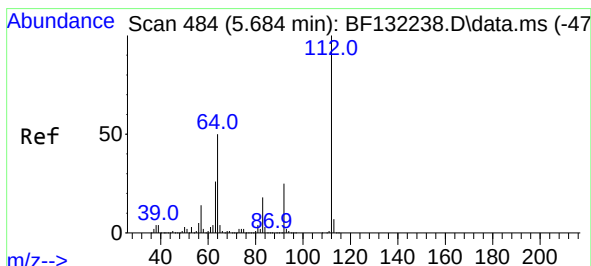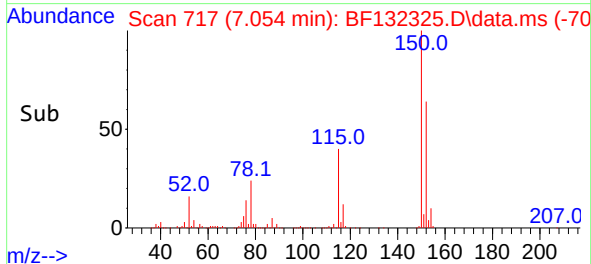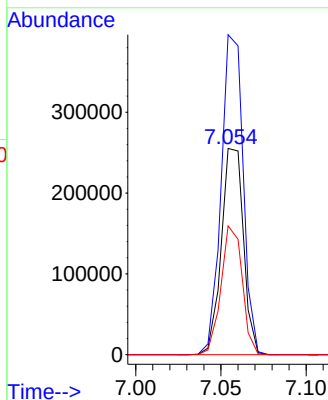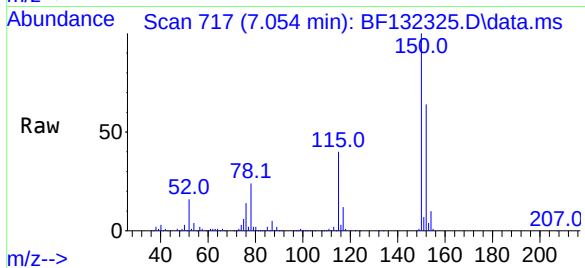

#5
2-Fluorophenol
Concen: 99.528 ng
RT: 5.690 min Scan# 485
Delta R.T. 0.012 min
Lab File: BF132325.D
Acq: 03 Feb 2023 16:59

Tgt Ion:112 Resp: 1428472
Ion Ratio Lower Upper
112 100
64 45.0 40.0 60.0
63 24.3 20.5 30.7


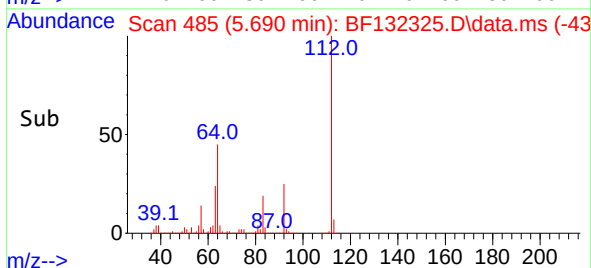
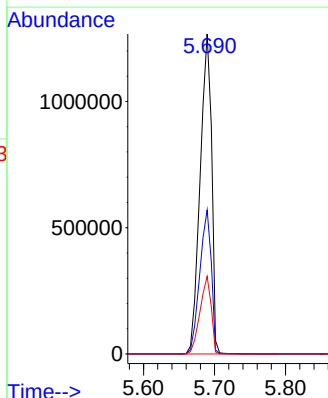
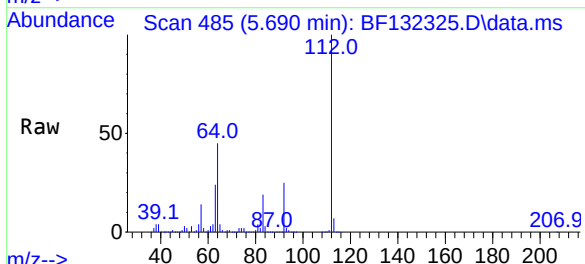


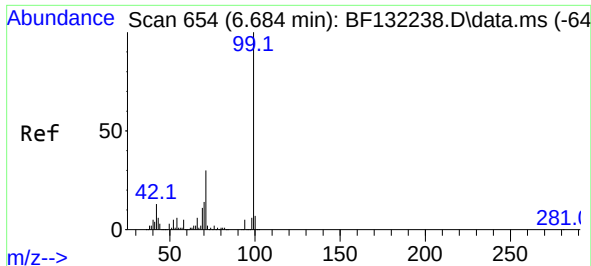

#7
Phenol-d6
Concen: 98.541 ng
RT: 6.678 min Scan# 61
Delta R.T. -0.000 min
Lab File: BF132325.D
Acq: 03 Feb 2023 16:59




Instrument :
BNA_F
ClientSampleId :
4-RAMP-E


Tgt Ion: 99 Resp: 1743646
Ion Ratio Lower Upper
99 100
42 11.6 10.1 15.1
71 31.6 24.2 36.4

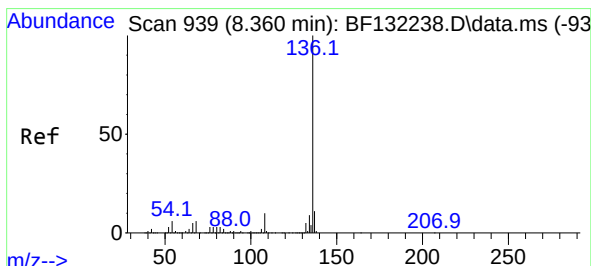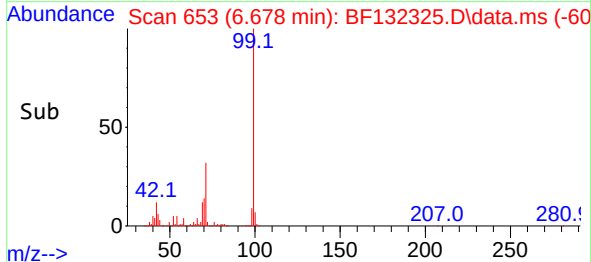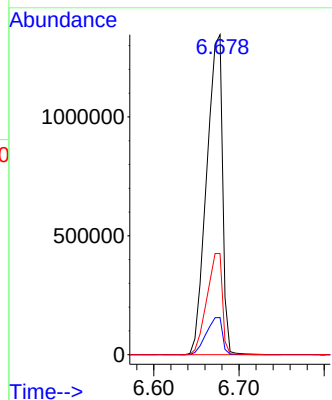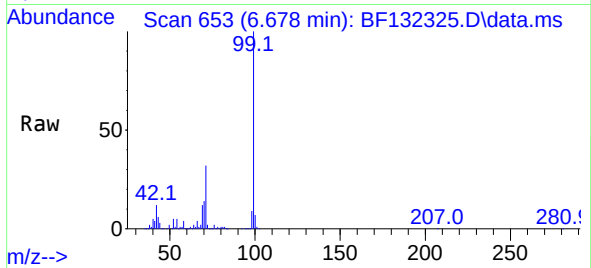

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.342 min Scan# 936
Delta R.T. -0.006 min
Lab File: BF132325.D
Acq: 03 Feb 2023 16:59

Tgt Ion:136 Resp: 886983
Ion Ratio Lower Upper
136 100
137 11.4 8.8 13.2
54 5.7 4.9 7.3
68 5.3 4.7 7.1


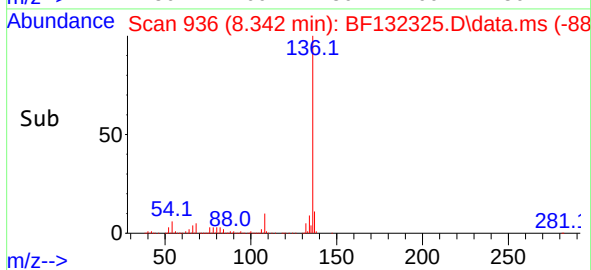
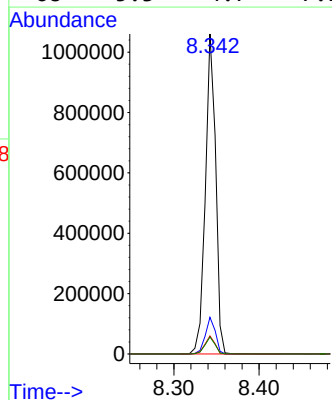
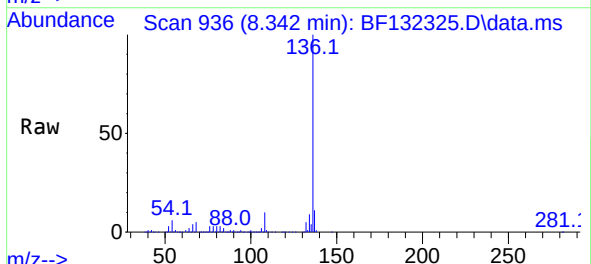


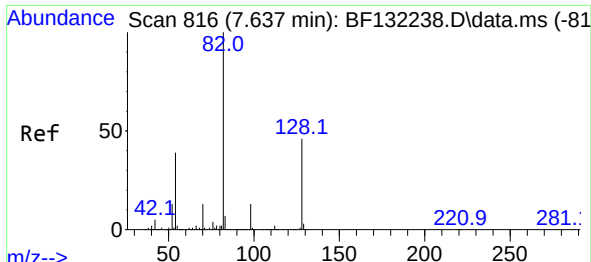

#23
Nitrobenzene-d5
Concen: 68.187 ng
RT: 7.625 min Scan# 81
Delta R.T. -0.006 min
Lab File: BF132325.D
Acq: 03 Feb 2023 16:59




Instrument :
BNA_F
ClientSampleId :
4-RAMP-E


Tgt Ion: 82 Resp: 1086857
Ion Ratio Lower Upper
82 100
128 51.2 37.0 55.4
54 37.1 31.5 47.3

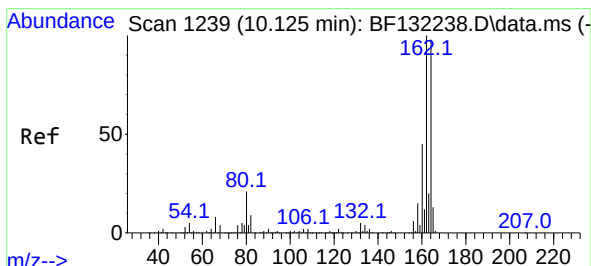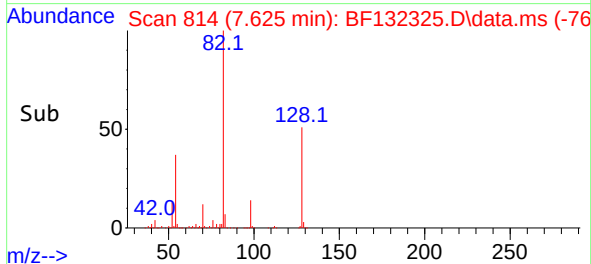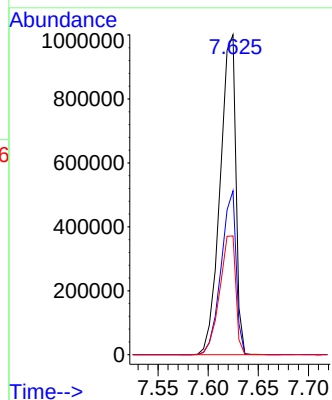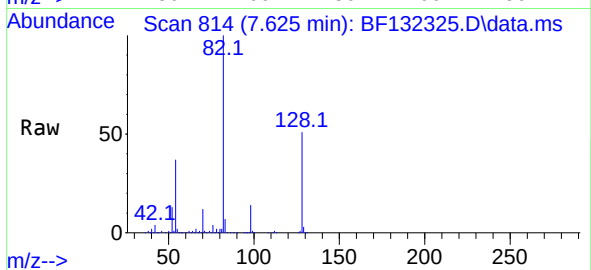

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.107 min Scan# 1236
Delta R.T. -0.006 min
Lab File: BF132325.D
Acq: 03 Feb 2023 16:59


Tgt Ion:164 Resp: 460643
Ion Ratio Lower Upper
164 100
162 103.1 82.0 123.0
160 46.5 37.1 55.7

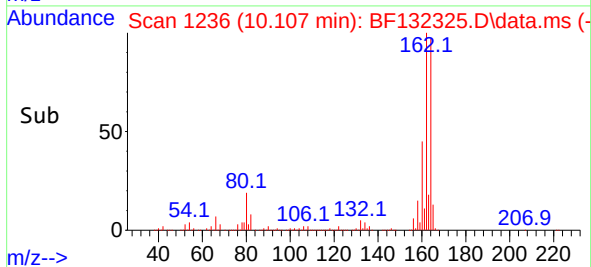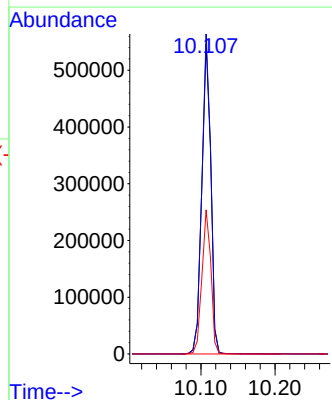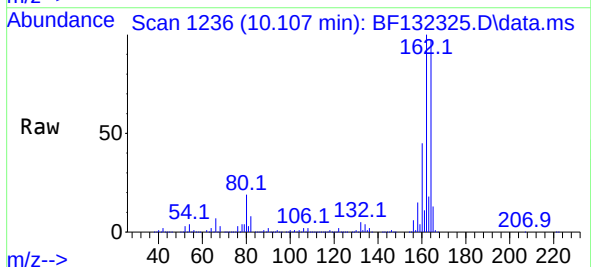



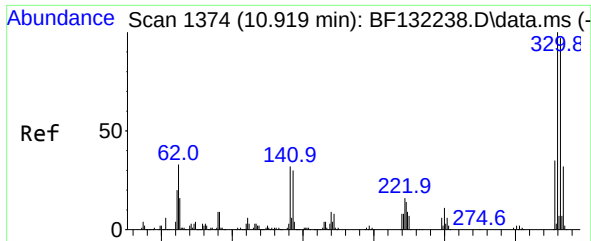


#42
2,4,6-Tribromophenol
Concen: 119.715 ng
RT: 10.907 min Scan# 11
Delta R.T. -0.000 min
Lab File: BF132325.D
Acq: 03 Feb 2023 16:59

Instrument :
BNA_F
ClientSampleId :
4-RAMP-E



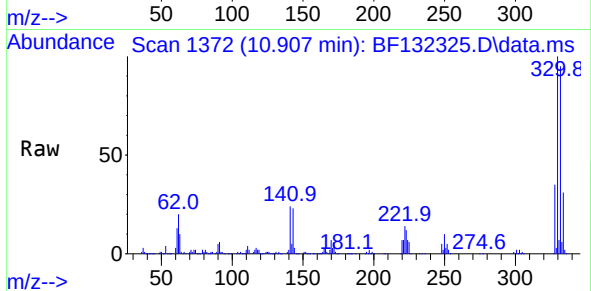



Tgt Ion:330 Resp: 567099
Ion Ratio Lower Upper
330 100
332 95.8 77.9 116.9
141 32.9 31.0 46.4

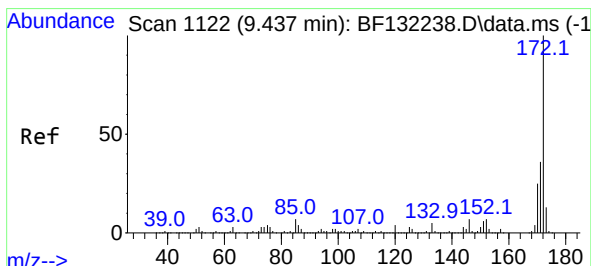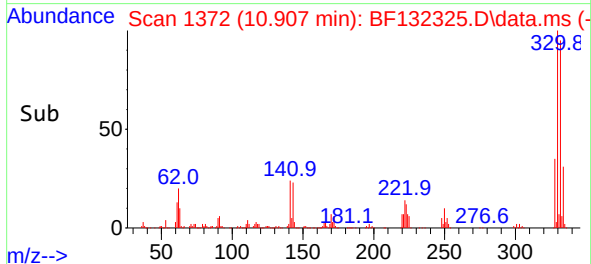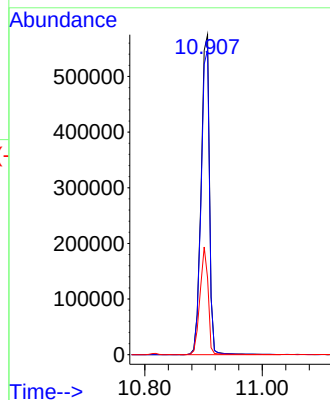

#45
2-Fluorobiphenyl
Concen: 63.480 ng
RT: 9.425 min Scan# 1120
Delta R.T. -0.000 min
Lab File: BF132325.D
Acq: 03 Feb 2023 16:59

Tgt Ion:172 Resp: 1893592
Ion Ratio Lower Upper
172 100
171 36.1 28.6 43.0
170 24.7 19.7 29.5


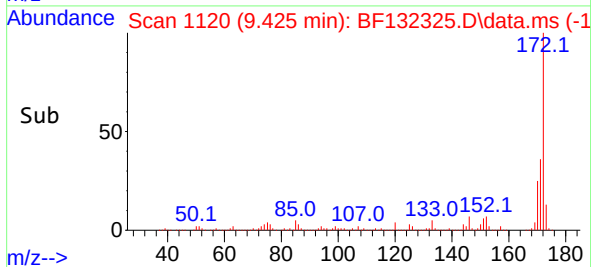
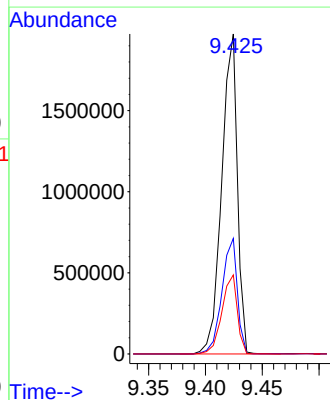
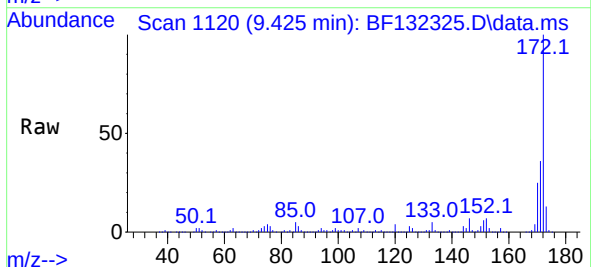


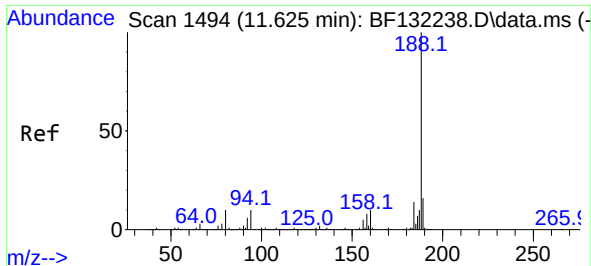

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.607 min Scan# 1494
Delta R.T. -0.006 min
Lab File: BF132325.D
Acq: 03 Feb 2023 16:59




Instrument :
BNA_F
ClientSampleId :
4-RAMP-E


Tgt Ion:188 Resp: 812117
Ion Ratio Lower Upper
188 100
94 9.2 8.2 12.2
80 9.2 8.3 12.5

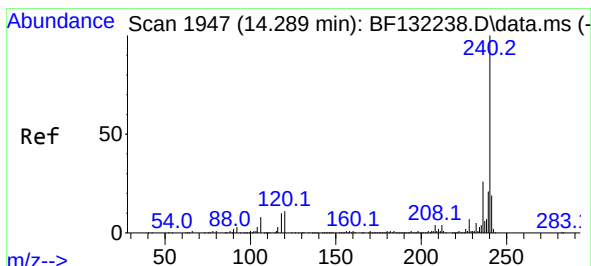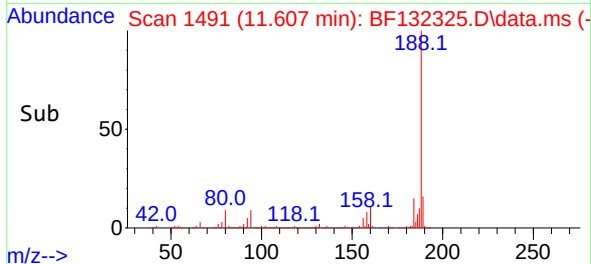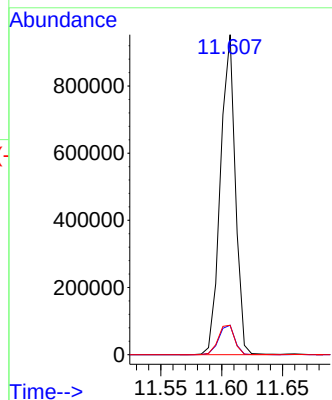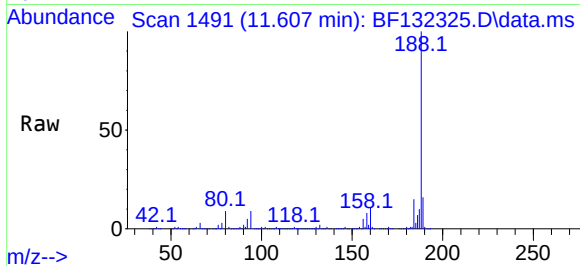

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.265 min Scan# 1943
Delta R.T. -0.006 min
Lab File: BF132325.D
Acq: 03 Feb 2023 16:59

Tgt Ion:240 Resp: 454162
Ion Ratio Lower Upper
240 100
120 12.0 8.8 13.2
236 25.8 21.0 31.6


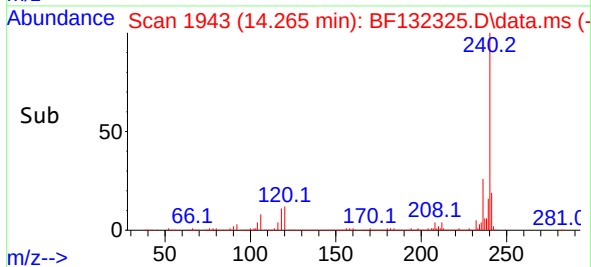
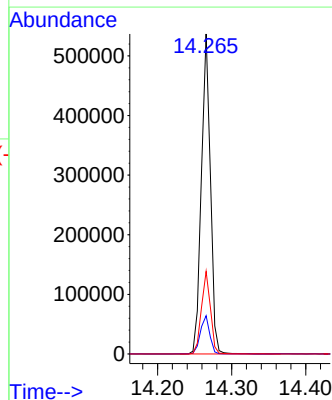
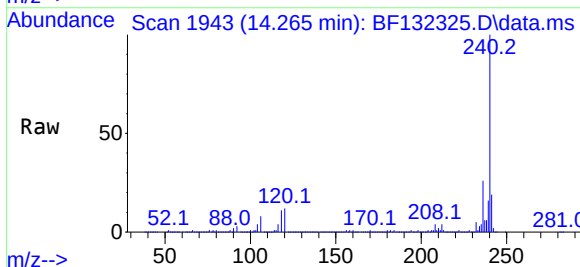


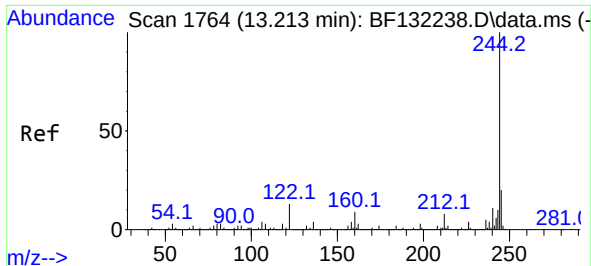

#79
 Terphenyl-d14
 Concen: 81.867 ng
 RT: 13.201 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: BF132325.D
 Acq: 03 Feb 2023 16:59




Instrument :
 BNA_F
 ClientSampleId :
 4-RAMP-E


Tgt Ion:244 Resp: 1922070
 Ion Ratio Lower Upper
 244 100
 212 7.9 6.4 9.6
 122 11.0 10.5 15.7

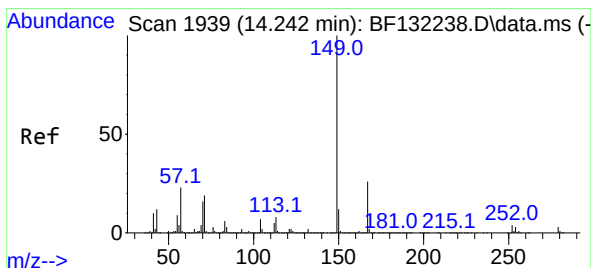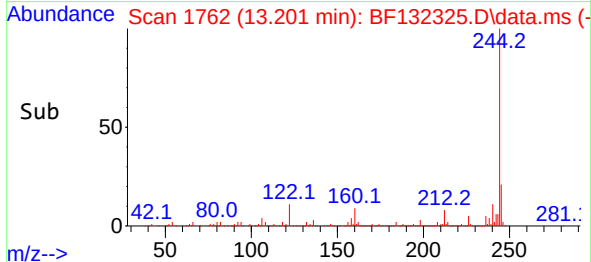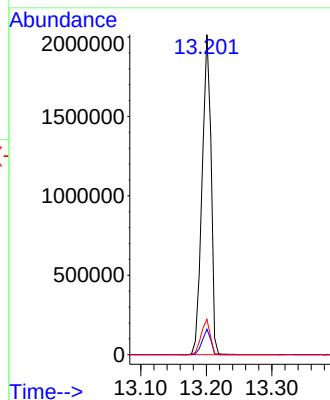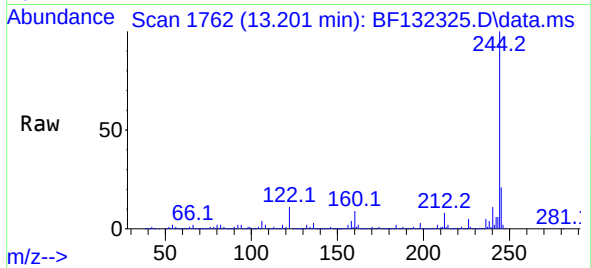

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 2.506 ng
 RT: 14.224 min Scan# 1936
 Delta R.T. -0.006 min
 Lab File: BF132325.D
 Acq: 03 Feb 2023 16:59

Tgt Ion:149 Resp: 54663
 Ion Ratio Lower Upper
 149 100
 167 23.8 20.7 31.1
 279 3.0 2.7 4.1

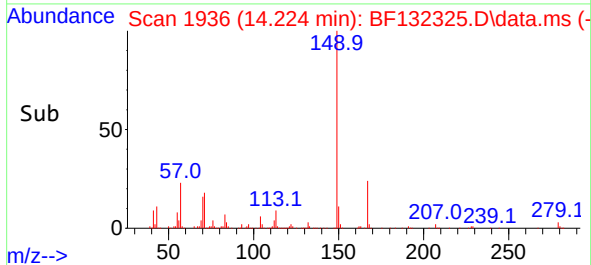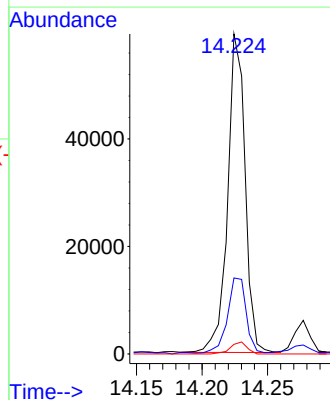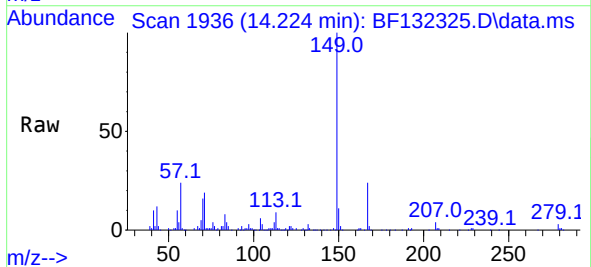

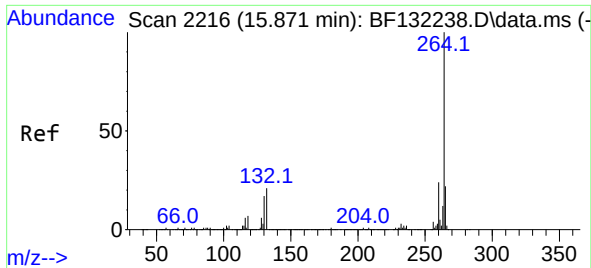

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.848 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BF132325.D
 Acq: 03 Feb 2023 16:59

Instrument :
 BNA_F
 ClientSampleId :
 4-RAMP-E

Tgt Ion:264 Resp: 356902
 Ion Ratio Lower Upper
 264 100
 260 23.6 19.0 28.4
 265 21.2 17.4 26.2

