

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020323\
 Data File : BF132321.D
 Acq On : 03 Feb 2023 14:34
 Operator : CG\JU
 Sample : PB150659BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB150659BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF132321.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.319	415	422	438	rBV	1365348	1957988	29.94%	4.748%
2	5.695	480	486	489	rBV	4108731	4721617	72.20%	11.450%
3	6.678	646	653	656	rBV	3677504	4690659	71.72%	11.375%
4	7.060	714	718	721	rVB	1362871	1237463	18.92%	3.001%
5	7.625	807	814	817	rBV	3134219	3235430	49.47%	7.846%
6	8.342	931	936	940	rBV	2036098	1718414	26.28%	4.167%
7	9.425	1113	1120	1123	rBV	6692252	6256235	95.66%	15.171%
8	10.107	1232	1236	1240	rBV	2218023	2016993	30.84%	4.891%
9	10.907	1367	1372	1375	rBV	4584057	4261041	65.16%	10.333%
10	11.607	1487	1491	1494	rBV	2510484	2096994	32.07%	5.085%
11	13.207	1757	1763	1766	rBV	6338688	6539819	100.00%	15.859%
12	14.265	1939	1943	1947	rBV	1543205	1386465	21.20%	3.362%
13	15.848	2206	2212	2227	rBV2	837701	1117937	17.09%	2.711%


Sum of corrected areas: 41237055

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020323\
Data File : BF132321.D
Acq On : 03 Feb 2023 14:34
Operator : CG\JU
Sample : PB150659BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB150659BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

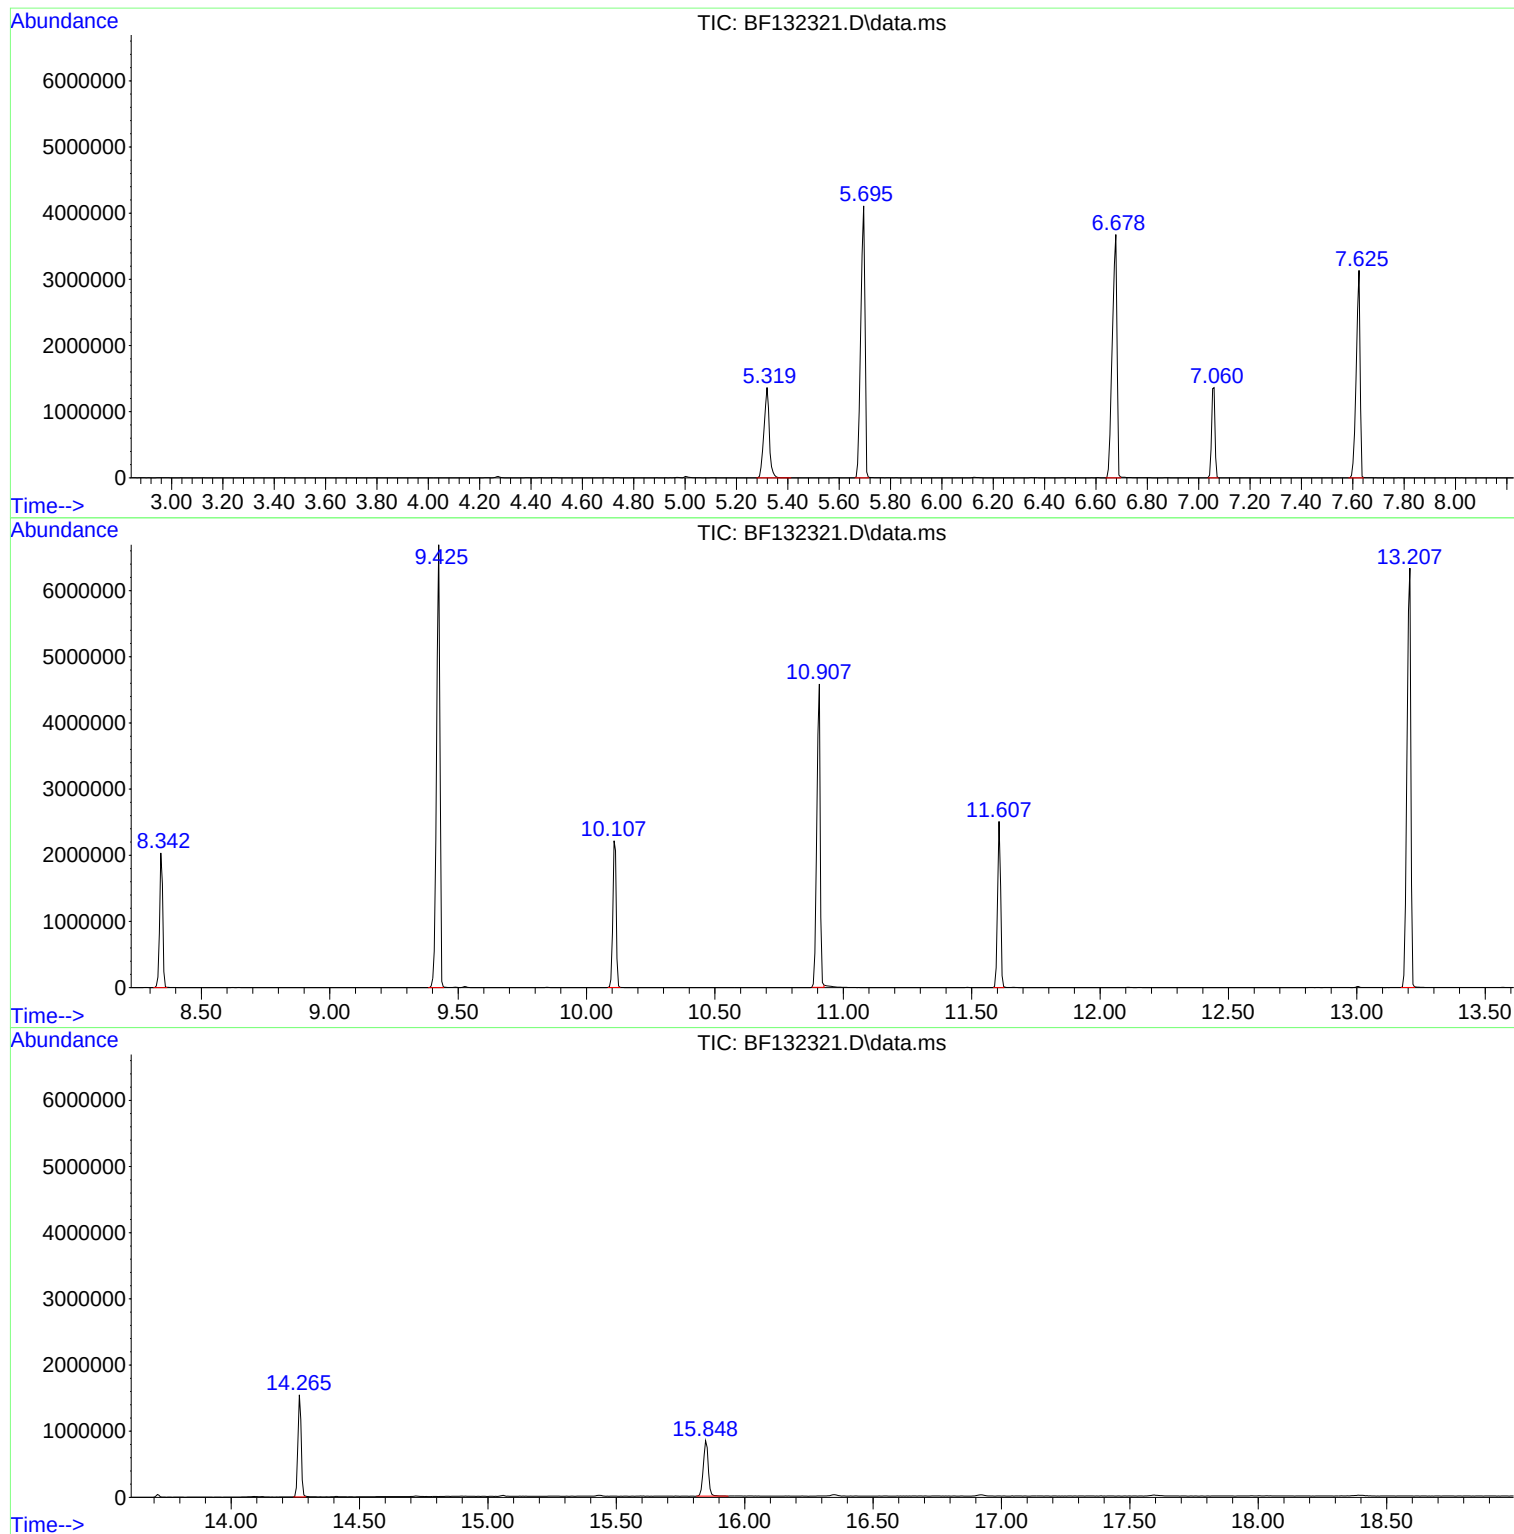

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020323\
Data File : BF132321.D
Acq On : 03 Feb 2023 14:34
Operator : CG\JU
Sample : PB150659BL
Misc :
ALS Vial : 8 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB150659BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
5.319	31.65 ng	1957990	1,4-Dichlorobenzene-d4	7.060	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2	(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	47
3	Guanidine	59	CH5N3	000113-00-8	43
4	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17
5	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10

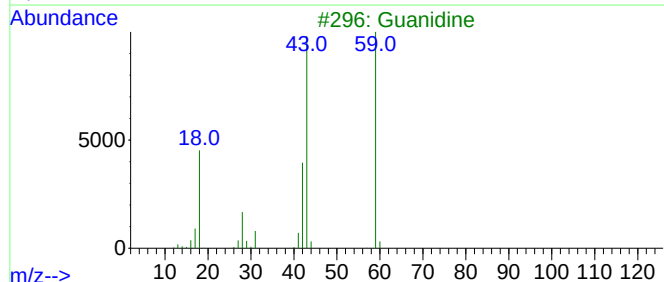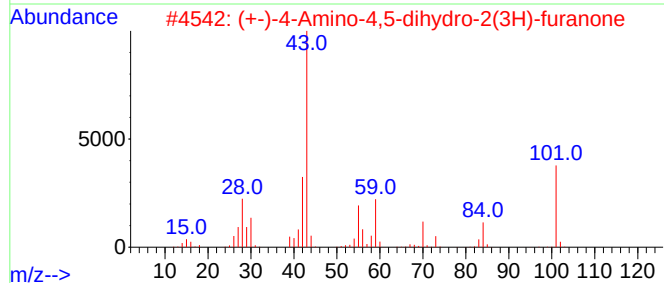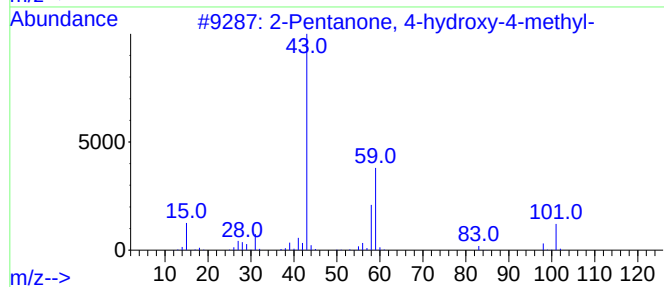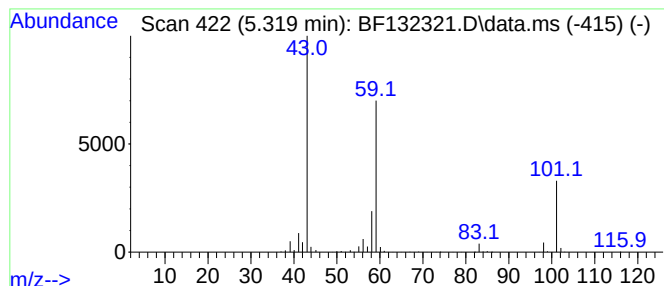

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020323\
Data File : BF132321.D
Acq On : 03 Feb 2023 14:34
Operator : CG\JU
Sample : PB150659BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB150659BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.319	31.6	ng	1957990	1	7.060	1237460	20.0