


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020323\
 Data File : BF132314.D
 Acq On : 03 Feb 2023 10:12
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Feb 04 01:32:42 2023

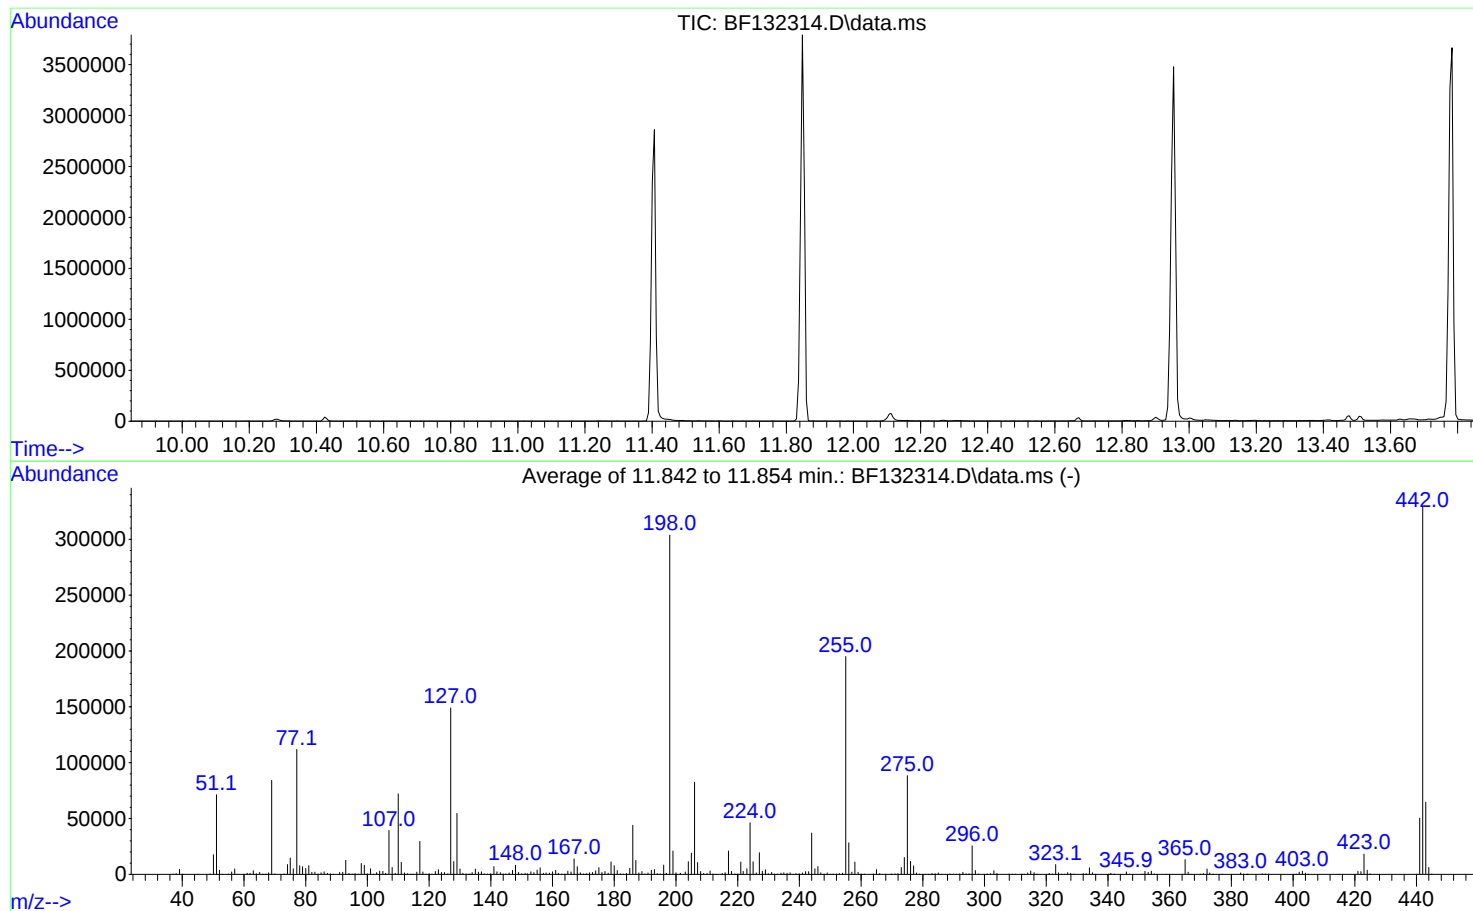




AutoFind: Scans 1531, 1532, 1533; Background Corrected with Scan 1526

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.5	71416	PASS
68	69	0.00	2	1.7	1392	PASS
69	198	0.00	100	27.7	84149	PASS
70	69	0.00	2	0.6	471	PASS
127	198	10	80	49.0	148933	PASS
197	198	0.00	2	0.3	935	PASS
198	198	100	100	100.0	303659	PASS
199	198	5	9	6.9	20989	PASS
275	198	10	60	29.1	88421	PASS
365	198	1	100	4.3	13193	PASS
441	198	0.01	100	16.6	50261	PASS
442	442	50	100	100.0	329365	PASS
443	442	15	24	19.6	64595	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020323\
Data File : BF132314.D
Acq On : 03 Feb 2023 10:12
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 04 03:59:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 04 01:32:42 2023
Response via : Initial Calibration

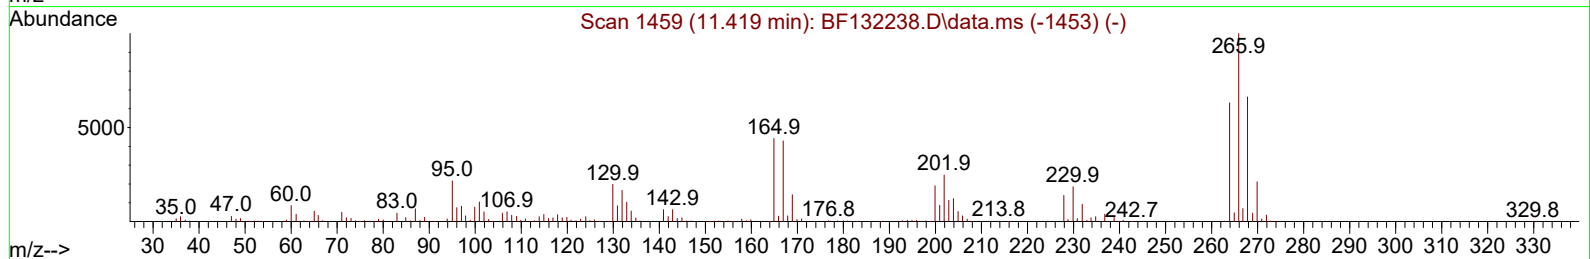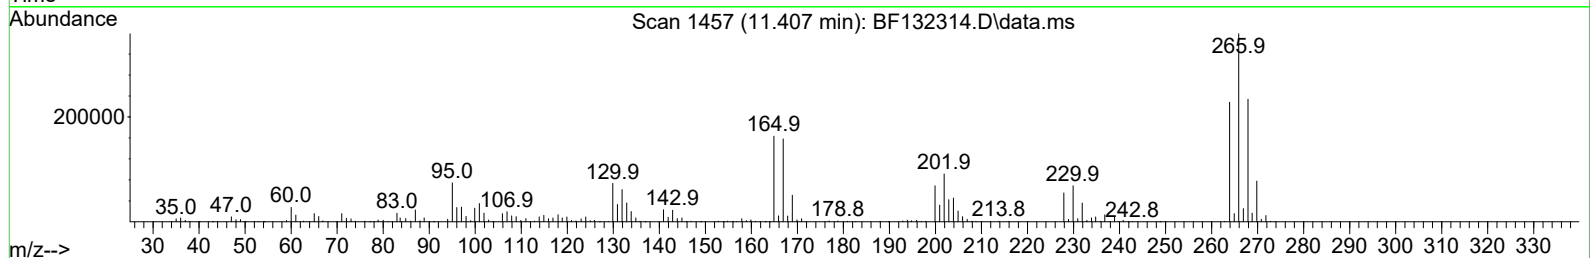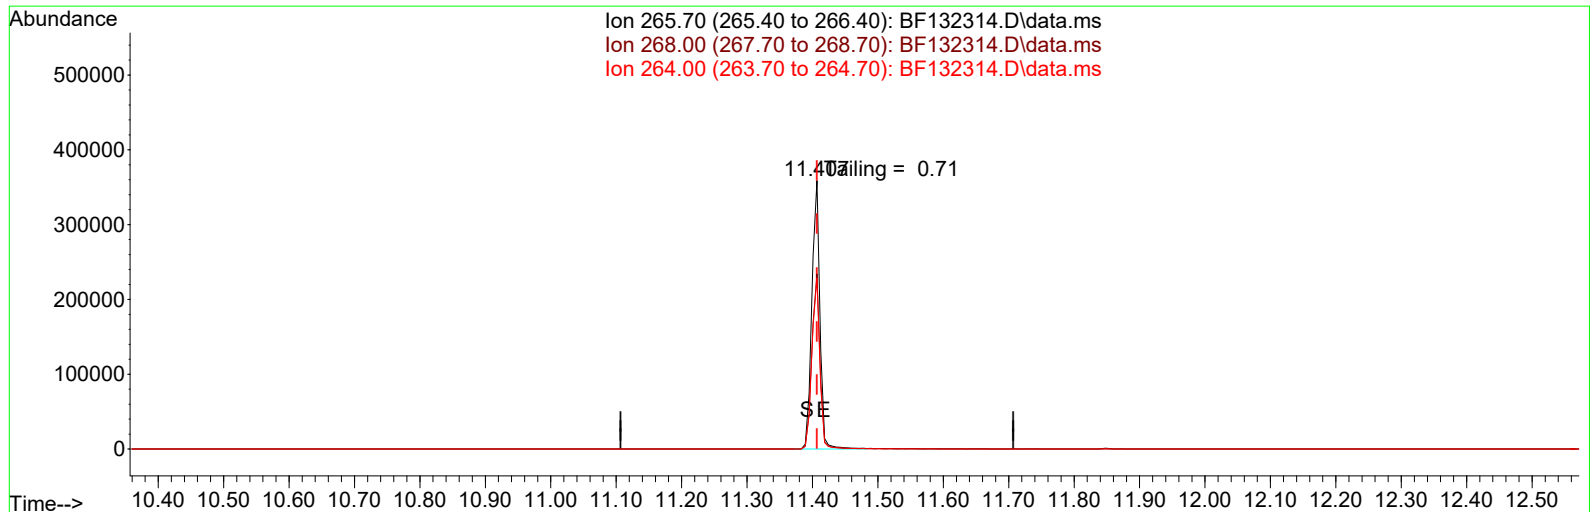

TIC: BF132314.D\data.ms

(70) Pentachlorophenol (C)

11.407min (-0.000) 745859.28 ng




response 308491

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	65.20
264.00	63.10	63.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020323\
Data File : BF132314.D
Acq On : 03 Feb 2023 10:12
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 04 03:59:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 04 01:32:42 2023
Response via : Initial Calibration

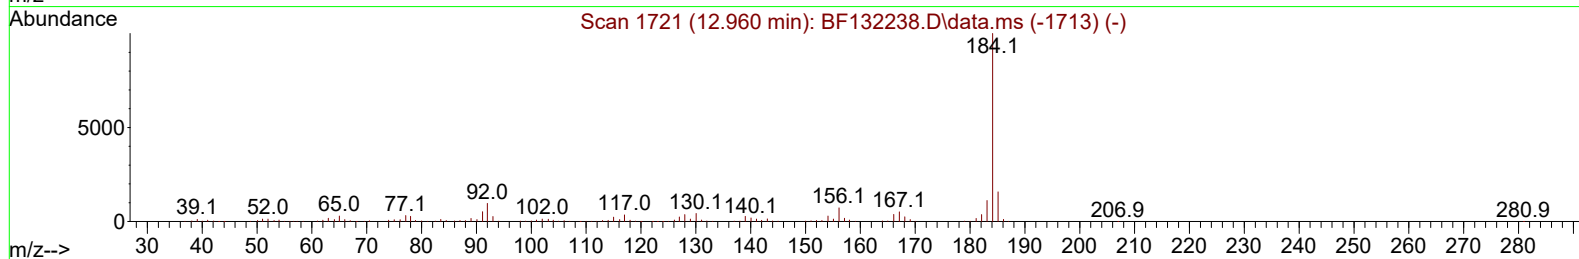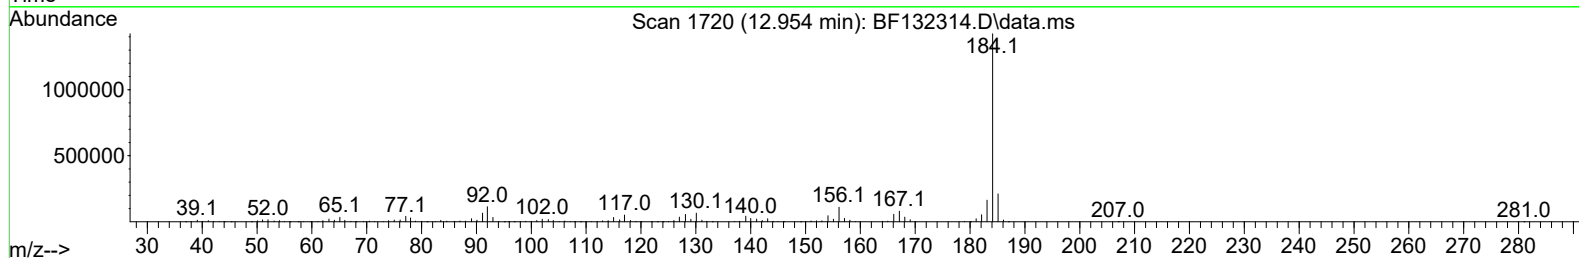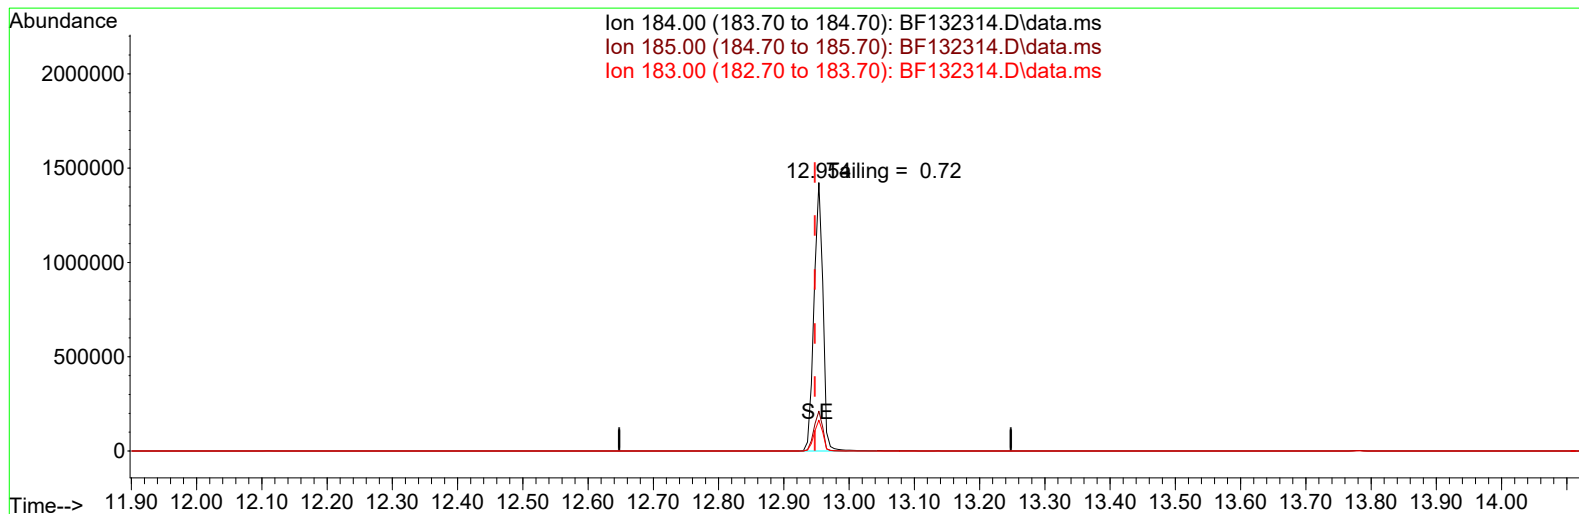

TIC: BF132314.D\data.ms

(77) Benzidine

12.954min (+ 0.006) 77737.14 ng

response 1369759

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.85
183.00	11.10	11.51
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/3/2023	BNA_F	<u>BF132314.D</u>
Compound Name	Response	Retention Time
DDT	649145	13.783
DDD	15148	13.477
DDE	616	13.136
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15764	664909	2.37

Instrument :
BNA_F
ClientSampleId :
DFTPP