
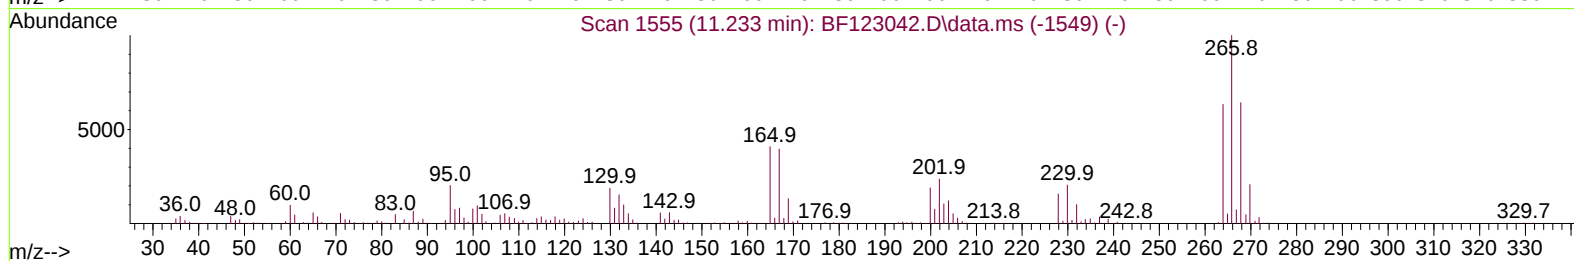
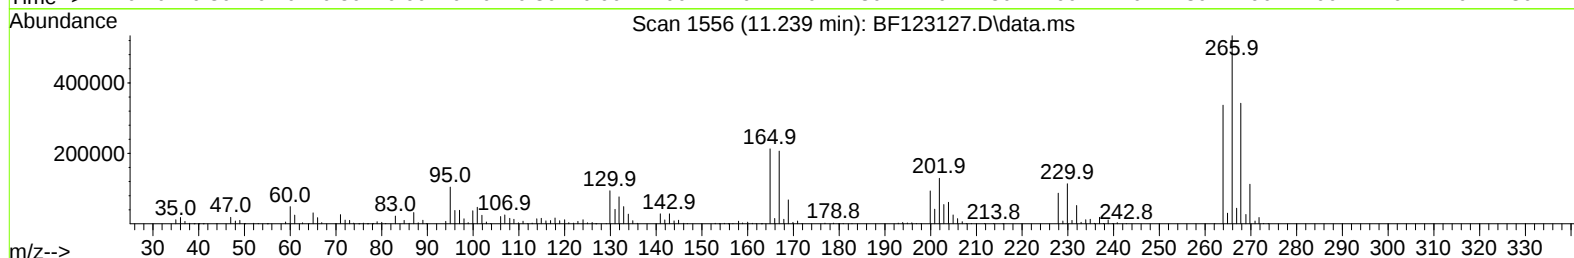


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020521\
 Data File : BF123127.D
 Acq On : 5 Feb 2021 9:57
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 04:06:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 29 12:29:00 2021
 Response via : Initial Calibration

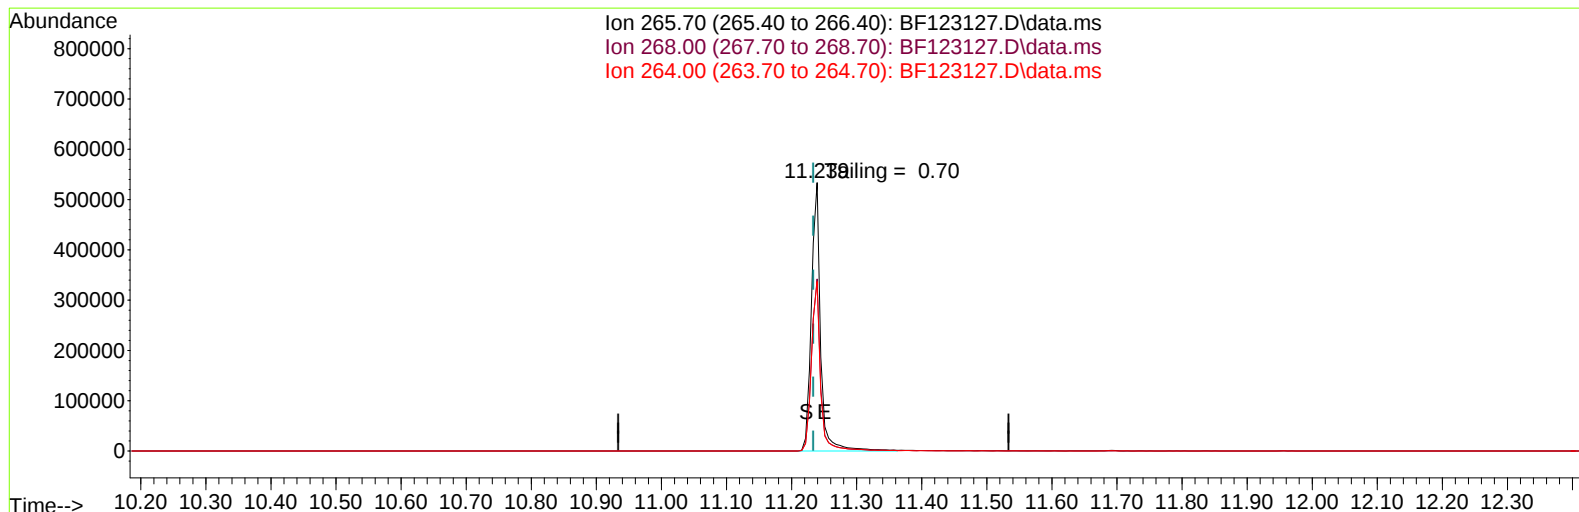

TIC: BF123127.D\data.ms




(70) Pentachlorophenol (C)

11.239min (+ 0.006) 37614.75 ng

response 531038

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.11
264.00	62.30	63.13
0.00	0.00	0.00

Quant Time: Feb 06 04:06:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 12:29:00 2021
Response via : Initial Calibration

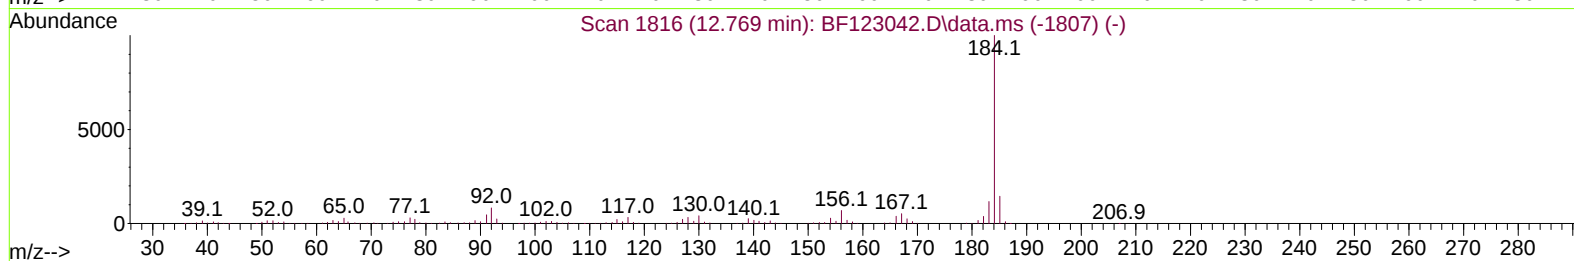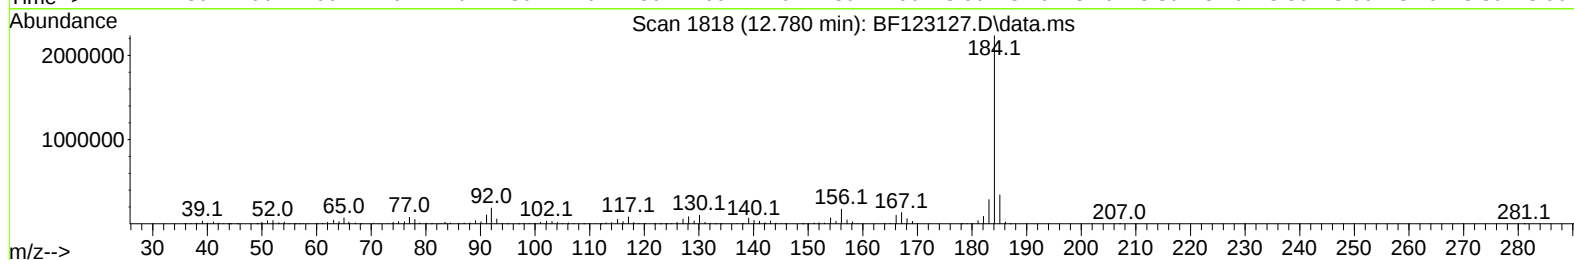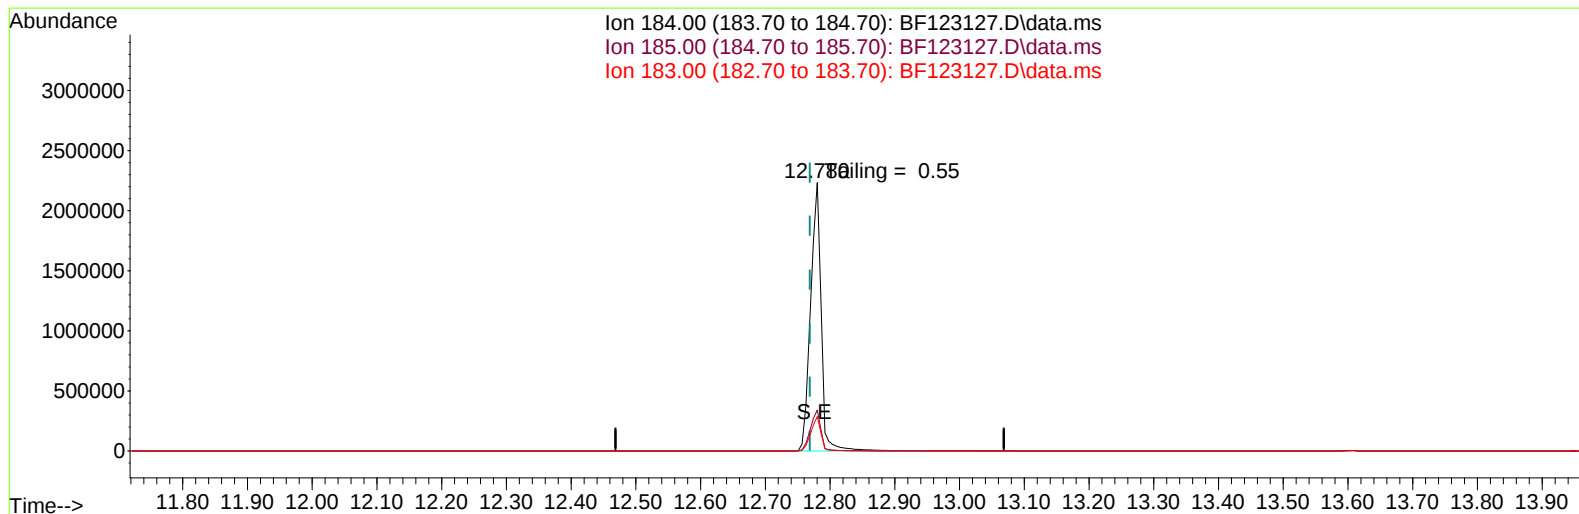

TIC: BF123127.D\data.ms

(77) Benzidine

12.780min (+ 0.012) 0.00 ng

response **2552196**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.31
183.00	12.10	12.84
0.00	0.00	0.00