

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020521\
 Data File : BF123131.D
 Acq On : 5 Feb 2021 12:40
 Operator : JU/CG
 Sample : PB134481BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB134481BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123131.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.252	18	28	34	rVB	83773	112757	1.16%	0.209%
2	5.528	579	585	588	rBV	5776177	6434460	66.29%	11.941%
3	6.522	748	754	757	rBV	5080579	6508242	67.05%	12.077%
4	6.892	813	817	821	rBV	1816449	1514800	15.61%	2.811%
5	7.457	907	913	916	rBV	3950823	4389736	45.23%	8.146%
6	8.175	1031	1035	1039	rBV	1939189	2003724	20.64%	3.718%
7	9.257	1213	1219	1222	rBV	7222456	7848996	80.87%	14.566%
8	9.939	1329	1335	1338	rBV	2454710	2391371	24.64%	4.438%
9	10.733	1463	1470	1473	rBV	4949231	5198642	53.56%	9.647%
10	11.433	1583	1589	1592	rBV	2569596	2489577	25.65%	4.620%
11	13.033	1854	1861	1864	rBV	8731303	9706059	100.00%	18.012%
12	14.086	2035	2040	2050	rBV	2680059	2581399	26.60%	4.790%
13	15.580	2288	2294	2310	rBV	1642029	2469131	25.44%	4.582%
14	16.057	2370	2375	2384	rBV	77432	133262	1.37%	0.247%
15	16.586	2460	2465	2471	rVB2	61121	105205	1.08%	0.195%




Sum of corrected areas: 53887361

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020521\
Data File : BF123131.D
Acq On : 5 Feb 2021 12:40
Operator : JU/CG
Sample : PB134481BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134481BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

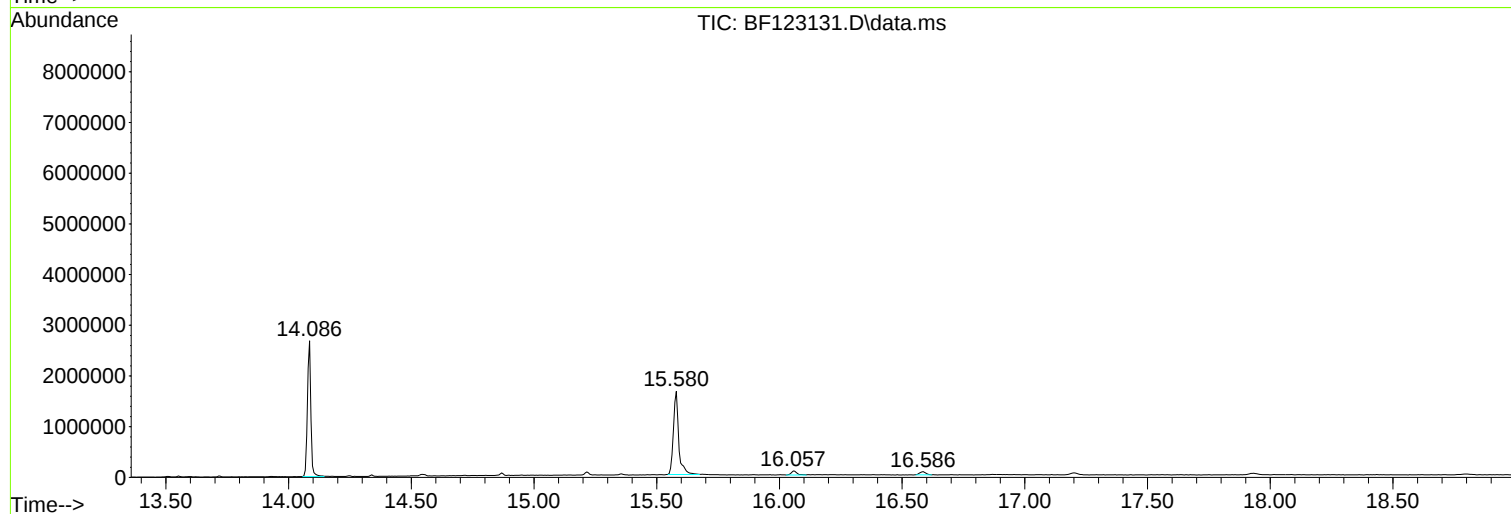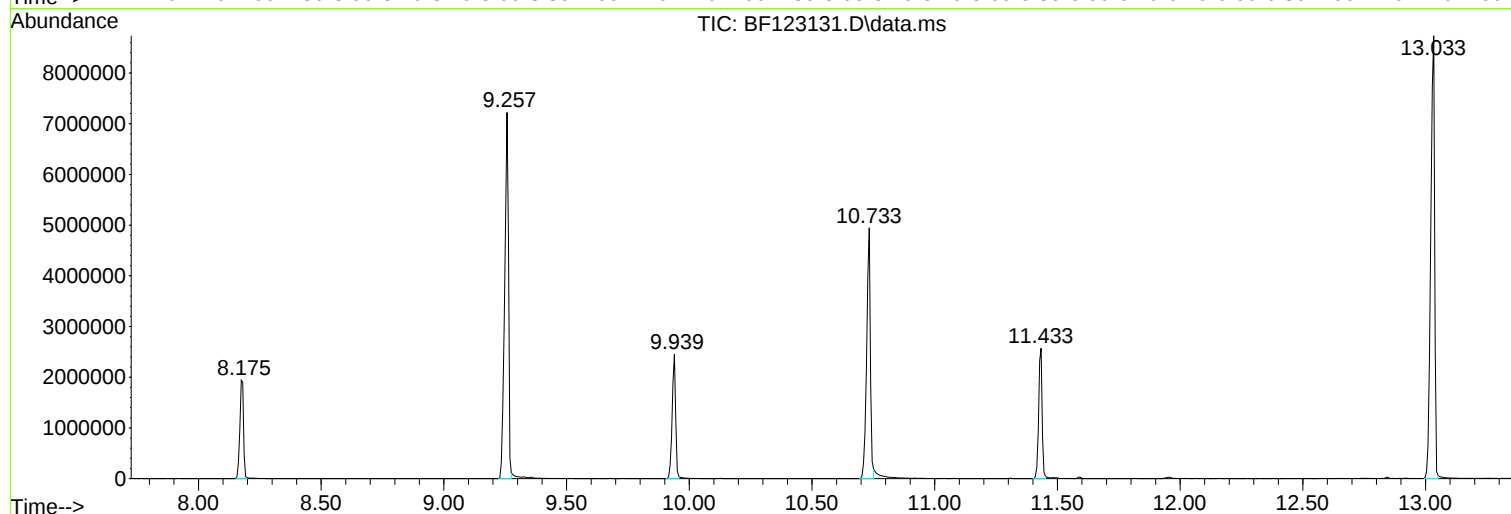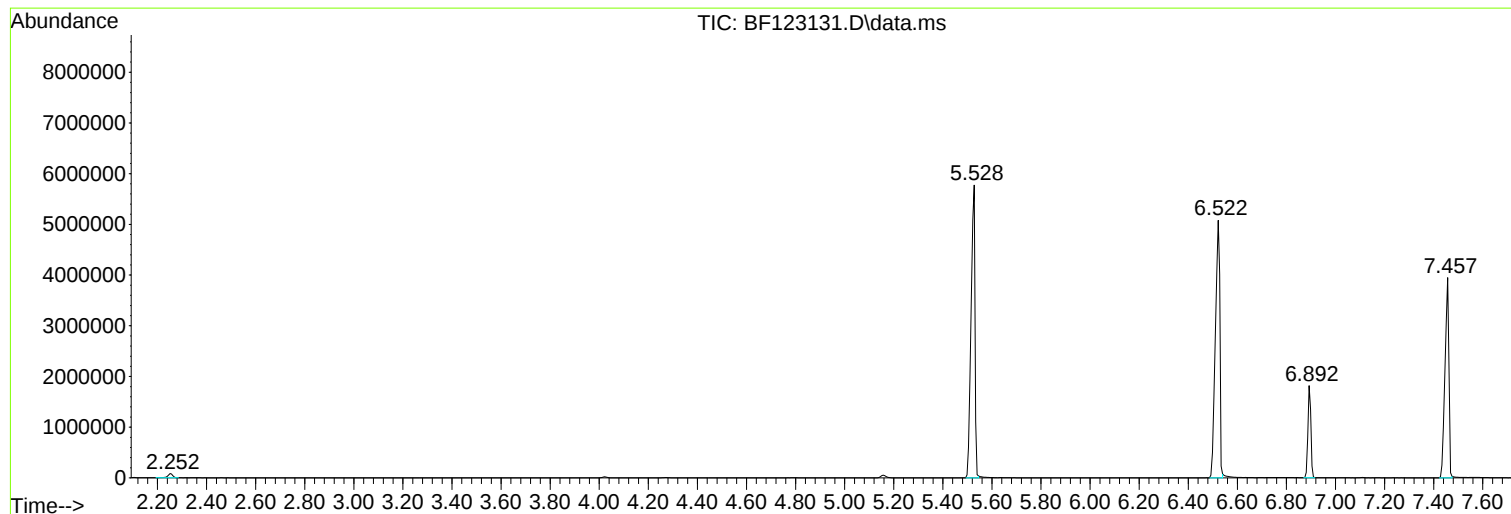

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020521\
Data File : BF123131.D
Acq On : 5 Feb 2021 12:40
Operator : JU/CG
Sample : PB134481BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134481BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020521\
Data File : BF123131.D
Acq On : 5 Feb 2021 12:40
Operator : JU/CG
Sample : PB134481BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134481BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------