
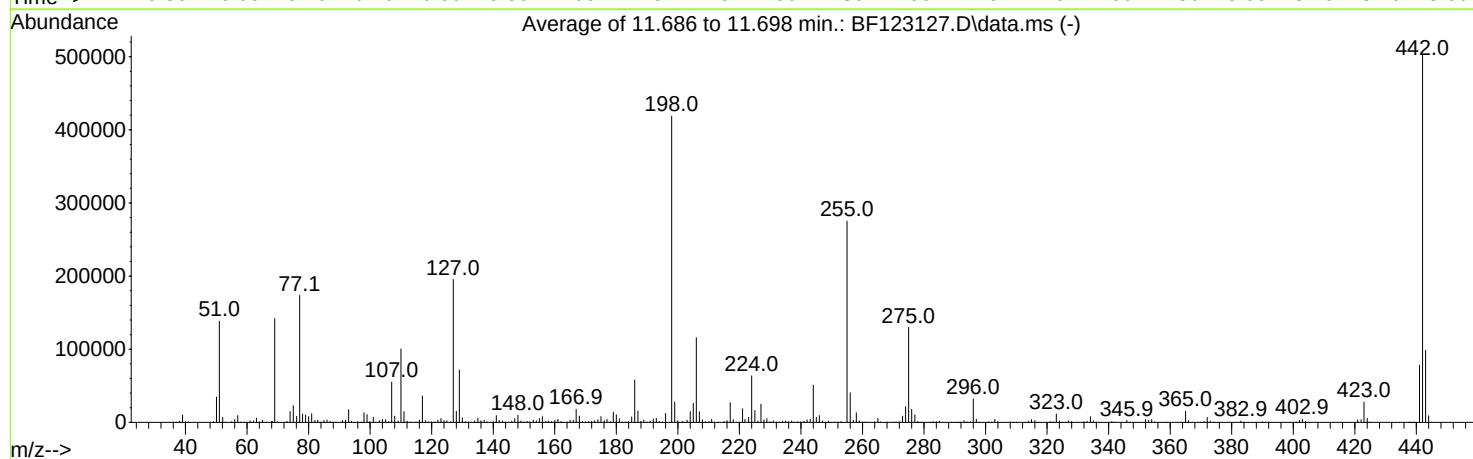


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020521\
 Data File : BF123127.D
 Acq On : 5 Feb 2021 9:57
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 29 12:29:00 2021

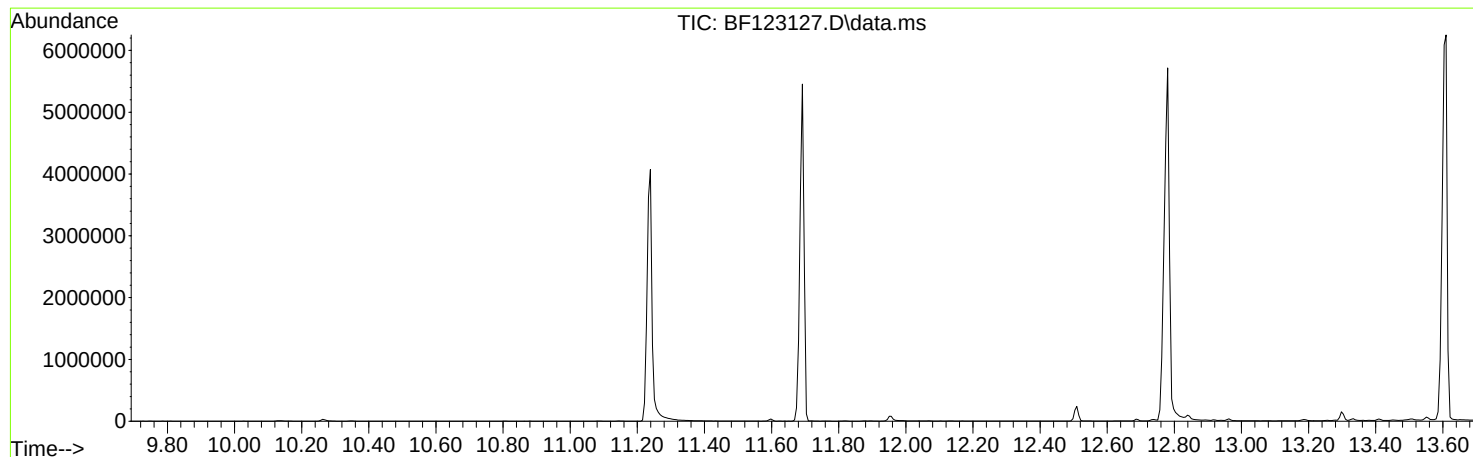

AutoFind: Scans 1632, 1633, 1634; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	138184	PASS
68	69	0.00	2	1.0	1436	PASS
69	198	0.00	100	33.9	141923	PASS
70	69	0.00	2	0.5	743	PASS
127	198	10	80	46.7	195416	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	418709	PASS
199	198	5	9	6.6	27808	PASS
275	198	10	60	31.0	129747	PASS
365	198	1	100	3.7	15345	PASS
441	198	0.01	100	18.7	78213	PASS
442	442	50	100	100.0	502997	PASS
443	442	15	24	19.6	98408	PASS