


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020623\
Data File : BF132334.D
Acq On : 06 Feb 2023 12:42
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 07 04:05:36 2023

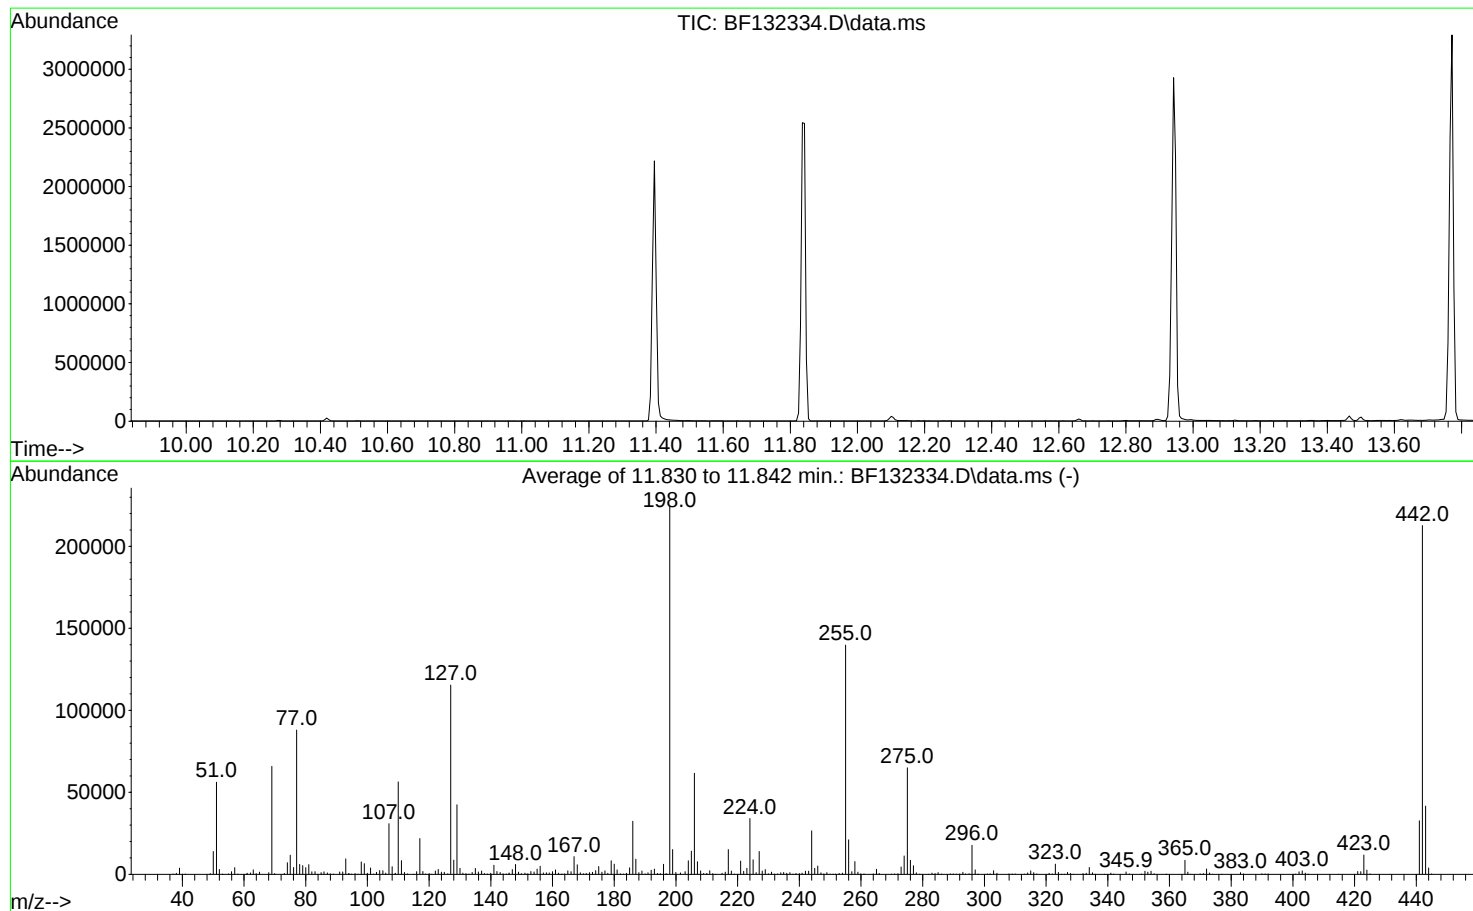




AutoFind: Scans 1529, 1530, 1531; Background Corrected with Scan 1524

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.0	56163	PASS
68	69	0.00	2	1.6	1067	PASS
69	198	0.00	100	29.3	65827	PASS
70	69	0.00	2	0.6	410	PASS
127	198	10	80	51.4	115381	PASS
197	198	0.00	2	0.1	336	PASS
198	198	100	100	100.0	224355	PASS
199	198	5	9	6.7	15117	PASS
275	198	10	60	28.9	64941	PASS
365	198	1	100	3.8	8577	PASS
441	198	0.01	100	14.5	32629	PASS
442	442	50	100	100.0	212736	PASS
443	442	15	24	19.6	41607	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020623\  
Data File : BF132334.D  
Acq On    : 06 Feb 2023  12:42  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 07 05:43:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 07 04:05:36 2023
Response via : Initial Calibration

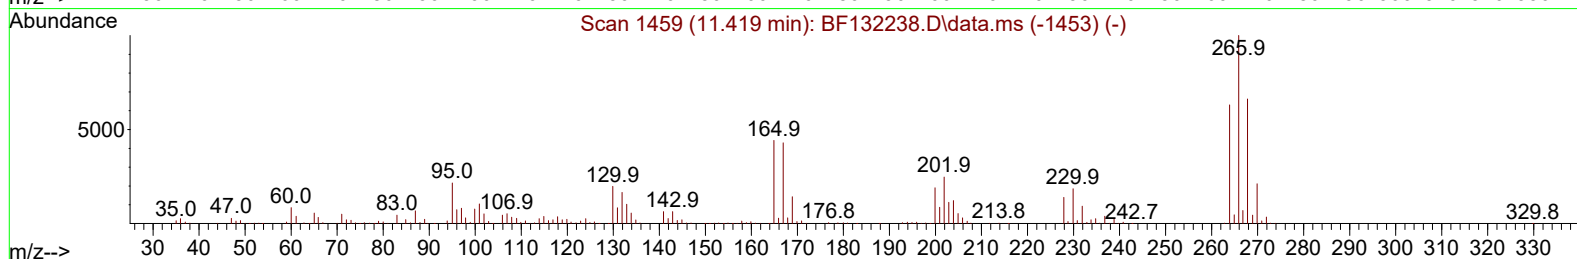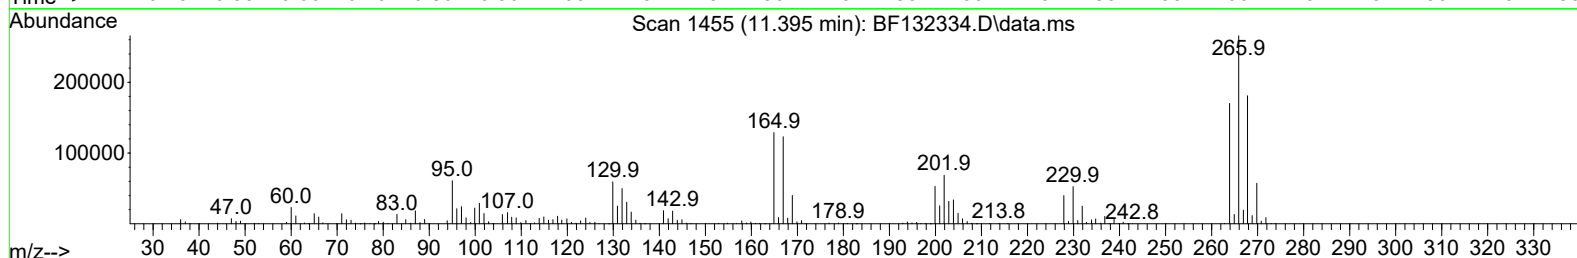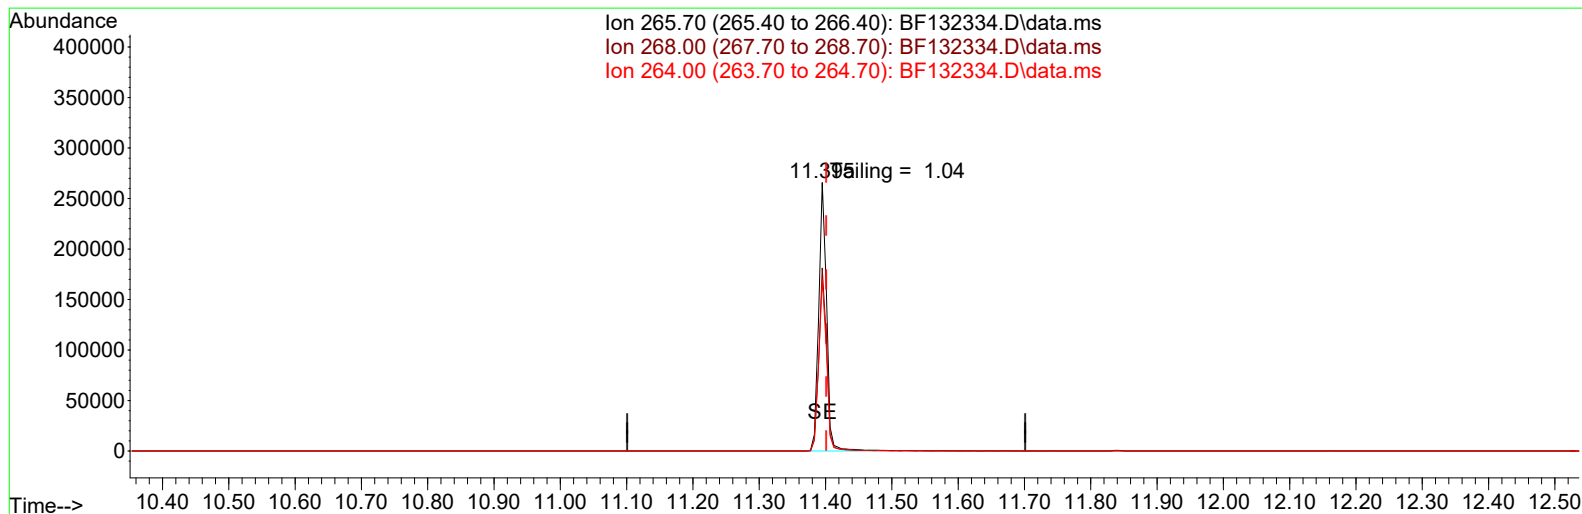

TIC: BF132334.D\data.ms

(70) Pentachlorophenol (C)

11.395min (-0.006) 24537.97 ng




response **219957**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	68.14
264.00	63.10	64.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020623\
Data File : BF132334.D
Acq On : 06 Feb 2023 12:42
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 07 05:43:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 07 04:05:36 2023
Response via : Initial Calibration

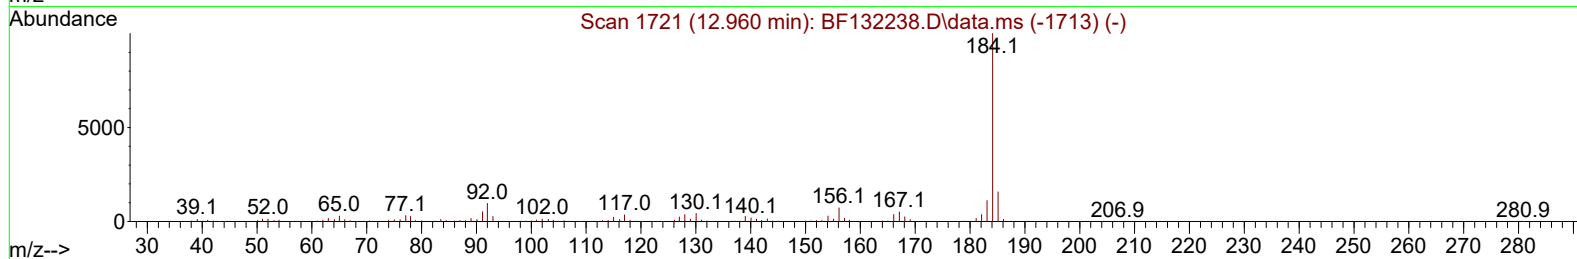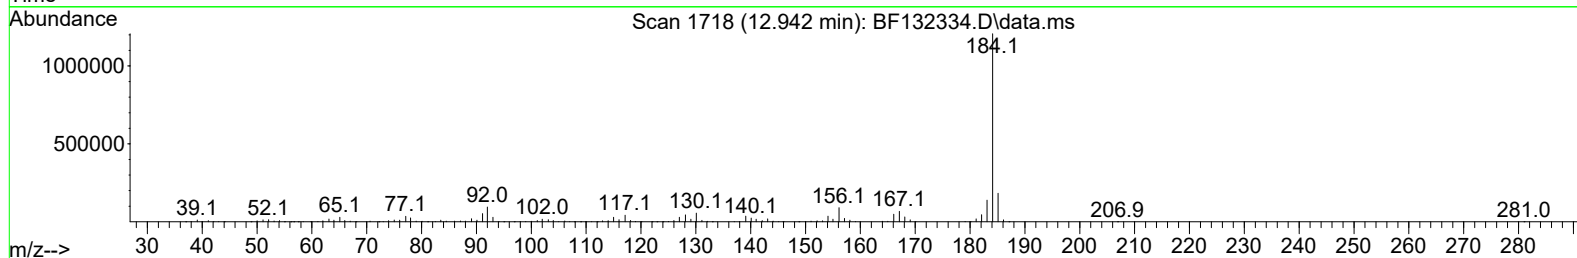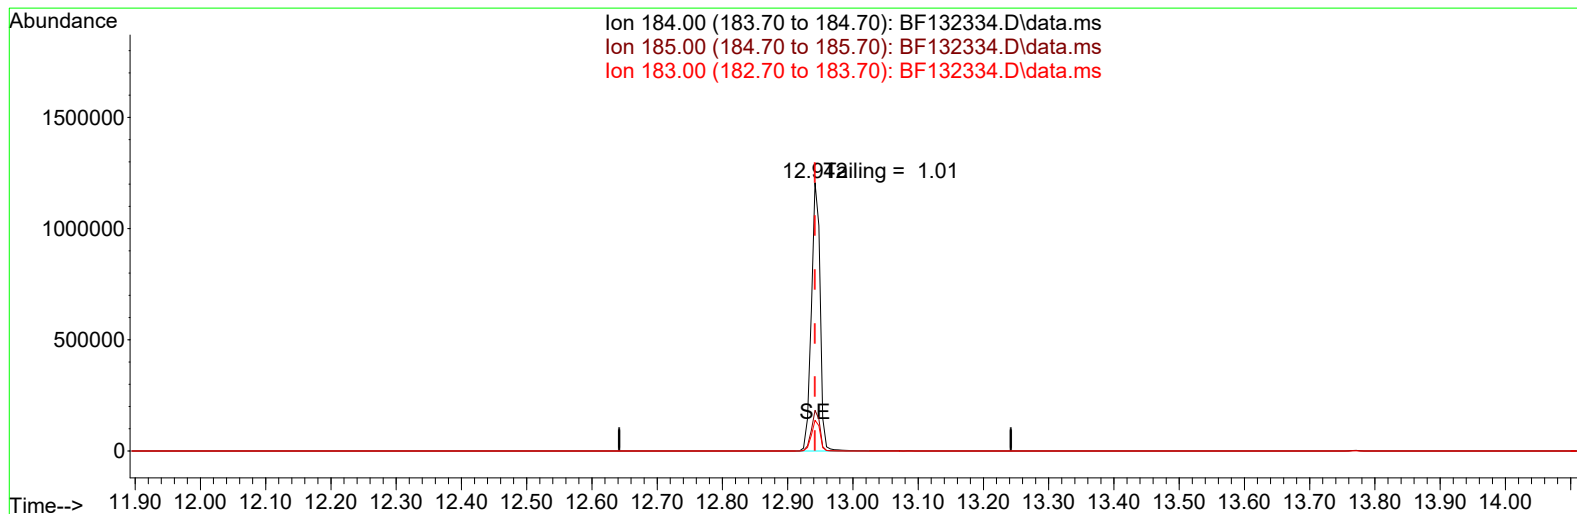

TIC: BF132334.D\data.ms

(77) Benzidine

12.942min (-0.000) 0.00 ng

response 1138542

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	15.17
183.00	11.10	11.49
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/6/2023	BNA_F	<u>BF132334.D</u>
Compound Name	Response	Retention Time
DDT	538270	13.771
DDD	11430	13.466
DDE	725	13.124
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12155	550425	2.21

Instrument :
BNA_F
ClientSampleId :
DFTPP