
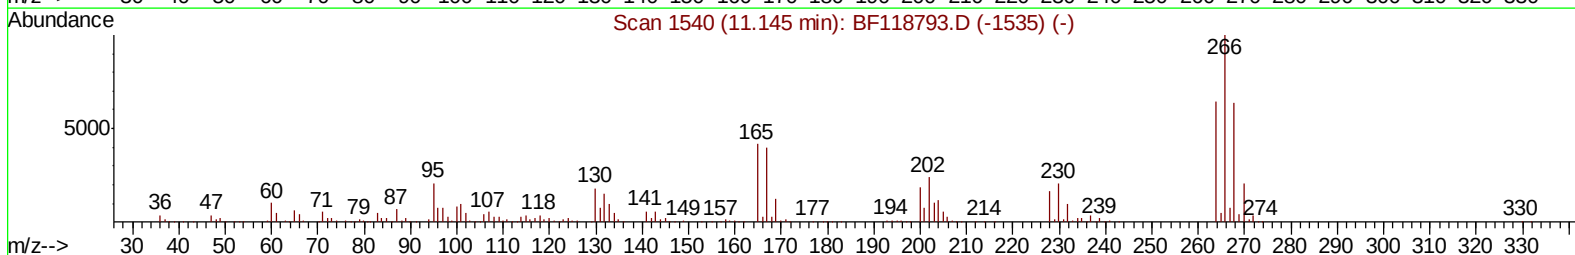
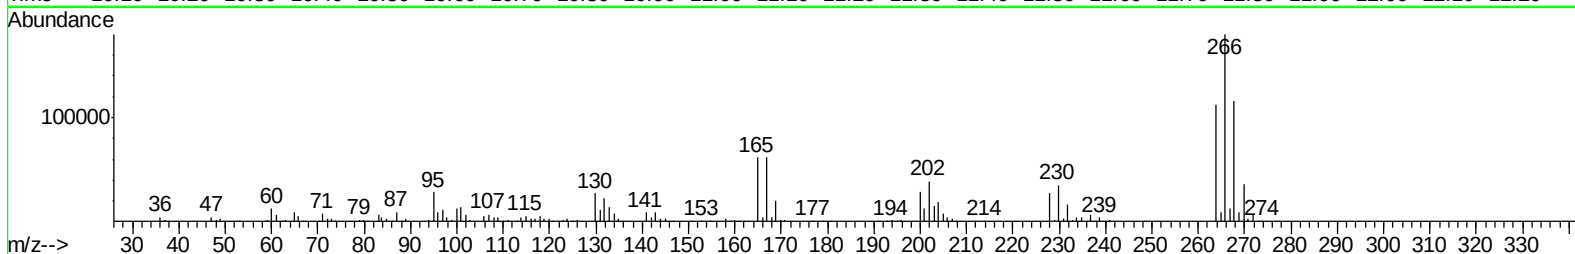


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF020720\
Data File : BF118844.D
Acq On : 7 Feb 2020 9:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 05:50:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF020320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 03 16:26:03 2020
Response via : Initial Calibration

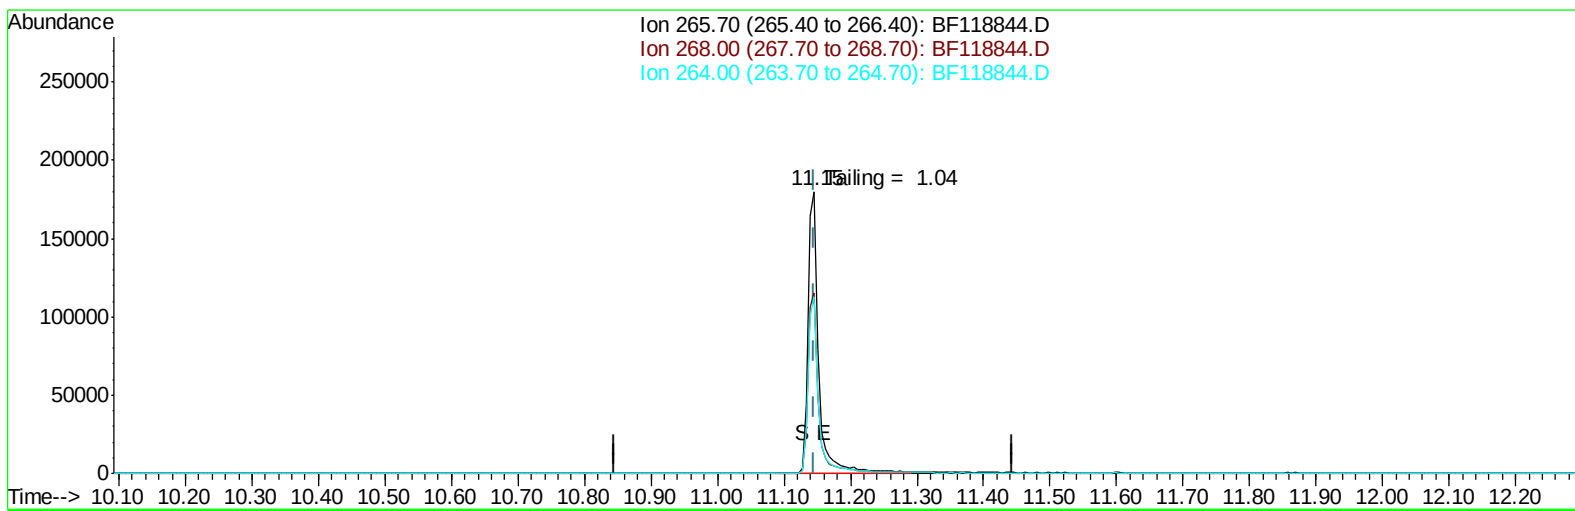

TIC: BF118844.D

(70) Pentachlorophenol (C)




11.145min (+0.000) 34021.68ng

response 204014

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	64.21
264.00	64.30	62.52
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF020720\
 Data File : BF118844.D
 Acq On : 7 Feb 2020 9:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 05:50:25 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF020320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 03 16:26:03 2020
 Response via : Initial Calibration

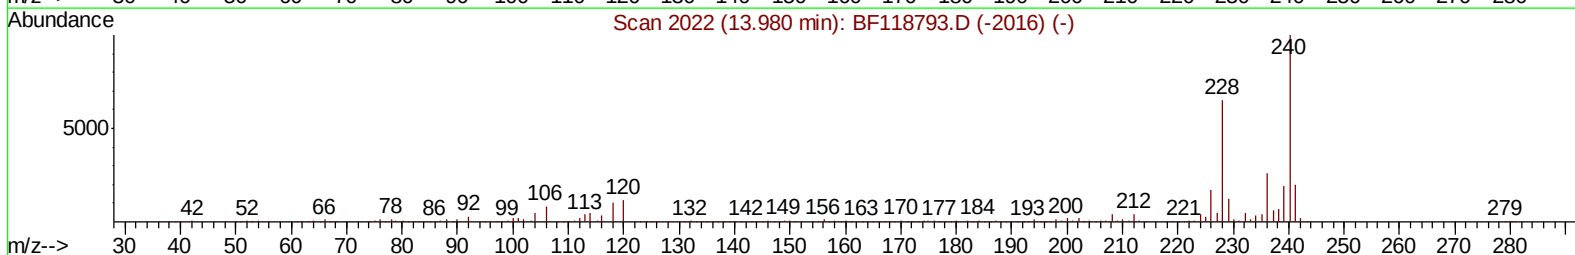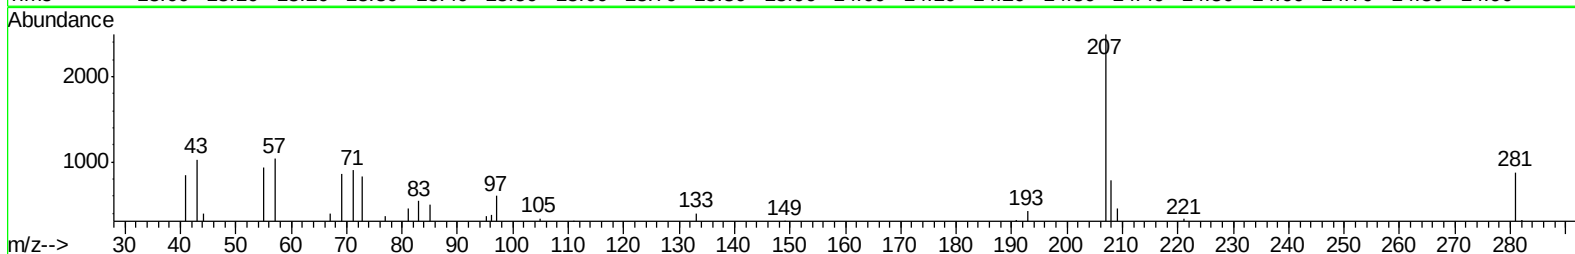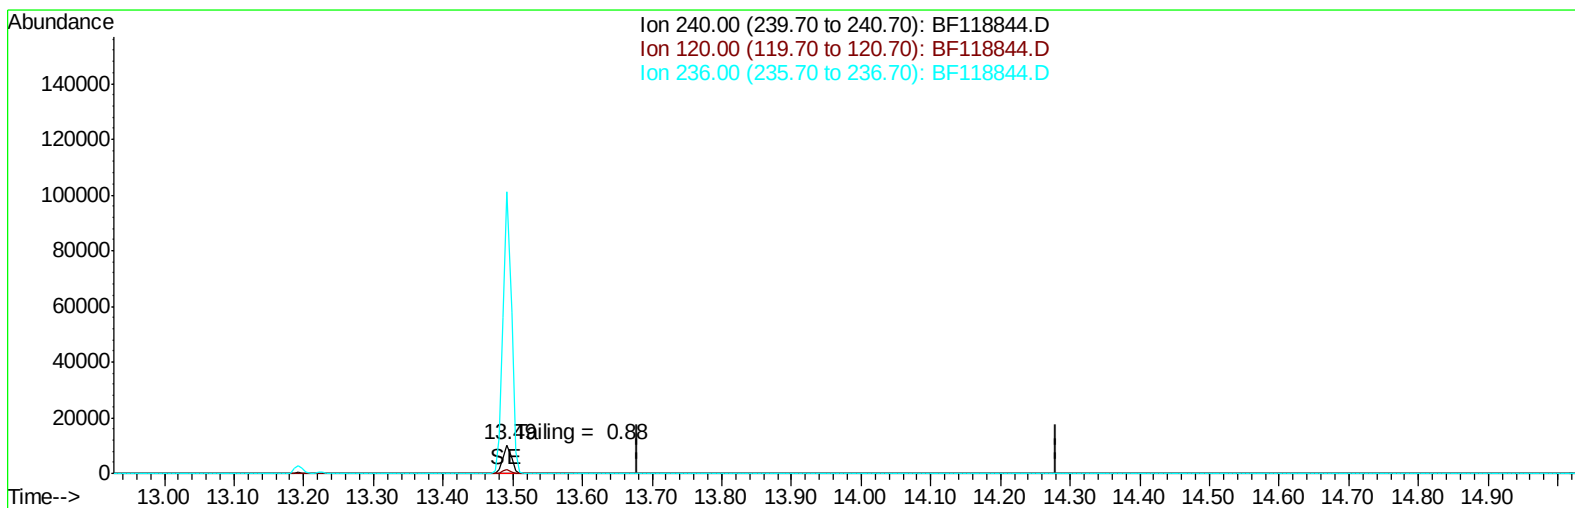

TIC: BF118844.D

(76) Chrysene-d12 (I)

13.980min (-13.980) 0.00ng

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	11.70	0.00#
236.00	26.30	0.00#
0.00	0.00	0.00