
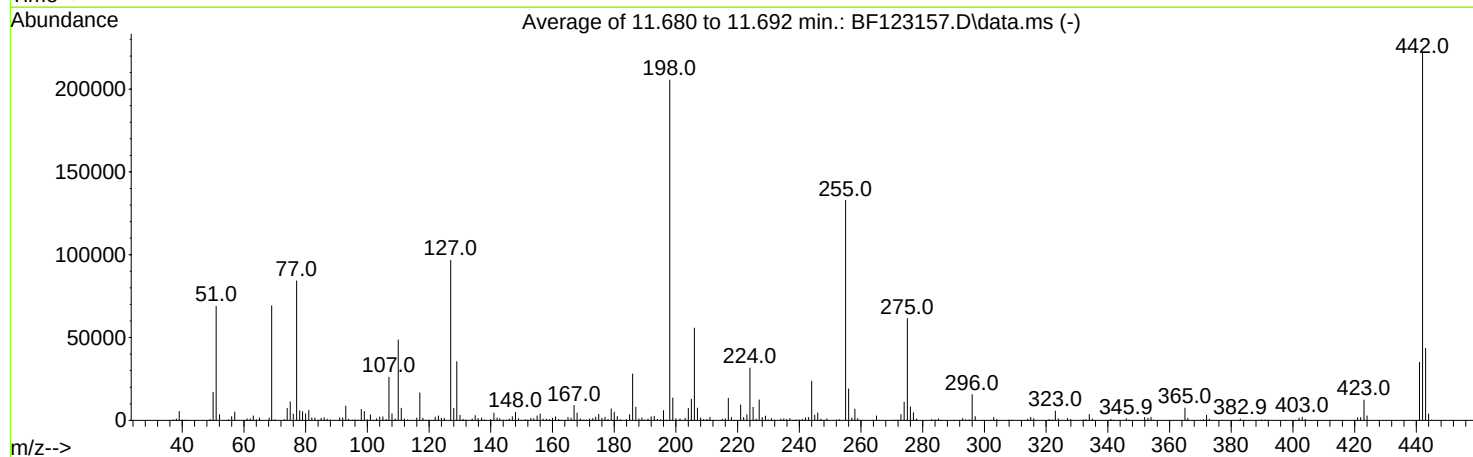


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020921\
 Data File : BF123157.D
 Acq On : 9 Feb 2021 9:39
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 29 12:29:00 2021

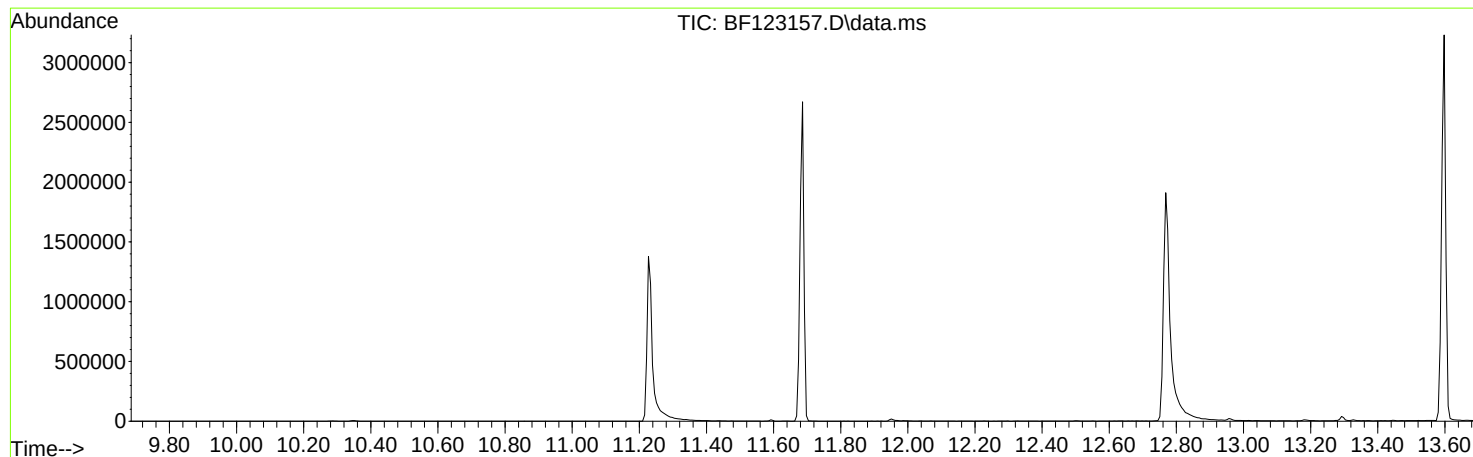

AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	68875	PASS
68	69	0.00	2	2.0	1353	PASS
69	198	0.00	100	33.6	69141	PASS
70	69	0.00	2	0.6	397	PASS
127	198	10	80	47.0	96613	PASS
197	198	0.00	2	0.1	215	PASS
198	198	100	100	100.0	205496	PASS
199	198	5	9	6.6	13509	PASS
275	198	10	60	29.9	61483	PASS
365	198	1	100	3.6	7469	PASS
441	198	0.01	100	17.1	35101	PASS
442	442	50	100	100.0	222080	PASS
443	442	15	24	19.6	43485	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/9/2021	BNA_F	<u>BF123157.D</u>
Compound Name	Response	Retention Time
DDT	555363	13.59
DDD	7742	13.29
DDE	2670	12.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10412	565775	1.84

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020921\
 Data File : BF123157.D
 Acq On : 9 Feb 2021 9:39
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 09 16:44:45 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 29 12:29:00 2021
 Response via : Initial Calibration

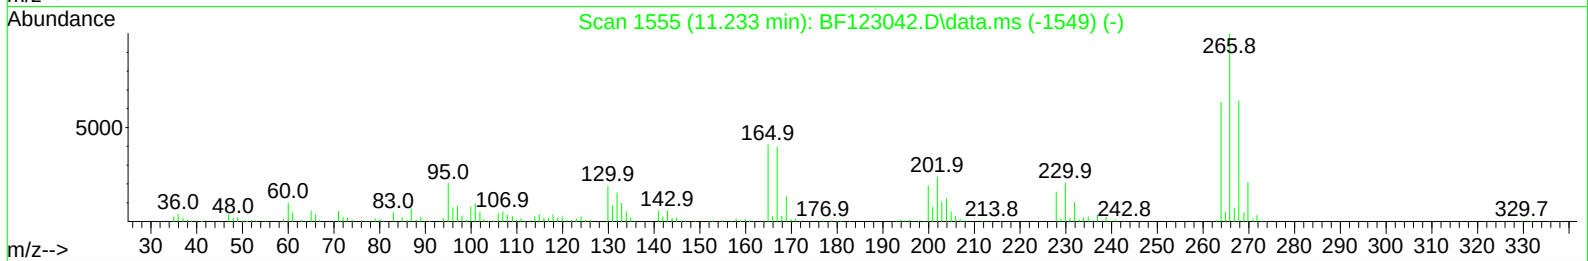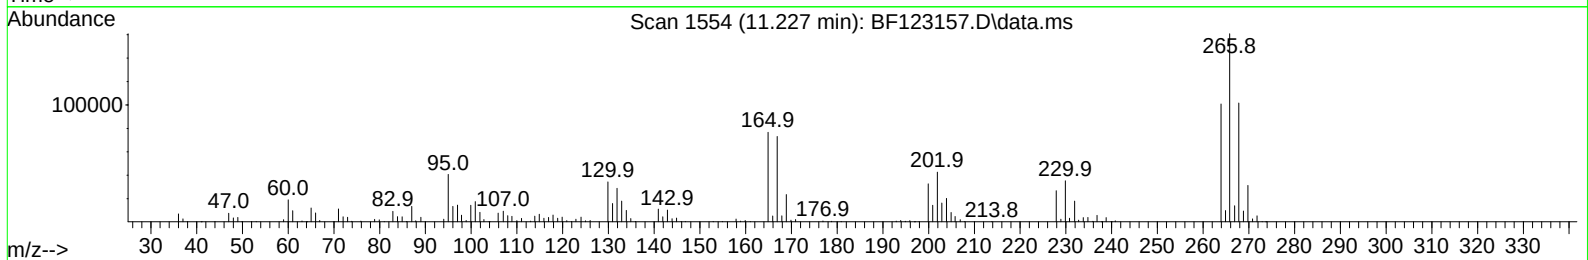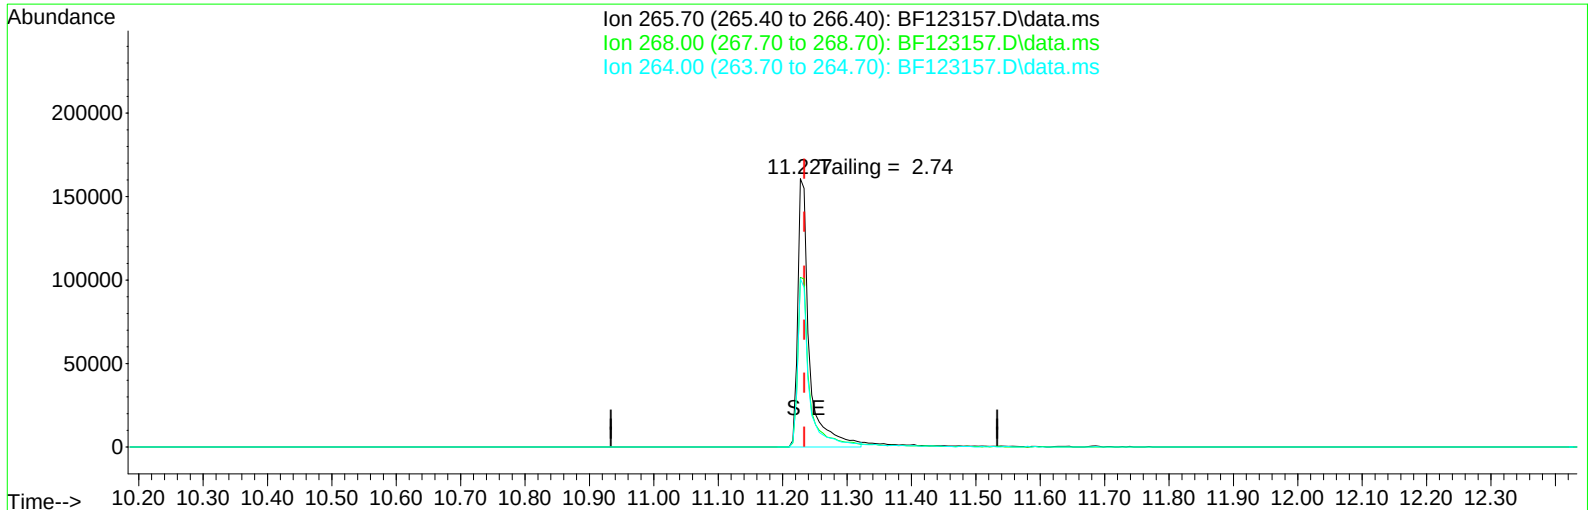

TIC: BF123157.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.006) 31767.77 ng




response 212369

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.22
264.00	62.30	62.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020921\
Data File : BF123157.D
Acq On : 9 Feb 2021 9:39
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 09 16:44:45 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 12:29:00 2021
Response via : Initial Calibration

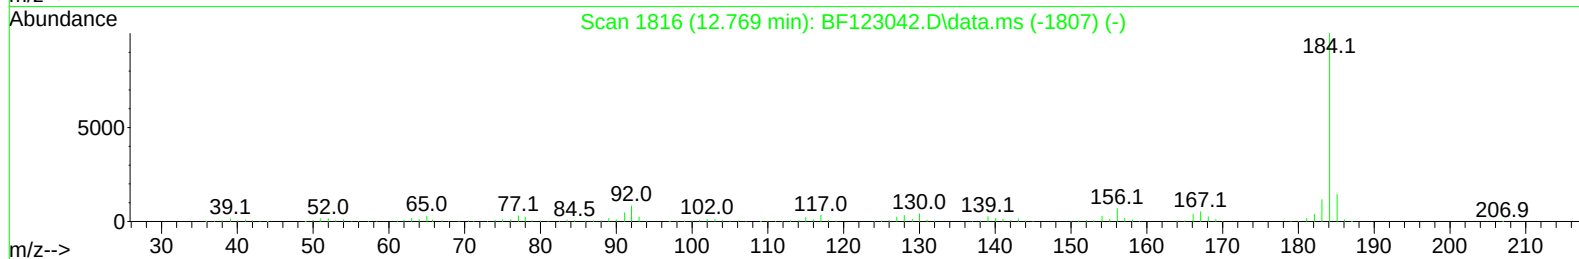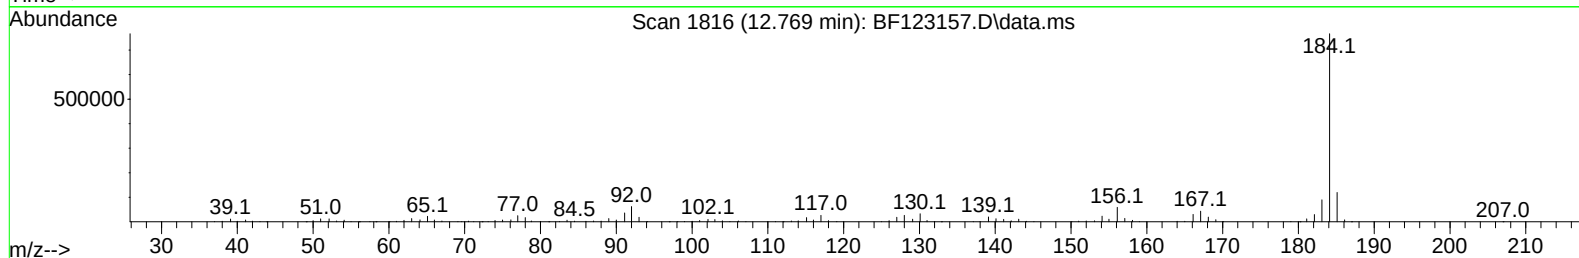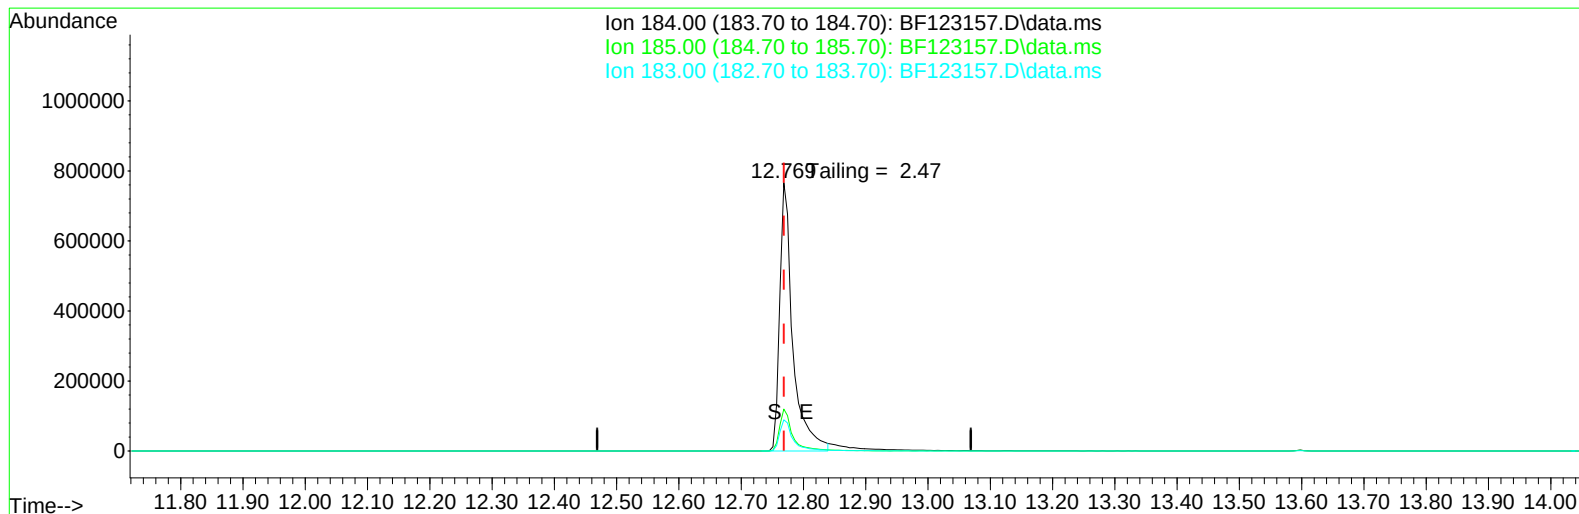

TIC: BF123157.D\data.ms

(77) Benzidine

12.769min (-0.000) 0.00 ng

response 1191256

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.63
183.00	12.10	11.67
0.00	0.00	0.00