


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF021020\
 Data File : BF118863.D
 Acq On : 10 Feb 2020 9:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 02:39:45 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF020320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 03 16:26:03 2020
 Response via : Initial Calibration

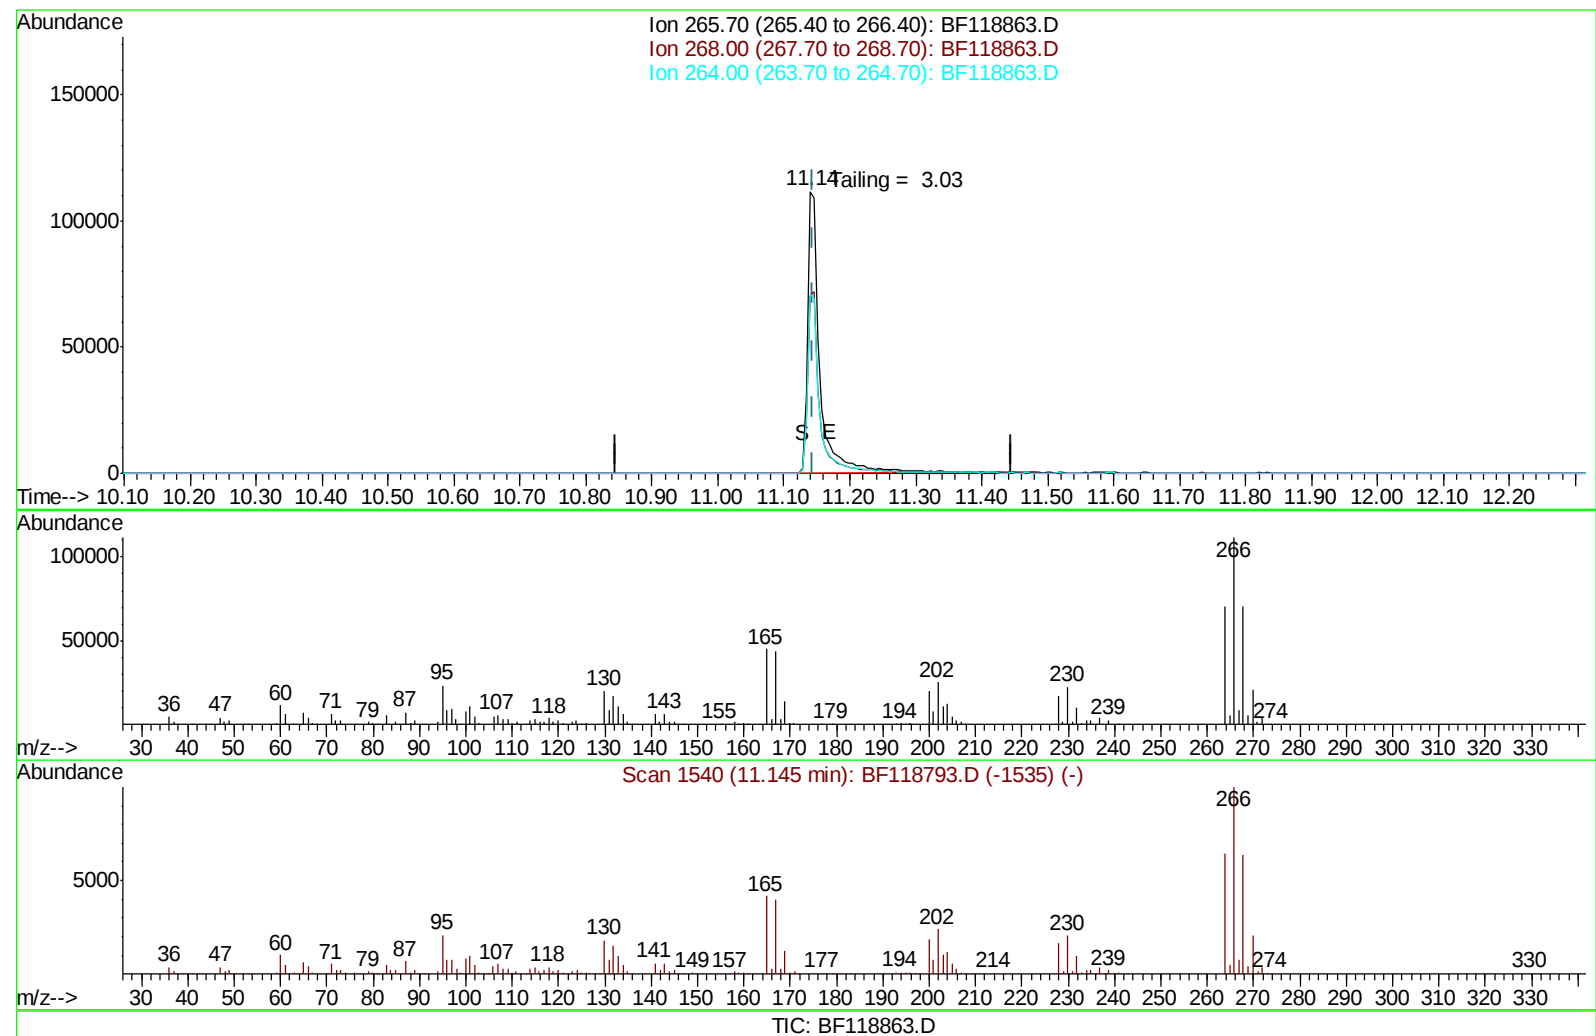

TIC: BF118863.D

(70) Pentachlorophenol (C)




11.139min (-0.006) 29913.44ng

response 149375

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	63.40
264.00	64.30	63.44
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF021020\
 Data File : BF118863.D
 Acq On : 10 Feb 2020 9:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 02:39:45 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF020320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 03 16:26:03 2020
 Response via : Initial Calibration

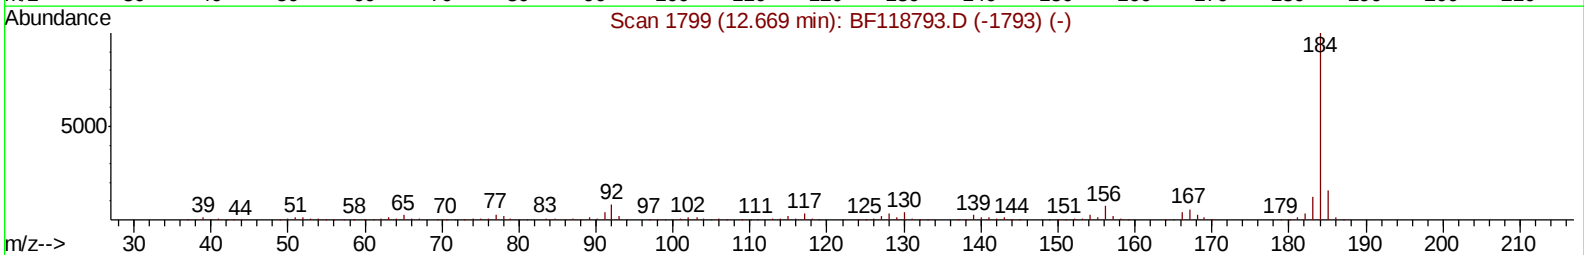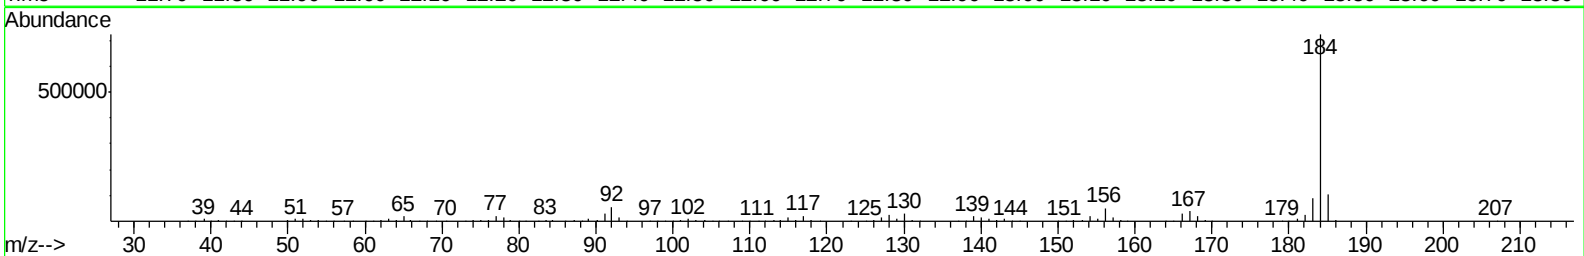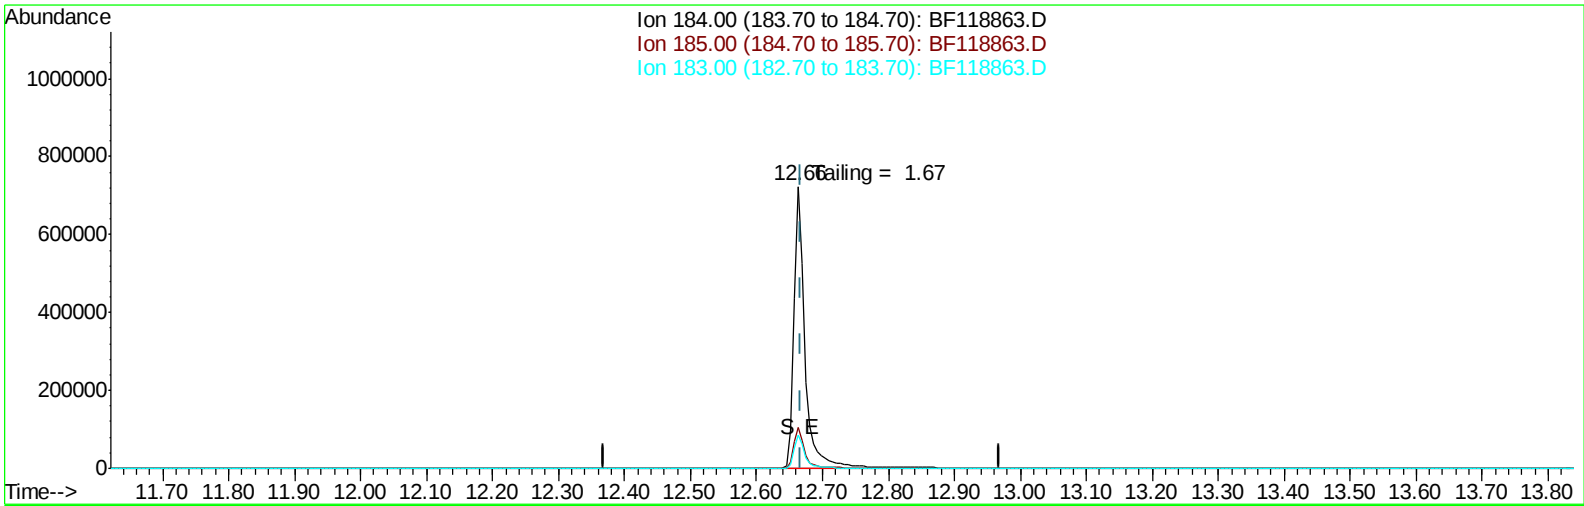

TIC: BF118863.D

(77) Benzidine

12.663min (-0.006) 0.00ng

response 860826

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.56
183.00	12.10	12.05
0.00	0.00	0.00