


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021020\
 Data File : BF118863.D
 Acq On : 10 Feb 2020 9:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF020320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 03 16:26:03 2020

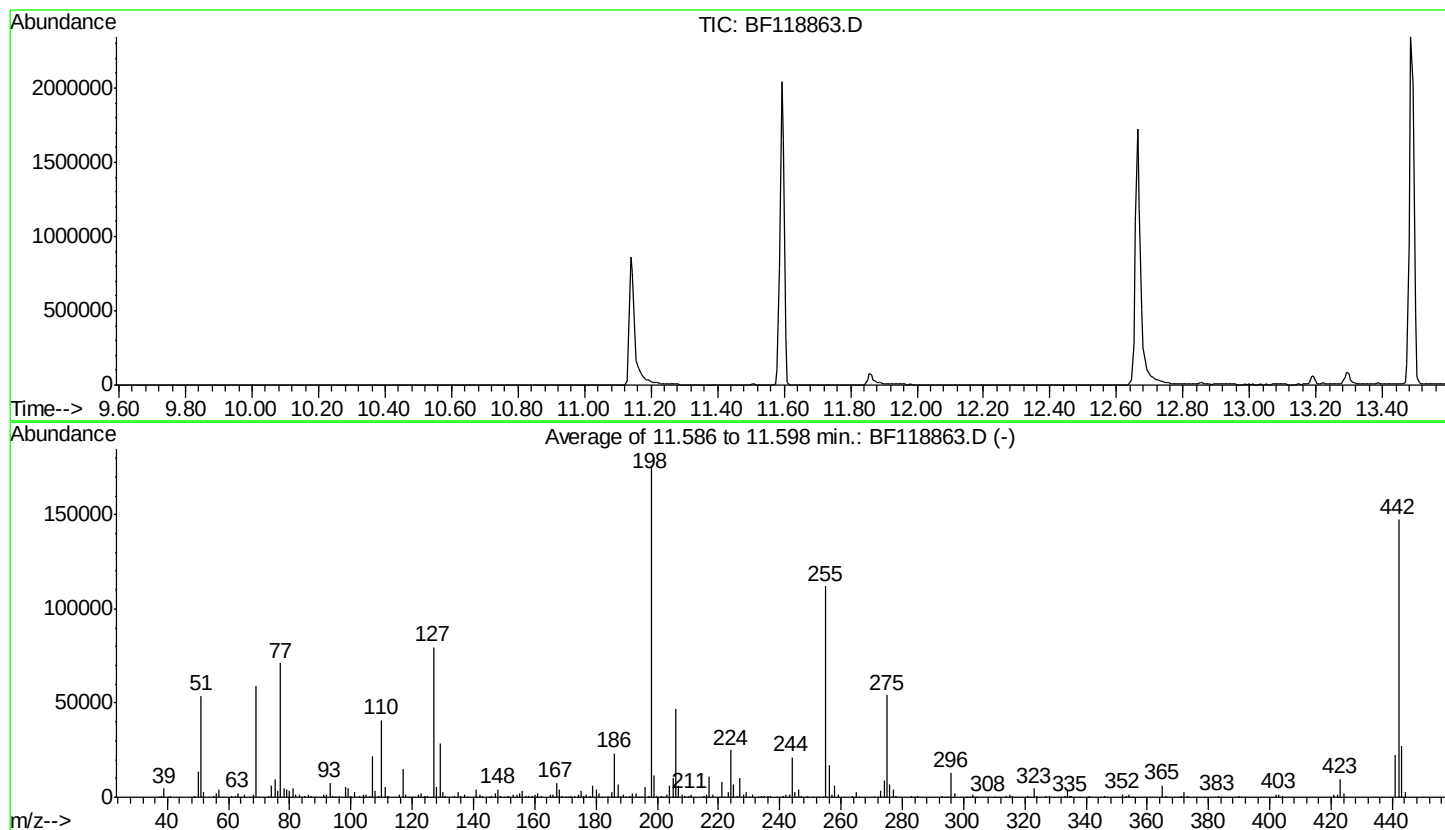

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	53709	PASS
68	69	0.00	2	1.9	1106	PASS
69	198	0.00	100	33.6	59186	PASS
70	69	0.00	2	0.4	257	PASS
127	198	10	80	45.3	79674	PASS
197	198	0.00	2	0.4	618	PASS
198	198	100	100	100.0	176029	PASS
199	198	5	9	6.7	11707	PASS
275	198	10	60	30.8	54165	PASS
365	198	1	100	3.6	6422	PASS
441	198	0.01	100	12.7	22295	PASS
442	198	50	100	83.6	147146	PASS
443	442	15	24	18.7	27488	PASS