
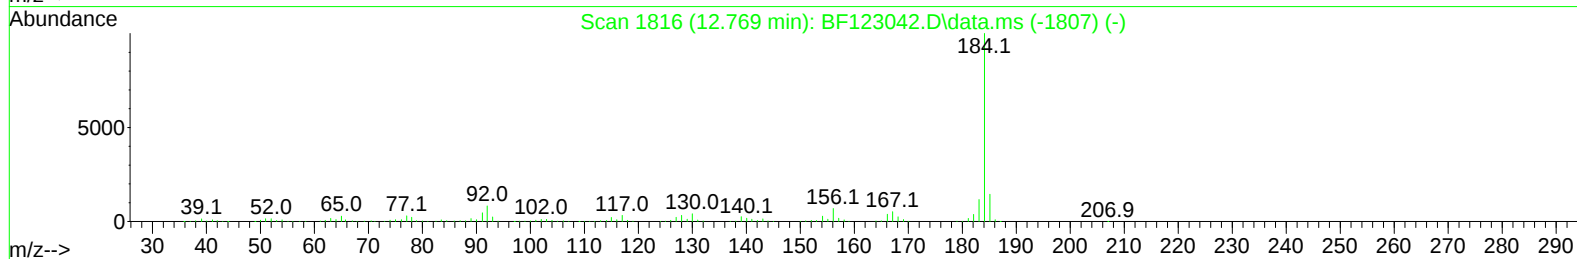
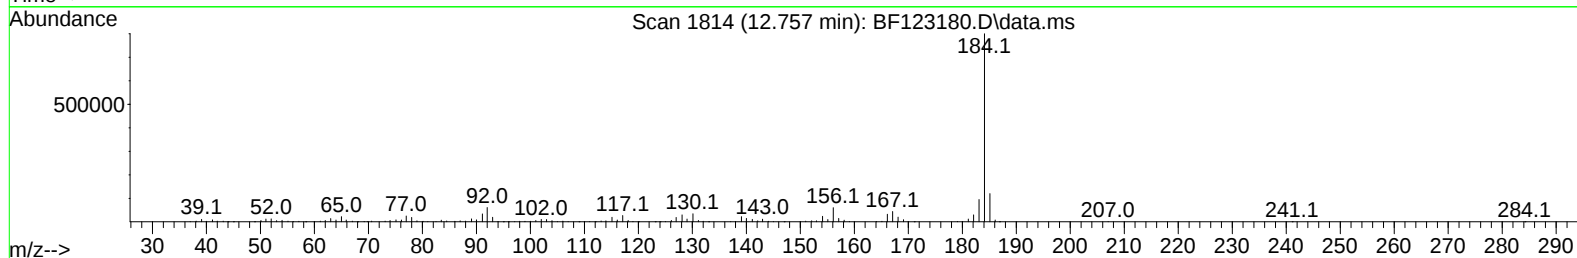


Quant Time: Feb 11 14:03:20 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 11 13:57:30 2021
Response via : Initial Calibration

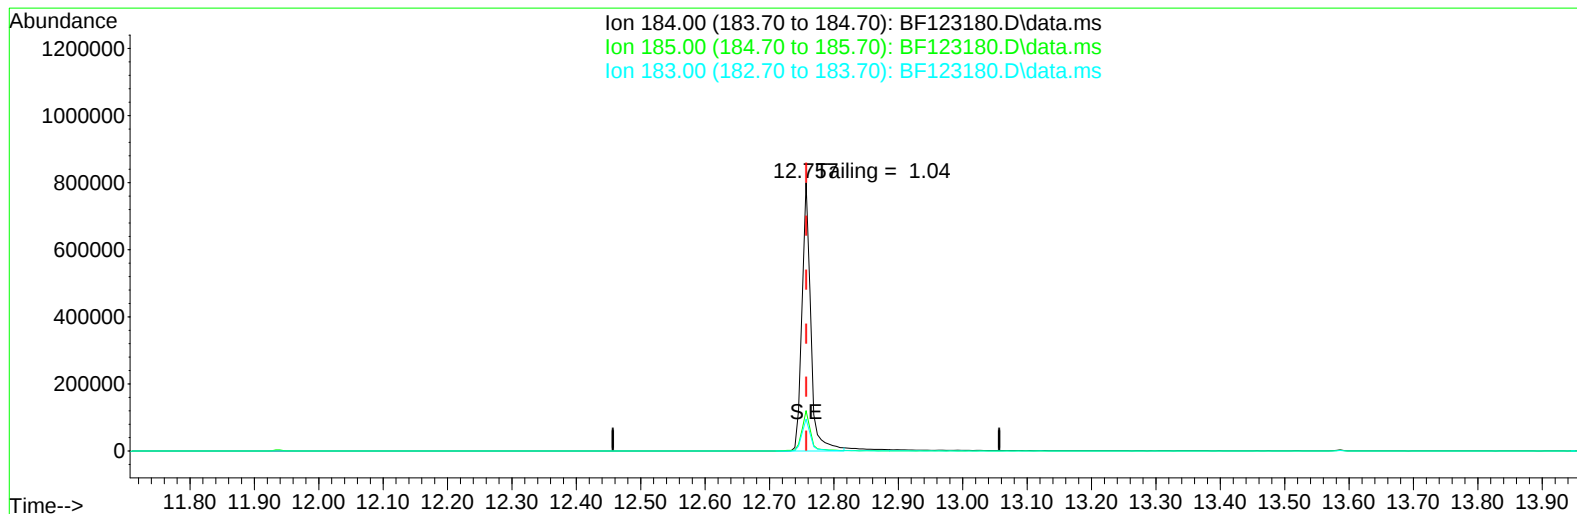

TIC: BF123180.D\data.ms

(77) Benzidine




12.757min (-0.000) 0.00 ng

response **801090**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.06
183.00	12.10	11.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021121\
 Data File : BF123180.D
 Acq On : 11 Feb 2021 11:43
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 14:03:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 11 13:57:30 2021
 Response via : Initial Calibration

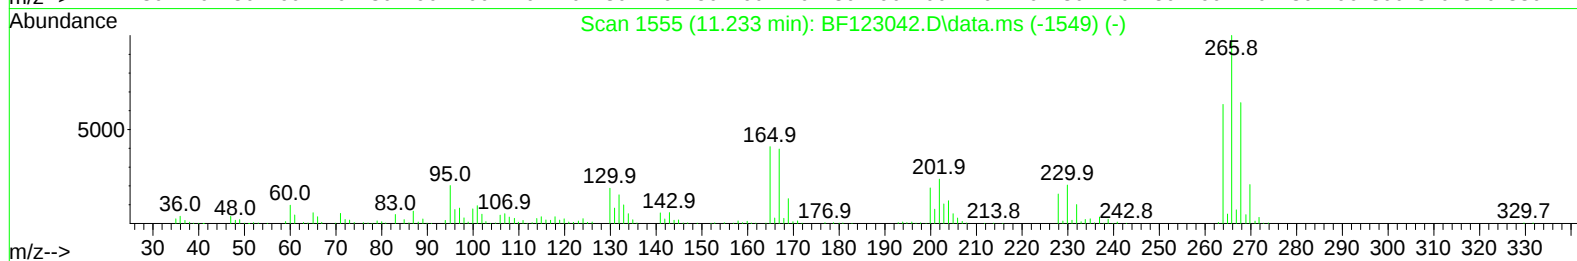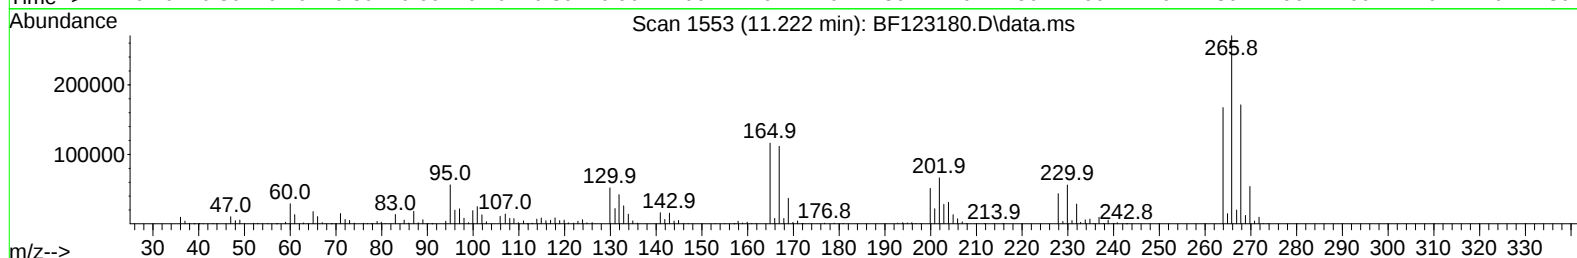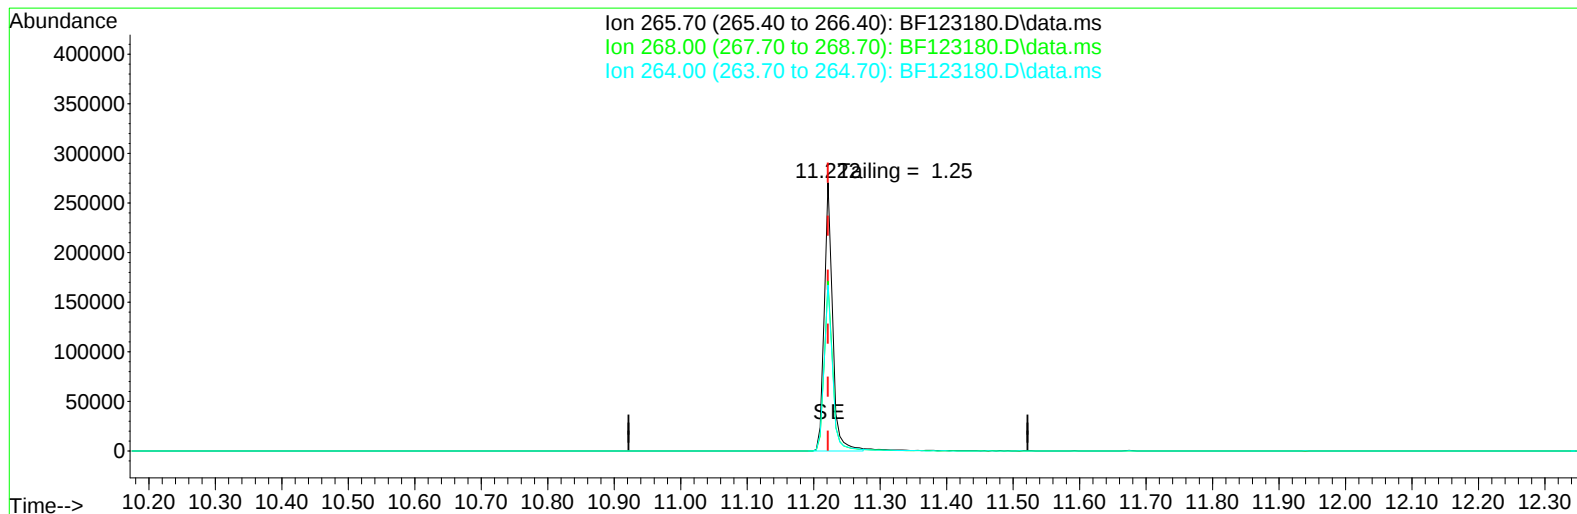

TIC: BF123180.D\data.ms

(70) Pentachlorophenol (C)

11.222min (-0.000) 38037.38 ng

response 242173

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.25
264.00	62.30	61.80
0.00	0.00	0.00