
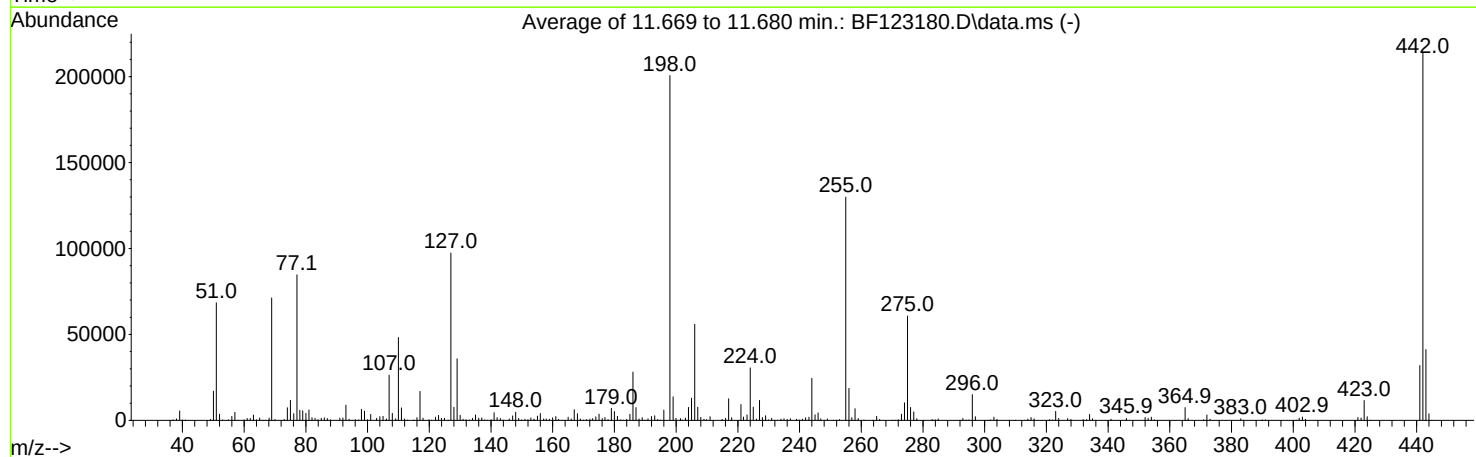


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021121\
 Data File : BF123180.D
 Acq On : 11 Feb 2021 11:43
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 11 14:10:38 2021

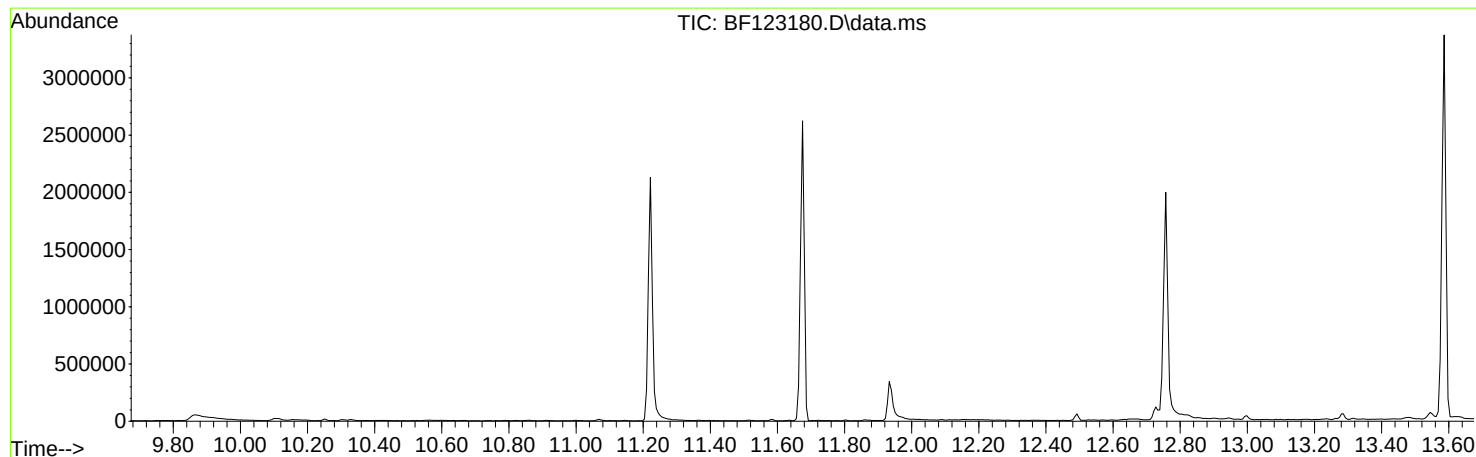

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	68472	PASS
68	69	0.00	2	1.9	1343	PASS
69	198	0.00	100	35.5	71179	PASS
70	69	0.00	2	0.8	556	PASS
127	198	10	80	48.5	97355	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	200597	PASS
199	198	5	9	6.8	13724	PASS
275	198	10	60	30.3	60704	PASS
365	198	1	100	3.7	7443	PASS
441	198	0.01	100	15.9	31917	PASS
442	442	50	100	100.0	214040	PASS
443	442	15	24	19.3	41232	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/11/2021	BNA_F	<u>BF123180.D</u>
Compound Name	Response	Retention Time
DDT	559476	13.58
DDD	10314	13.28
DDE	1643	12.94
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11957	571433	2.09

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021121\
 Data File : BF123180.D
 Acq On : 11 Feb 2021 11:43
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 11 14:03:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 11 13:57:30 2021
 Response via : Initial Calibration

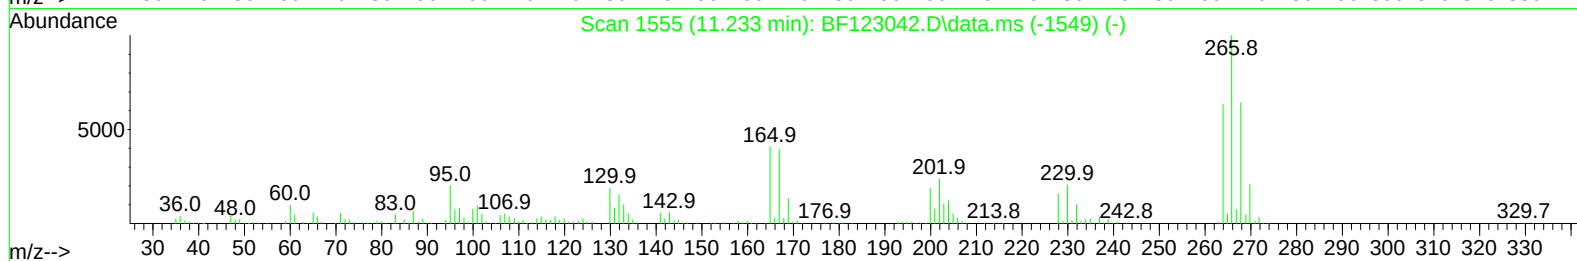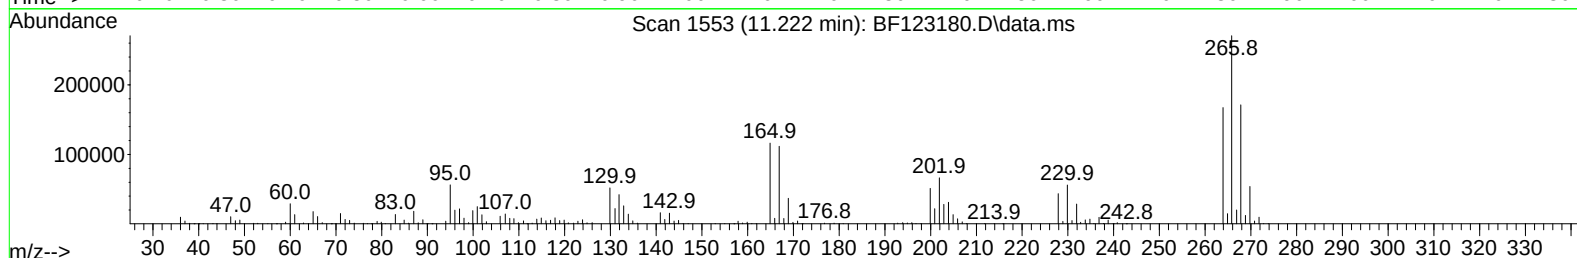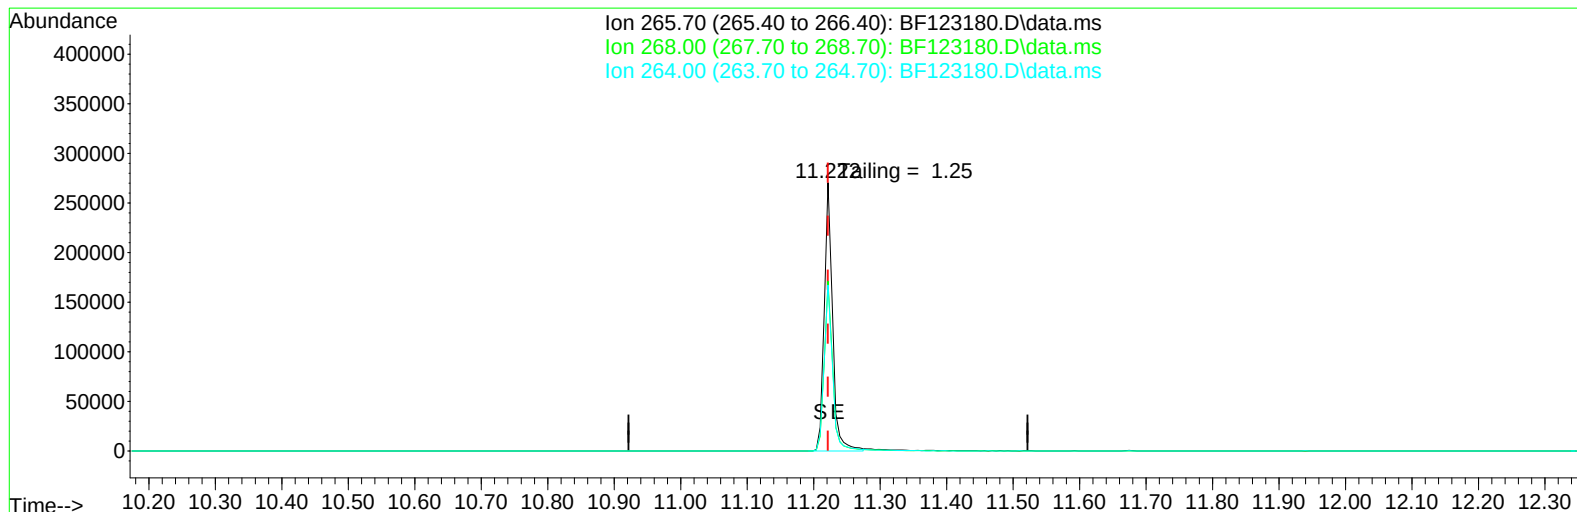

TIC: BF123180.D\data.ms

(70) Pentachlorophenol (C)

11.222min (-0.000) 38037.38 ng

response 242173

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.25
264.00	62.30	61.80
0.00	0.00	0.00

