
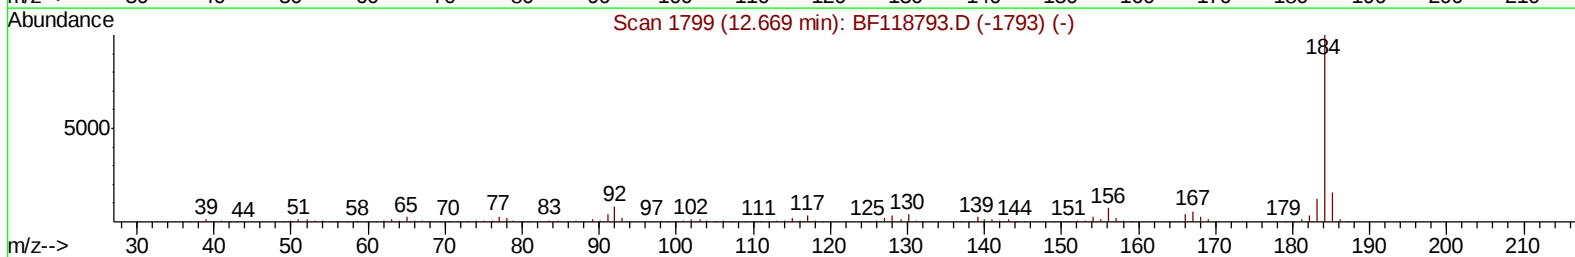
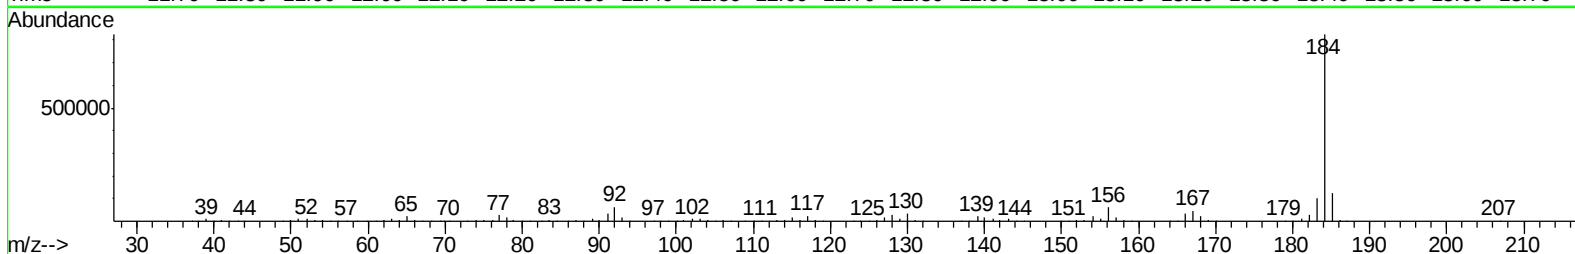


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF021320\
 Data File : BF118916.D
 Acq On : 13 Feb 2020 11:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 02:40:35 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF020320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 14 00:49:42 2020
 Response via : Initial Calibration

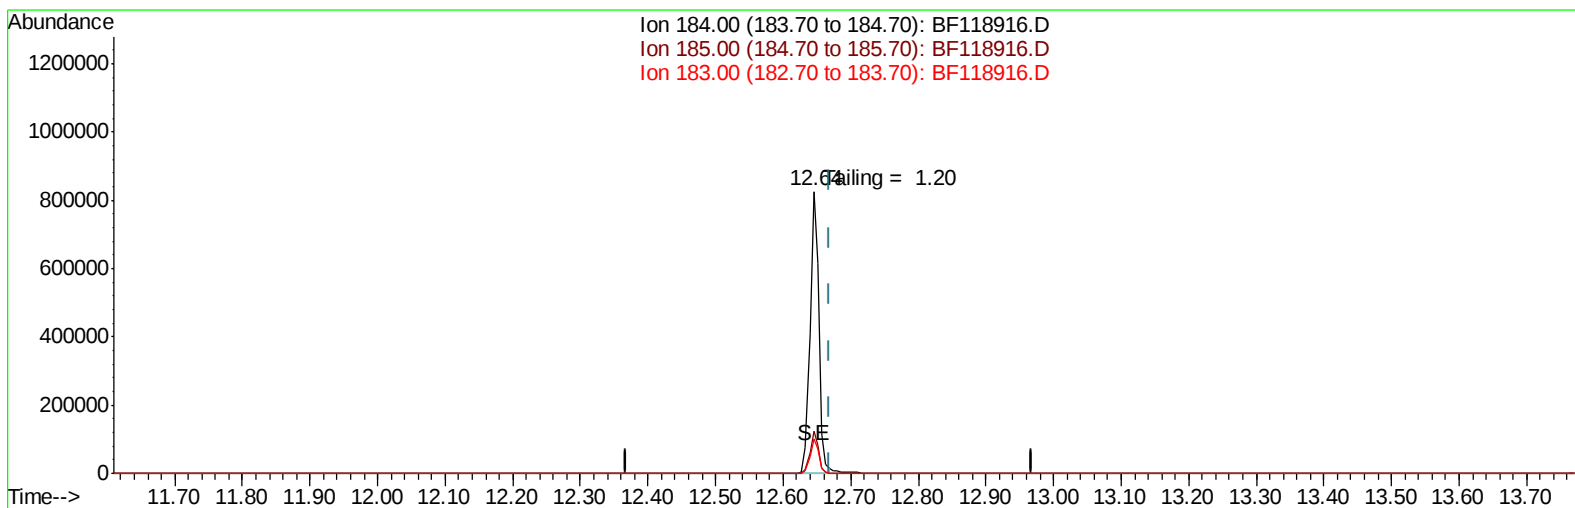

TIC: BF118916.D

(77) Benzidine




12.645min (-0.024) 0.00ng

response 752105

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	15.09
183.00	12.10	12.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF021320\
Data File : BF118916.D
Acq On : 13 Feb 2020 11:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 02:40:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF020320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 14 00:49:42 2020
Response via : Initial Calibration

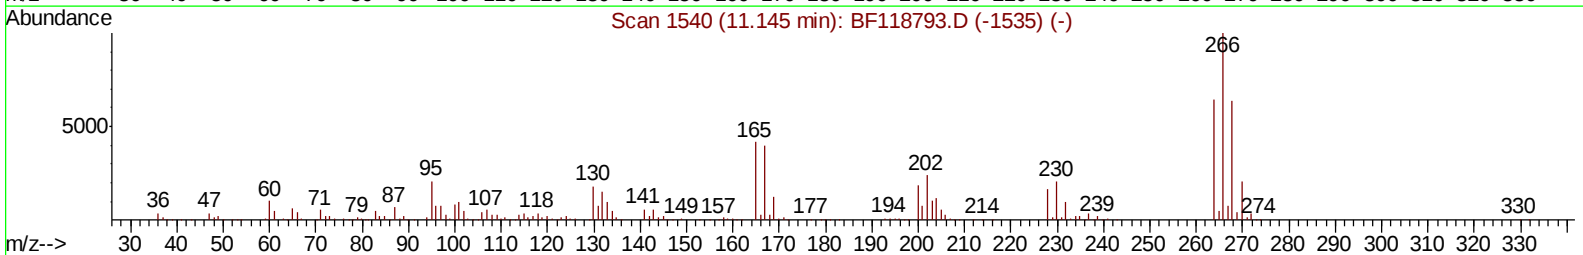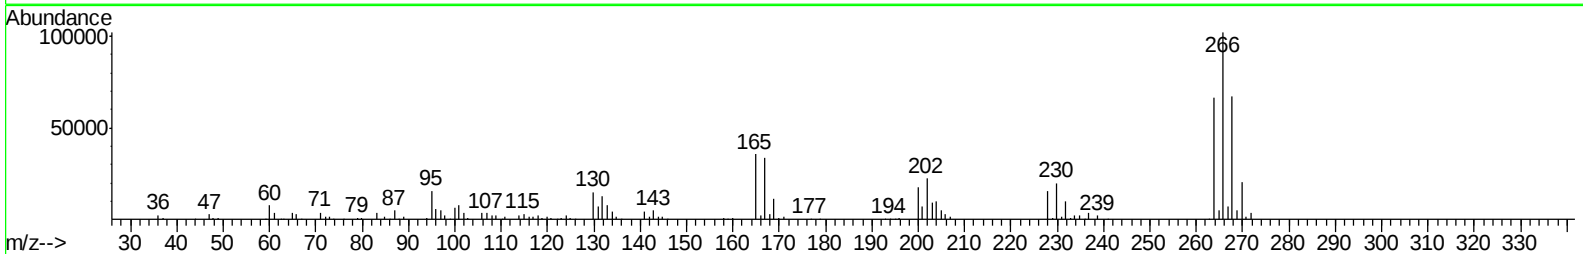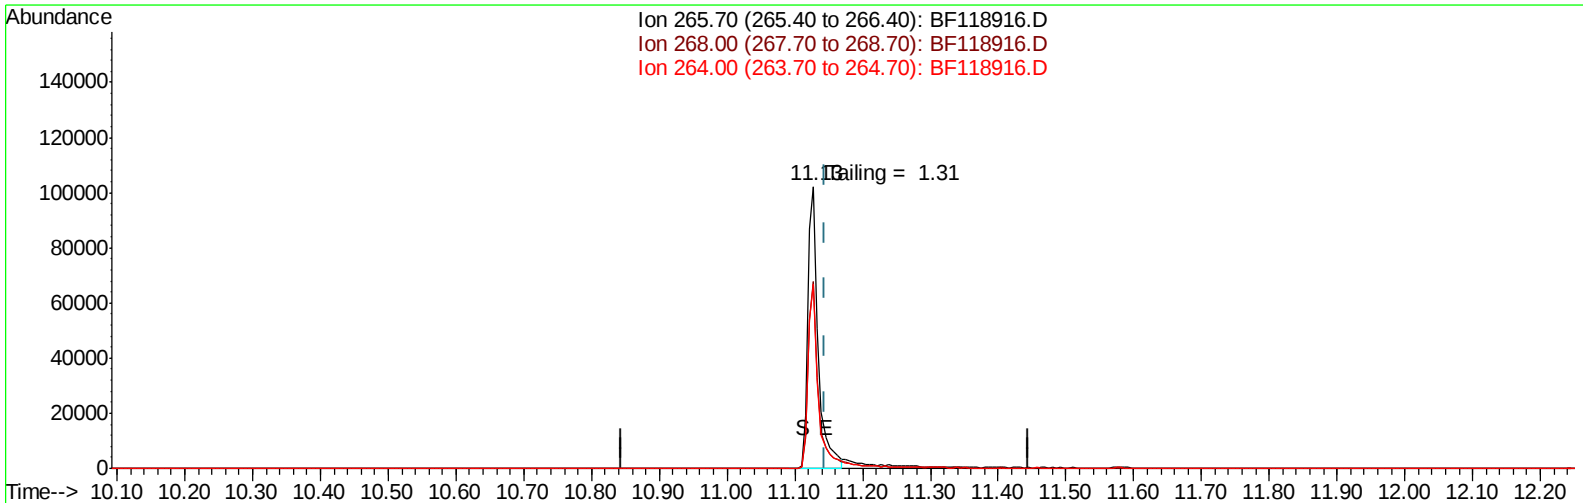

TIC: BF118916.D

(70) Pentachlorophenol (C)

11.127min (-0.018) 24453.77ng

response 118783

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	66.22
264.00	64.30	65.31
0.00	0.00	0.00