


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021320\
 Data File : BF118916.D
 Acq On : 13 Feb 2020 11:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF020320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 14 00:49:42 2020

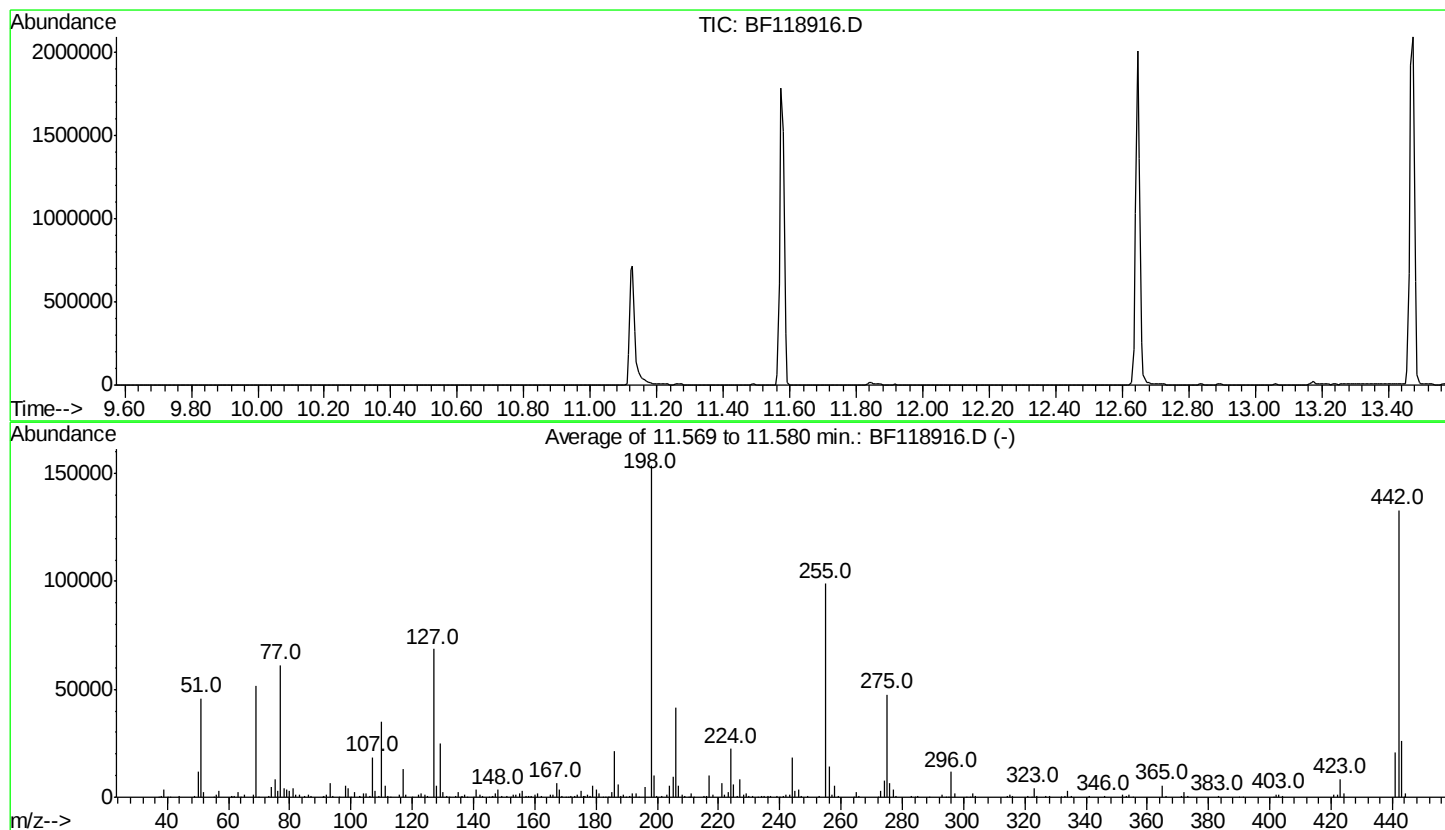

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.9	45880	PASS
68	69	0.00	2	2.0	1036	PASS
69	198	0.00	100	33.4	51336	PASS
70	69	0.00	2	0.5	265	PASS
127	198	10	80	44.7	68685	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	153632	PASS
199	198	5	9	6.7	10352	PASS
275	198	10	60	31.0	47650	PASS
365	198	1	100	3.6	5491	PASS
441	198	0.01	100	13.5	20740	PASS
442	198	50	100	86.7	133157	PASS
443	442	15	24	19.5	26032	PASS