
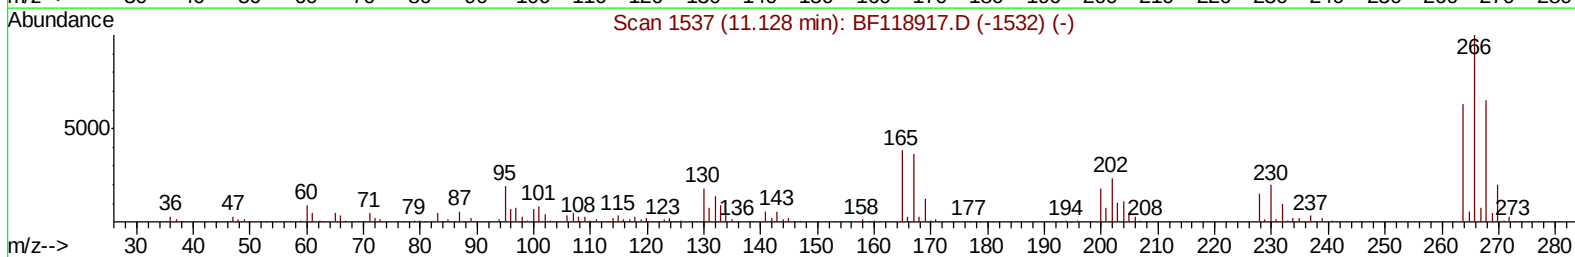
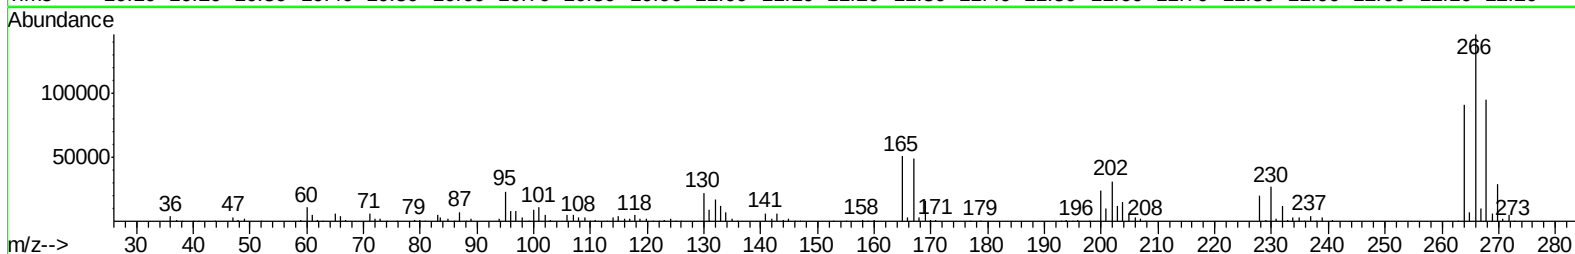


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF021420\
 Data File : BF118931.D
 Acq On : 14 Feb 2020 13:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 17 00:46:29 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF020320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 15 03:51:59 2020
 Response via : Initial Calibration

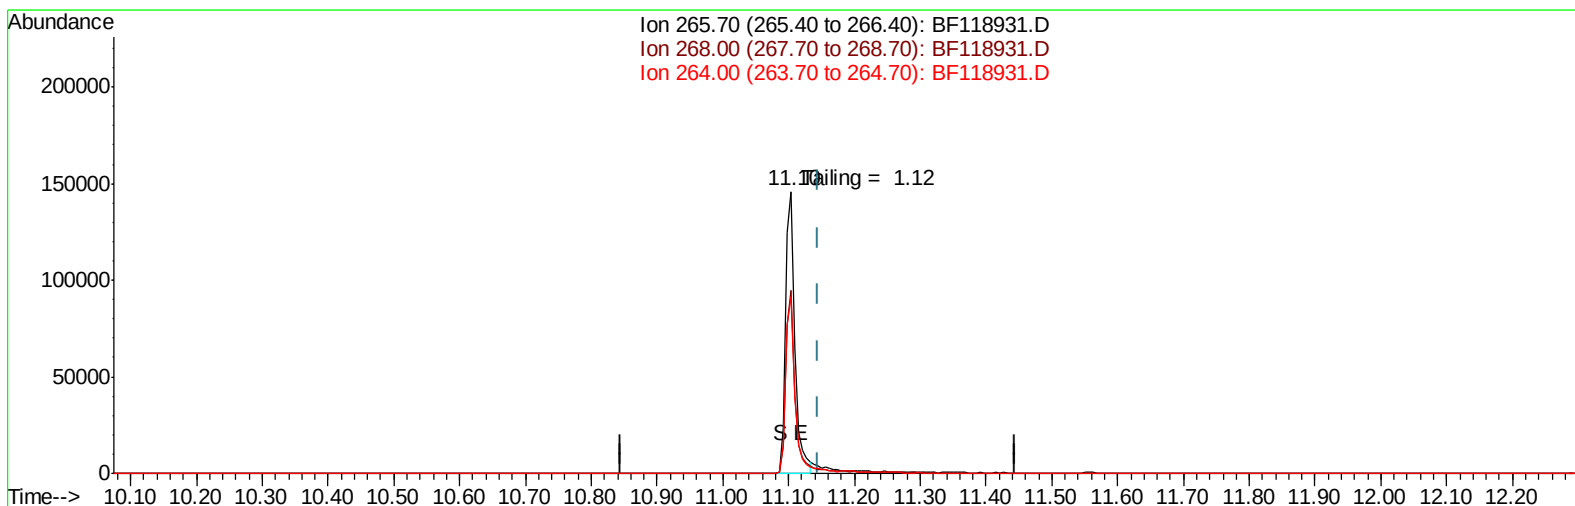

TIC: BF118931.D

(70) Pentachlorophenol (C)




11.104min (-0.041) 28206.65ng

response 157827

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	65.03
264.00	64.30	62.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF021420\
 Data File : BF118931.D
 Acq On : 14 Feb 2020 13:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 17 00:46:29 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF020320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 15 03:51:59 2020
 Response via : Initial Calibration

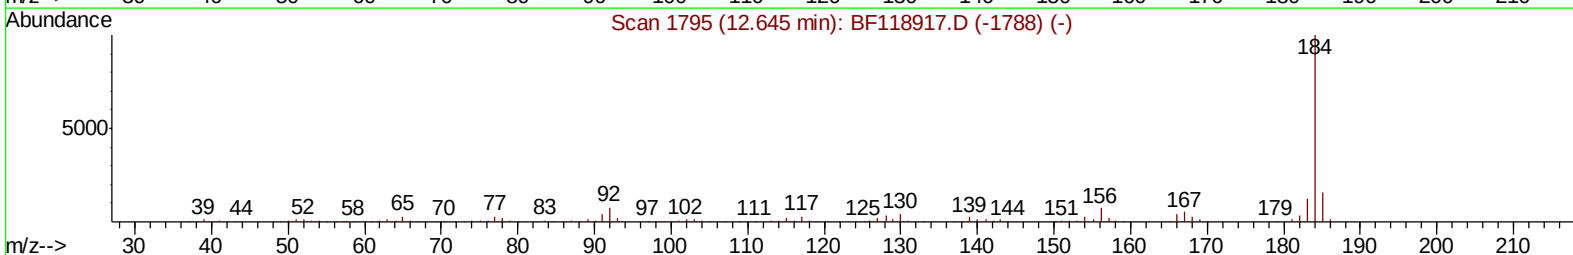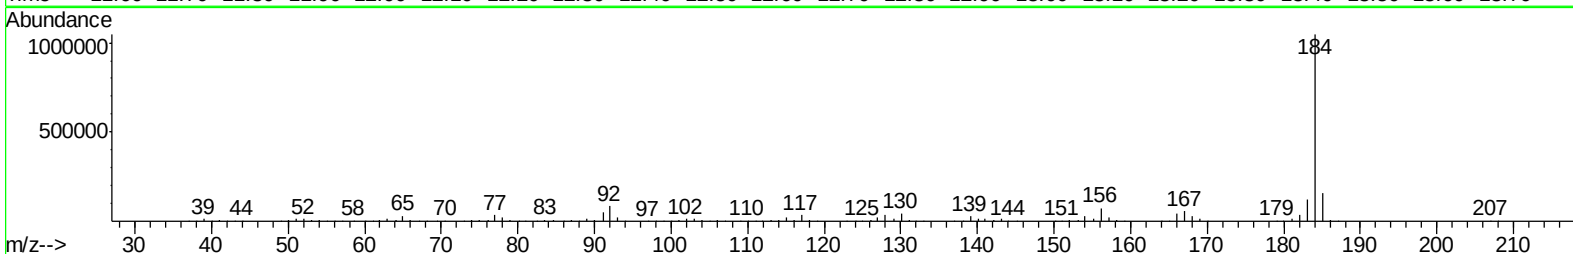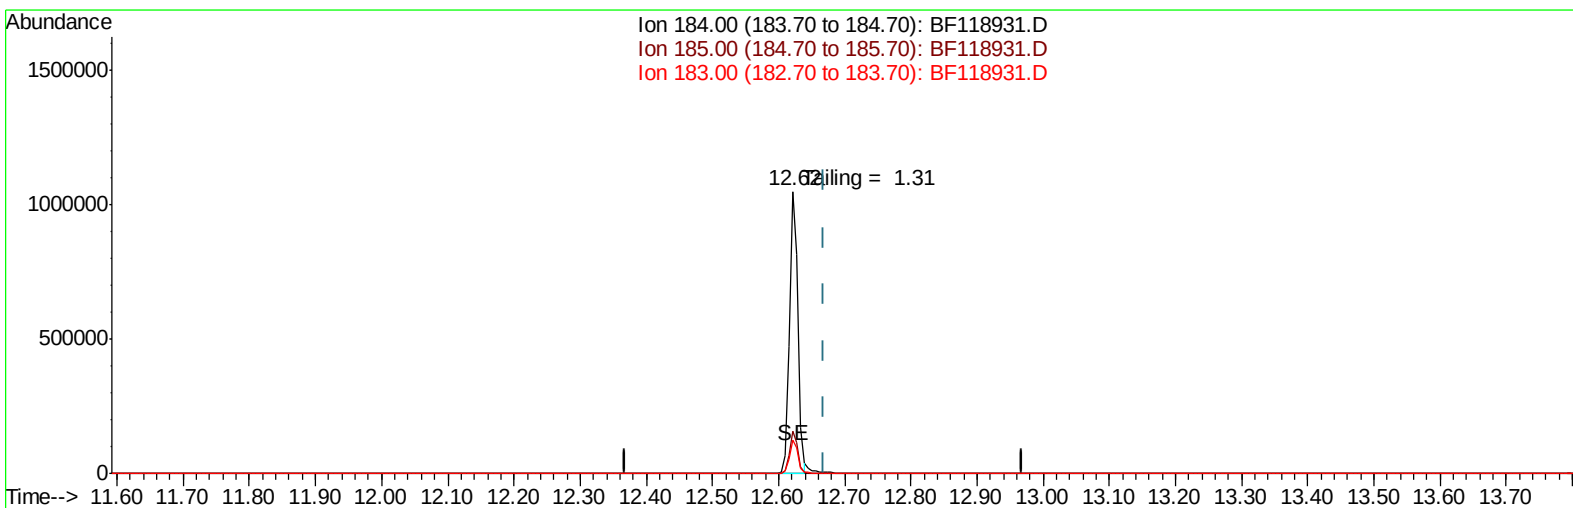

TIC: BF118931.D

(77) Benzidine

12.621min (-0.047) 0.00ng

response 950002

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	15.19
183.00	12.10	12.01
0.00	0.00	0.00