

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF021420\
 Data File : BF118935.D
 Acq On : 14 Feb 2020 16:50
 Operator : CG/JU
 Sample : PB126820BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB126820BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF020320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.981	490	492	498	rVB	74477	86226	1.43%	0.243%
2	5.398	559	563	581	rBV	2621791	2577576	42.63%	7.252%
3	6.410	731	735	749	rBV	1589659	1383414	22.88%	3.892%
4	6.775	793	797	801	rBV	1158667	931077	15.40%	2.619%
5	6.934	819	824	827	rBV	4013013	3670856	60.71%	10.328%
6	7.339	887	893	896	rBV	2971435	2898414	47.94%	8.154%
7	8.057	1011	1015	1021	rBV	1431138	1215662	20.11%	3.420%
8	9.133	1193	1198	1201	rBV	5961513	5627308	93.07%	15.832%
9	9.810	1306	1313	1316	rBV	1671457	1505511	24.90%	4.236%
10	10.245	1380	1387	1390	rBV	93243	79354	1.31%	0.223%
11	10.598	1442	1447	1450	rBV	4051113	3790944	62.70%	10.665%
12	10.716	1464	1467	1476	rVB	106235	112501	1.86%	0.317%
13	11.163	1540	1543	1546	rBV2	81592	68633	1.14%	0.193%
14	11.292	1561	1565	1568	rBV	1787171	1553430	25.69%	4.370%
15	12.392	1746	1752	1755	rBV3	91303	114917	1.90%	0.323%
16	12.880	1829	1835	1838	rBV	5787265	6046533	100.00%	17.011%
17	13.927	2009	2013	2021	rVB	2202636	1997053	33.03%	5.619%
18	14.698	2140	2144	2149	rVB	82798	81116	1.34%	0.228%
19	15.021	2195	2199	2204	rBV	87706	94678	1.57%	0.266%
20	15.356	2251	2256	2268	rBV	1355434	1709033	28.26%	4.808%


Sum of corrected areas: 35544236

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF021420\
Data File : BF118935.D
Acq On : 14 Feb 2020 16:50
Operator : CG/JU
Sample : PB126820BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB126820BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF020320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

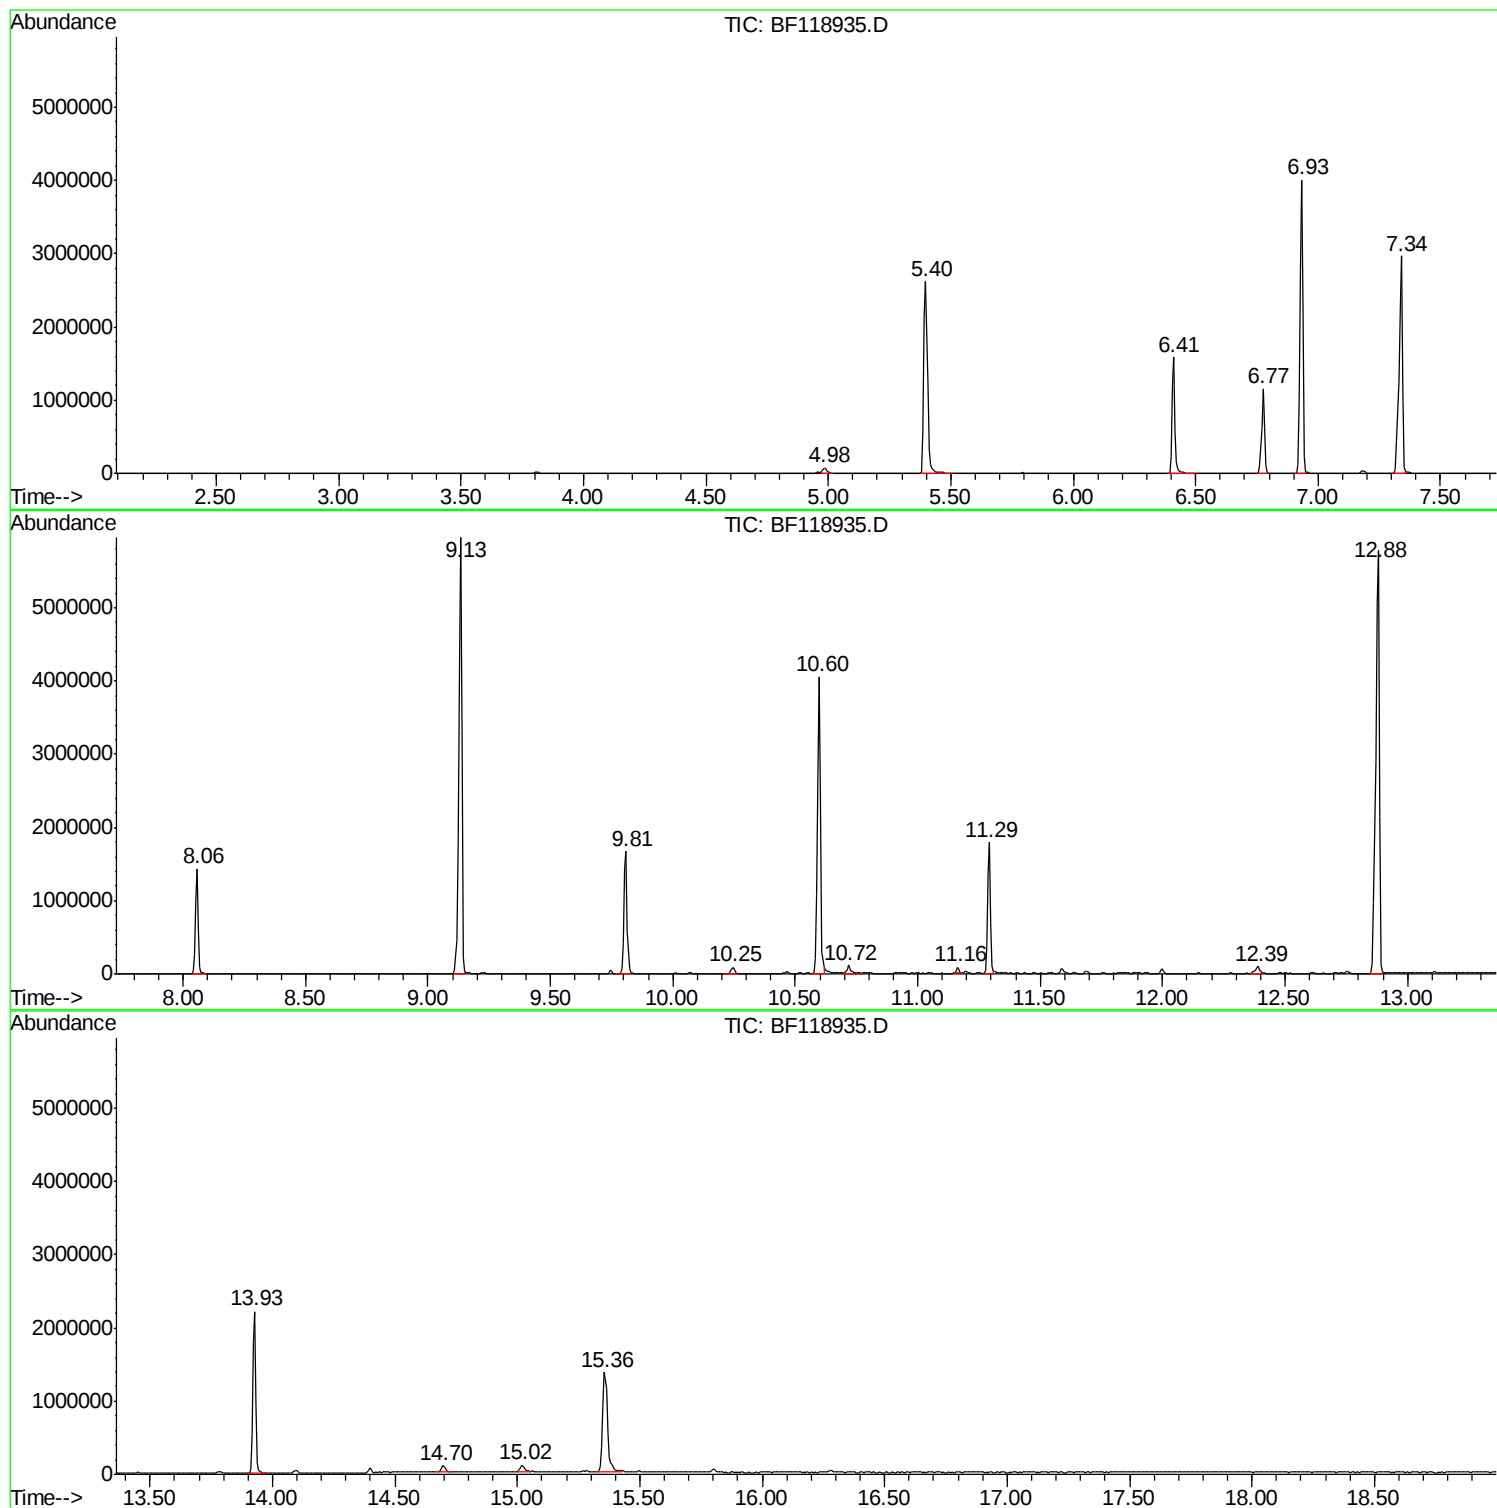

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF021420\
Data File : BF118935.D
Acq On : 14 Feb 2020 16:50
Operator : CG/JU
Sample : PB126820BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB126820BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF020320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF021420\
Data File : BF118935.D
Acq On : 14 Feb 2020 16:50
Operator : CG/JU
Sample : PB126820BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB126820BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF020320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc