


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021420\
 Data File : BF118931.D
 Acq On : 14 Feb 2020 13:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF020320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Feb 15 03:51:59 2020

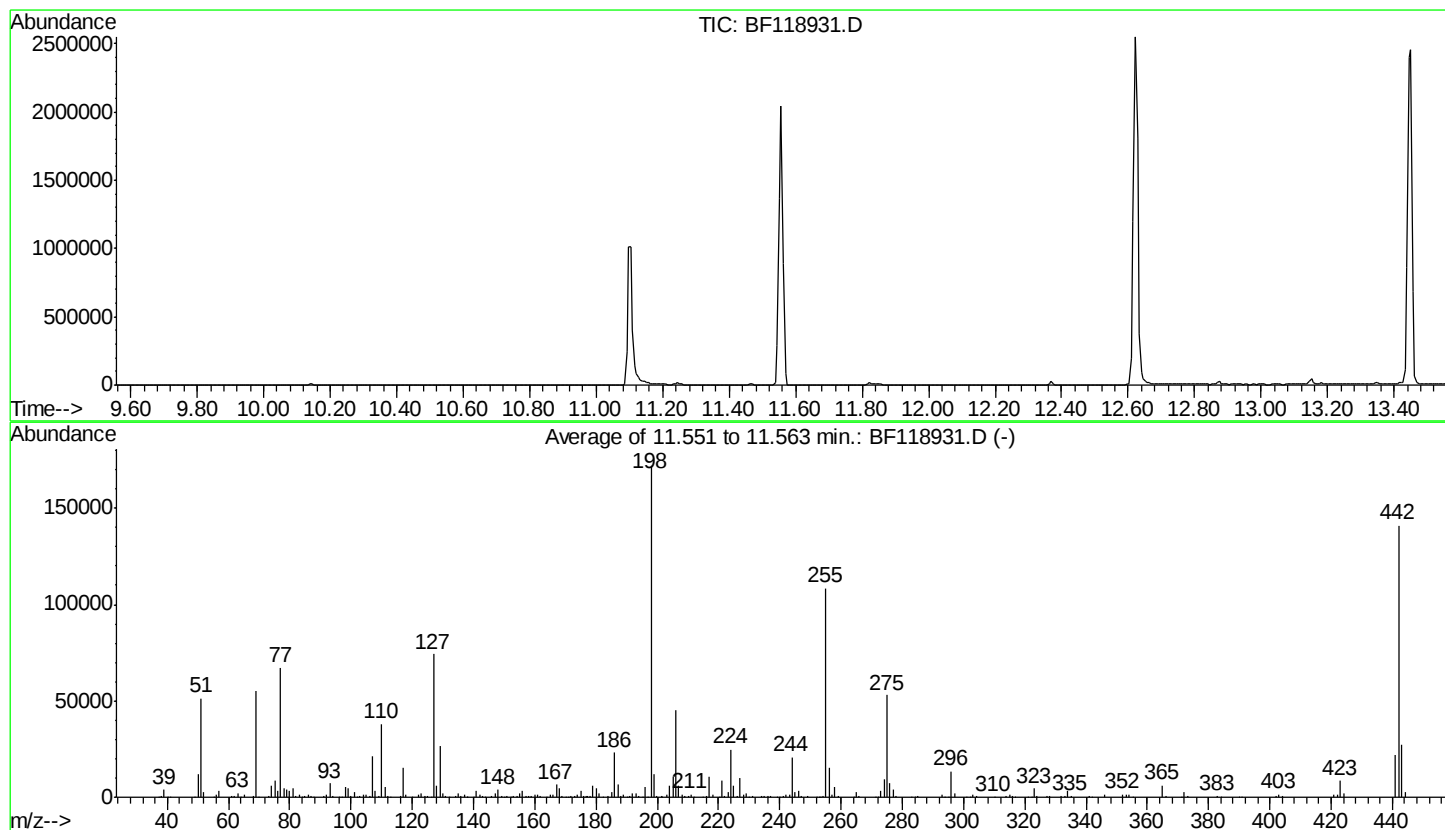

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.9	51424	PASS
68	69	0.00	2	1.6	902	PASS
69	198	0.00	100	32.0	55154	PASS
70	69	0.00	2	0.2	127	PASS
127	198	10	80	43.1	74208	PASS
197	198	0.00	2	0.1	195	PASS
198	198	100	100	100.0	172101	PASS
199	198	5	9	6.9	11840	PASS
275	198	10	60	30.7	52874	PASS
365	198	1	100	3.6	6150	PASS
441	198	0.01	100	12.6	21664	PASS
442	198	50	100	82.0	141082	PASS
443	442	15	24	19.1	26936	PASS