

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF021519\
 Data File : BF112580.D
 Acq On : 15 Feb 2019 15:54
 Operator : JU/SJ
 Sample : PB117127BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB117127BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.063	503	506	516	rBV	58434	80342	2.48%	0.353%
2	5.475	573	576	593	rBV	1729572	1788630	55.14%	7.864%
3	6.481	743	747	765	rBV	1765566	1906709	58.78%	8.383%
4	6.610	765	769	778	rVV	2335064	2059490	63.49%	9.055%
5	6.834	803	807	817	rBV	648250	651437	20.08%	2.864%
6	6.987	829	833	851	rBV	1715868	1632980	50.34%	7.180%
7	7.398	898	903	923	rBV	1066690	1257934	38.78%	5.531%
8	8.116	1020	1025	1041	rBV	821649	898716	27.71%	3.951%
9	9.192	1201	1208	1223	rBV	2592470	2801920	86.38%	12.319%
10	9.875	1318	1324	1337	rBV	1111129	1119225	34.50%	4.921%
11	10.669	1455	1459	1483	rBV	1819444	1818100	56.05%	7.993%
12	11.363	1573	1577	1598	rVB	1190780	1248003	38.47%	5.487%
13	12.945	1842	1846	1850	rBV	3276276	3243676	100.00%	14.261%
14	14.016	2024	2028	2036	rBV	1131624	1128409	34.79%	4.961%
15	14.451	2099	2102	2106	rVB2	37127	33636	1.04%	0.148%
16	14.757	2151	2154	2159	rVB2	41985	44778	1.38%	0.197%
17	15.092	2207	2211	2215	rVB2	51758	63869	1.97%	0.281%
18	15.463	2271	2274	2275	rBV	47909	47982	1.48%	0.211%
19	15.498	2275	2280	2289	rVB	584911	864531	26.65%	3.801%
20	15.892	2344	2347	2353	rVB	39669	54596	1.68%	0.240%


Sum of corrected areas: 22744963

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF021519\
Data File : BF112580.D
Acq On : 15 Feb 2019 15:54
Operator : JU/SJ
Sample : PB117127BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB117127BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

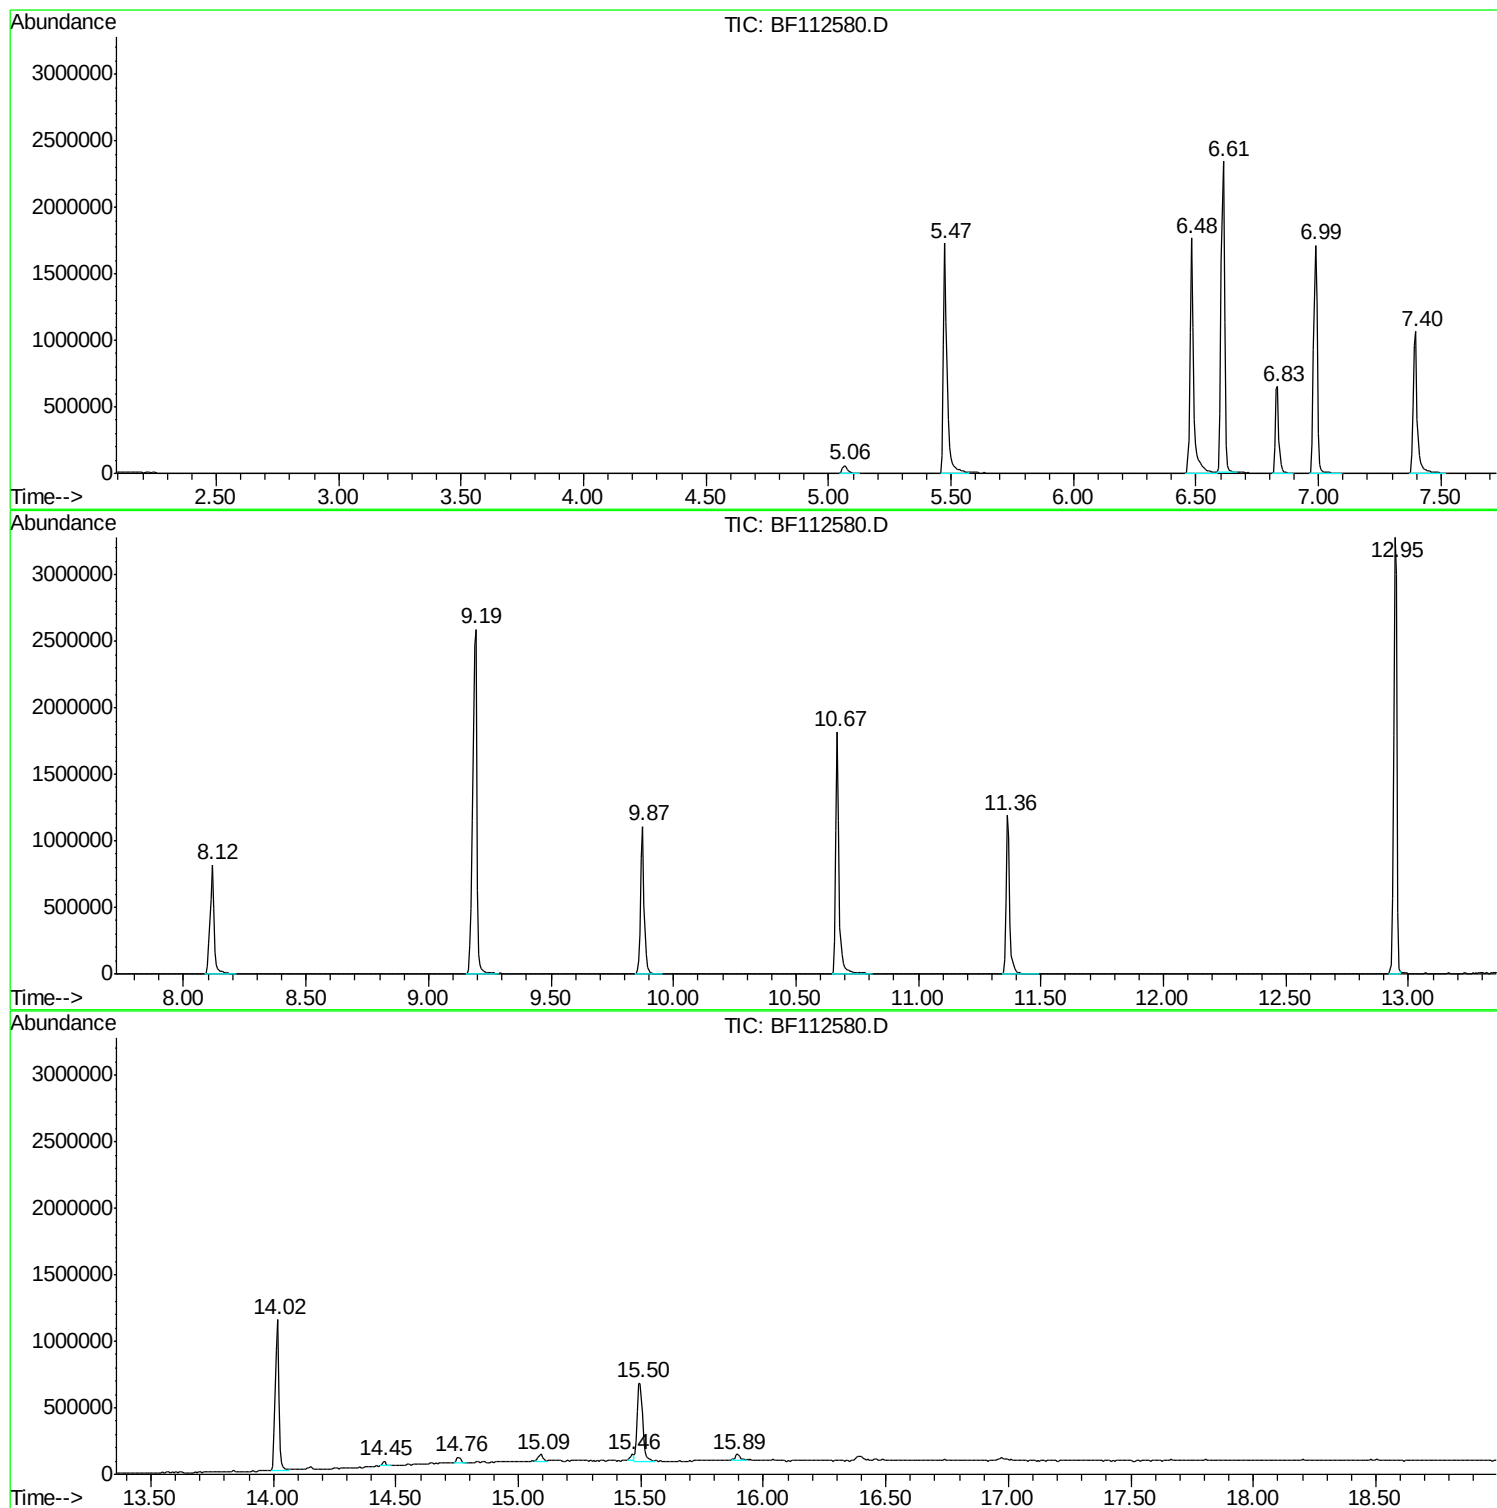

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF021519\
Data File : BF112580.D
Acq On : 15 Feb 2019 15:54
Operator : JU/SJ
Sample : PB117127BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB117127BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.06	2.47 ng	80342	1,4-Dichlorobenzene-d4	6.83

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	35
3			5-Hexen-2-one	98	C6H10O	000109-49-9	9
4			Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9
5			Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9

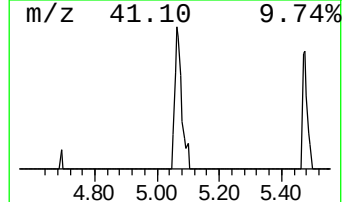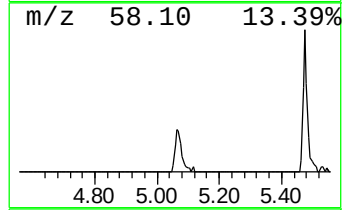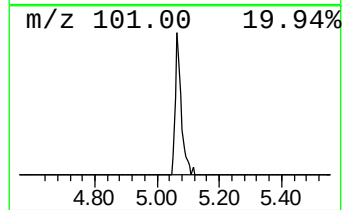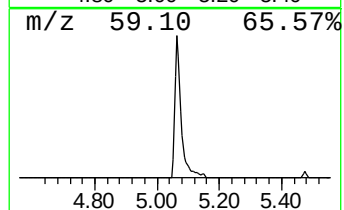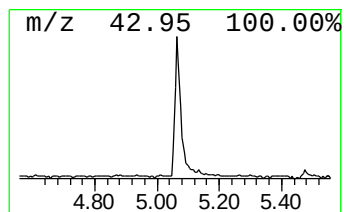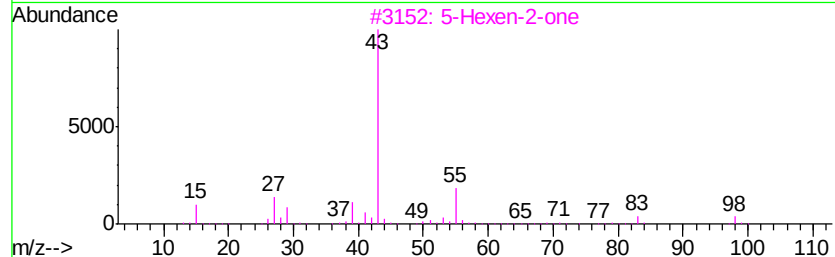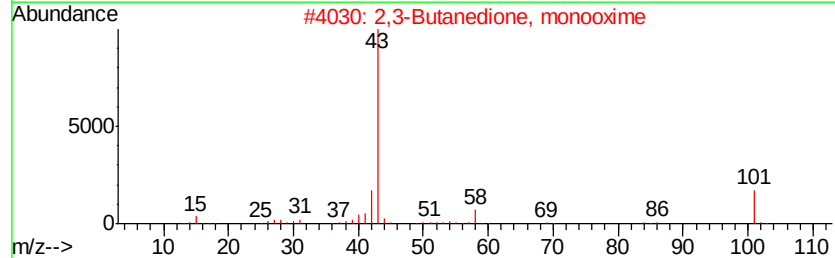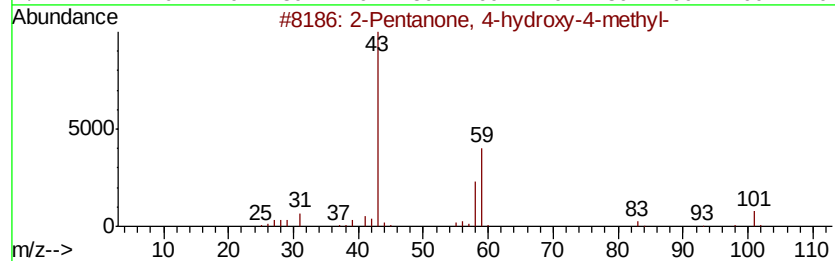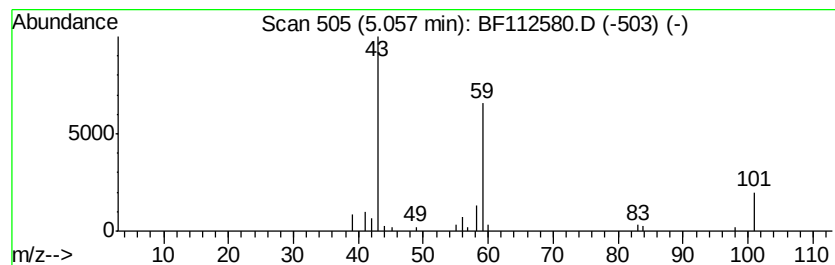

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF021519\
Data File : BF112580.D
Acq On : 15 Feb 2019 15:54
Operator : JU/SJ
Sample : PB117127BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB117127BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.61 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.61	63.23 ng	2059490	1,4-Dichlorobenzene-d4	6.83

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	12
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

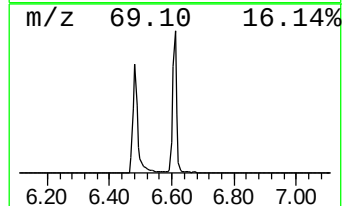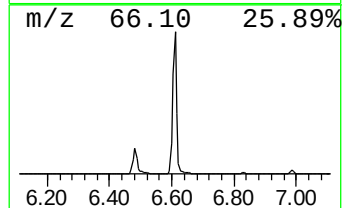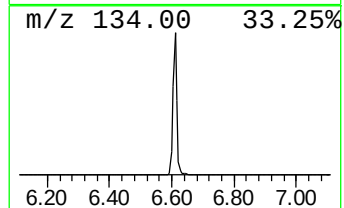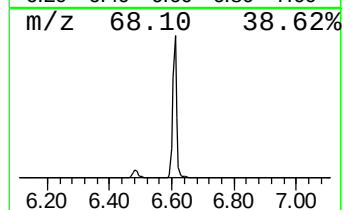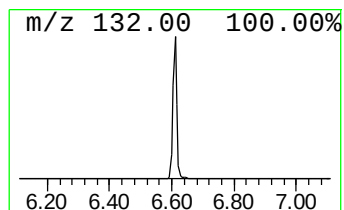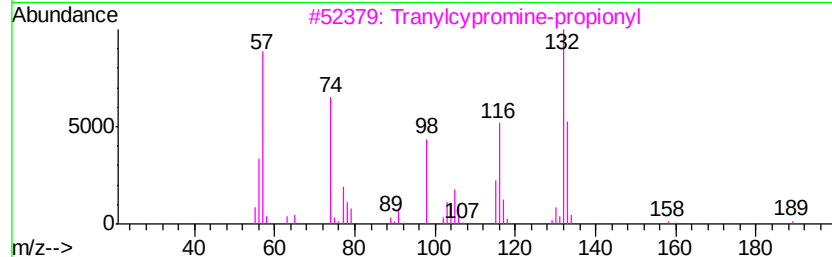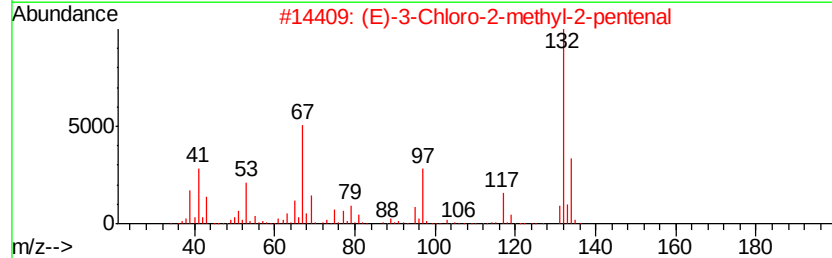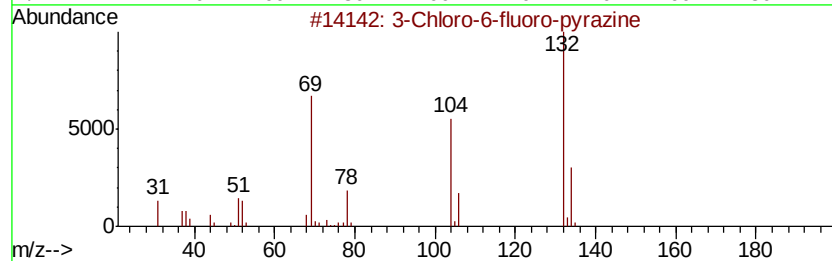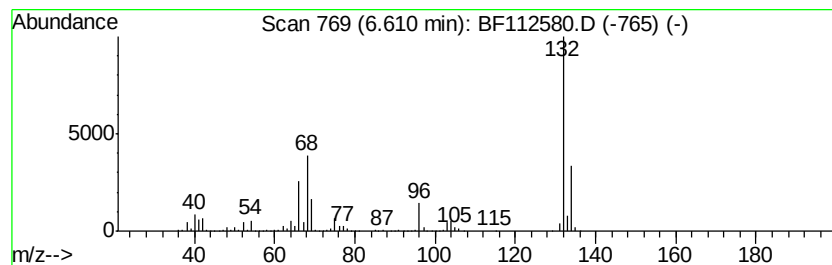

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF021519\
Data File : BF112580.D
Acq On : 15 Feb 2019 15:54
Operator : JU/SJ
Sample : PB117127BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB117127BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.06	2.5	ng	80342	1	6.83	651437	20.0
unknown6.61	6.61	63.2	ng	2059490	1	6.83	651437	20.0