
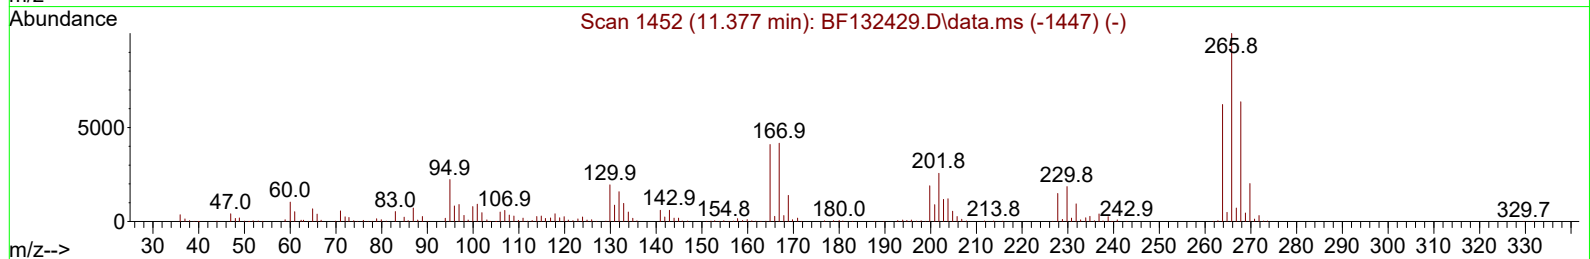
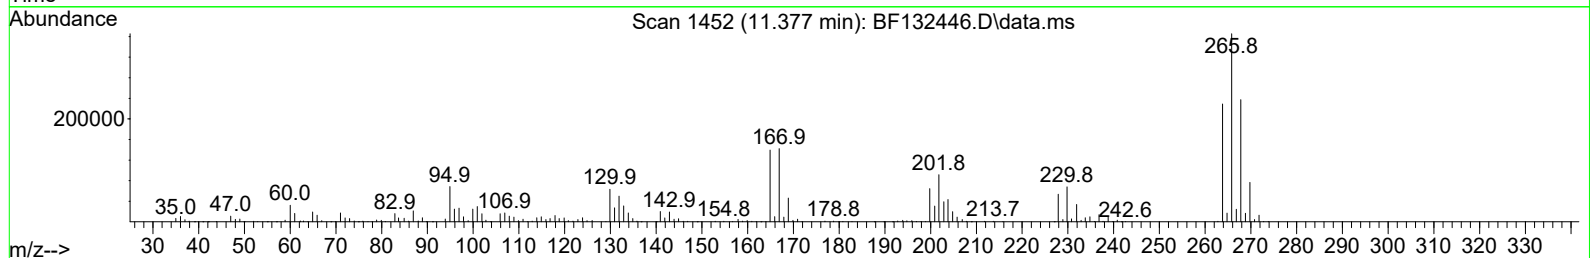


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021723\
Data File : BF132446.D
Acq On : 17 Feb 2023 09:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 04:54:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 18 00:58:25 2023
Response via : Initial Calibration

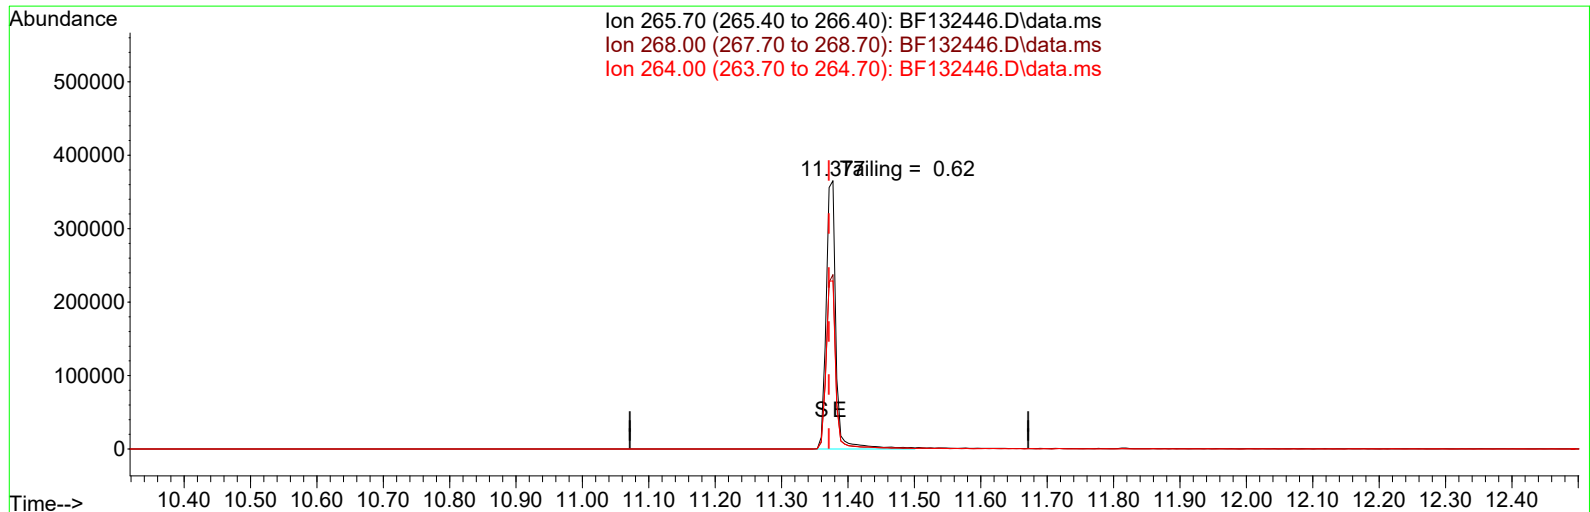

TIC: BF132446.D\data.ms

(70) Pentachlorophenol (C)




11.377min (+ 0.006) 764402.18 ng

response 375684

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.99
264.00	62.20	62.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021723\
 Data File : BF132446.D
 Acq On : 17 Feb 2023 09:35
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 04:54:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 18 00:58:25 2023
 Response via : Initial Calibration

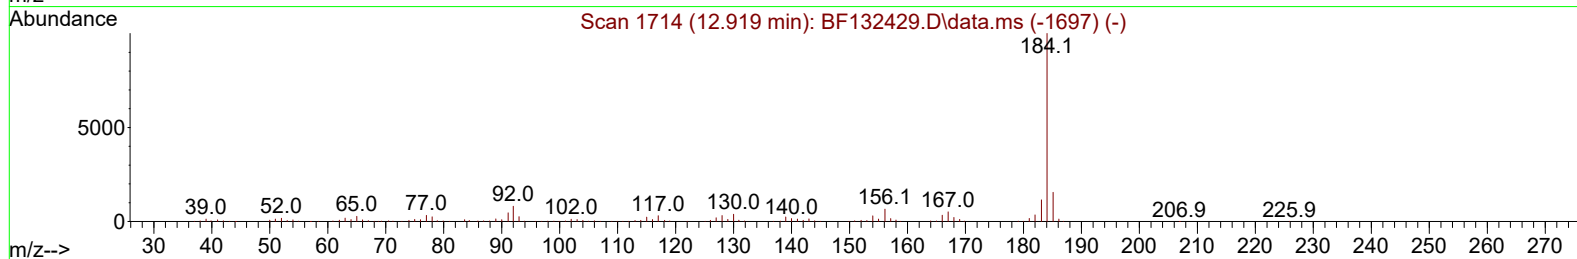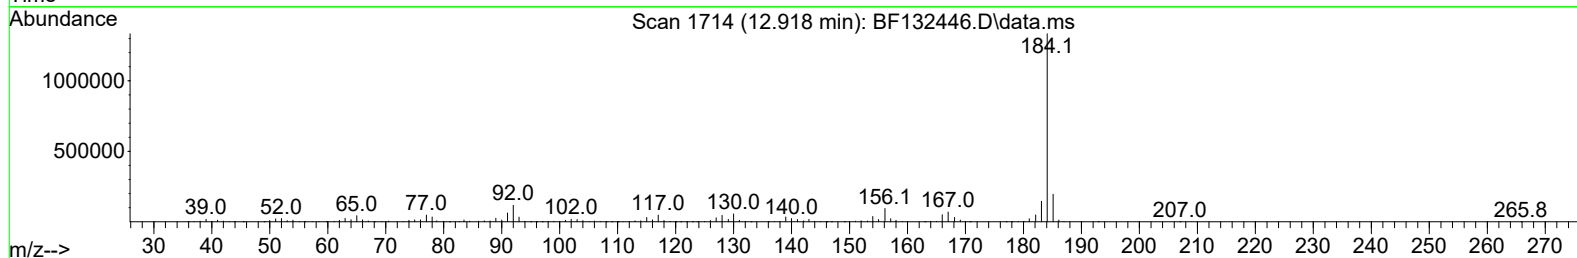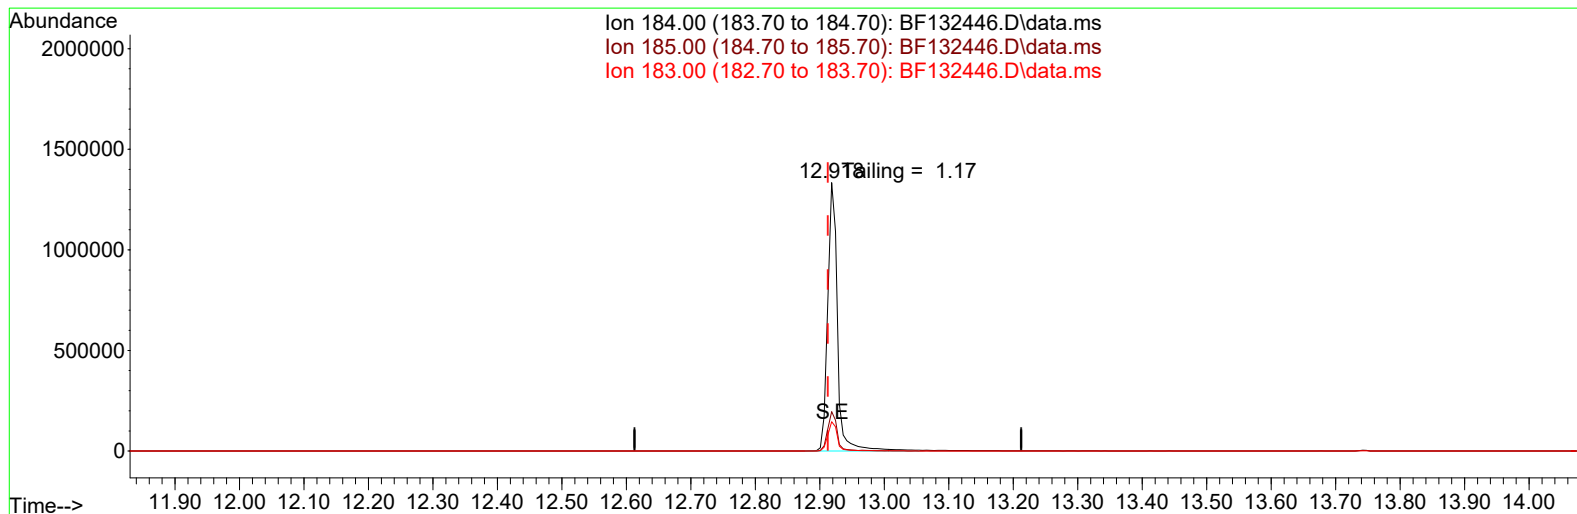

TIC: BF132446.D\data.ms

(77) Benzidine

12.918min (+ 0.006) 0.00 ng

response 1406642

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.69
183.00	11.50	10.94
0.00	0.00	0.00