
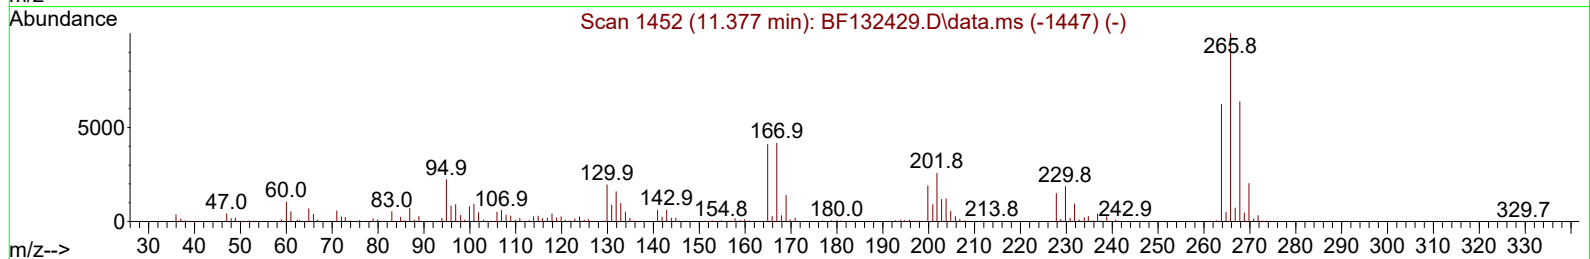
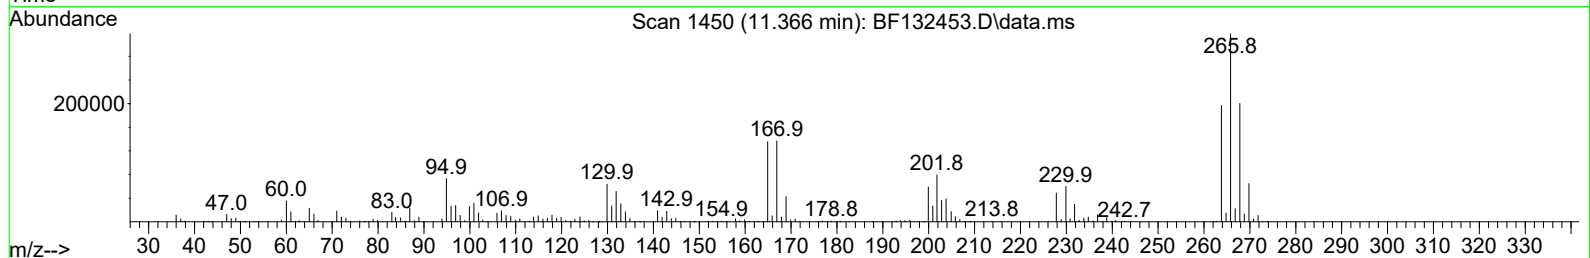


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021723\
Data File : BF132453.D
Acq On : 17 Feb 2023 16:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 04:55:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 18 00:58:25 2023
Response via : Initial Calibration

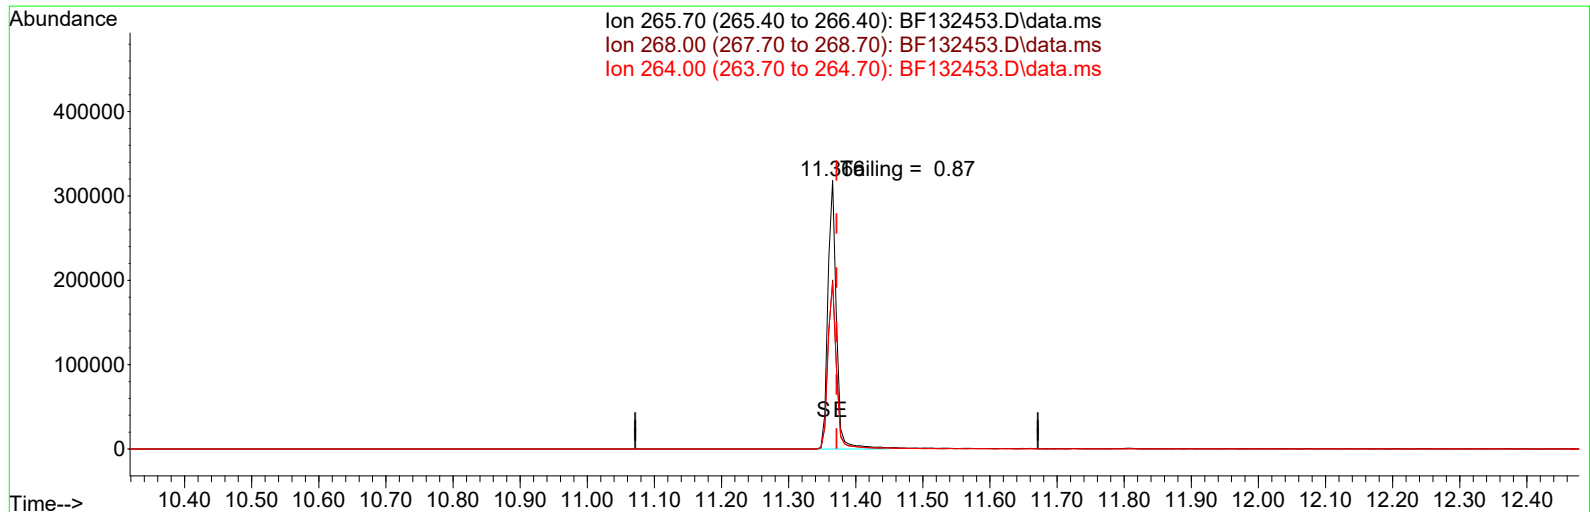

TIC: BF132453.D\data.ms

(70) Pentachlorophenol (C)




11.366min (-0.006) 387755.74 ng

response 284477

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.95
264.00	62.20	61.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021723\
Data File : BF132453.D
Acq On : 17 Feb 2023 16:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 04:55:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 18 00:58:25 2023
Response via : Initial Calibration

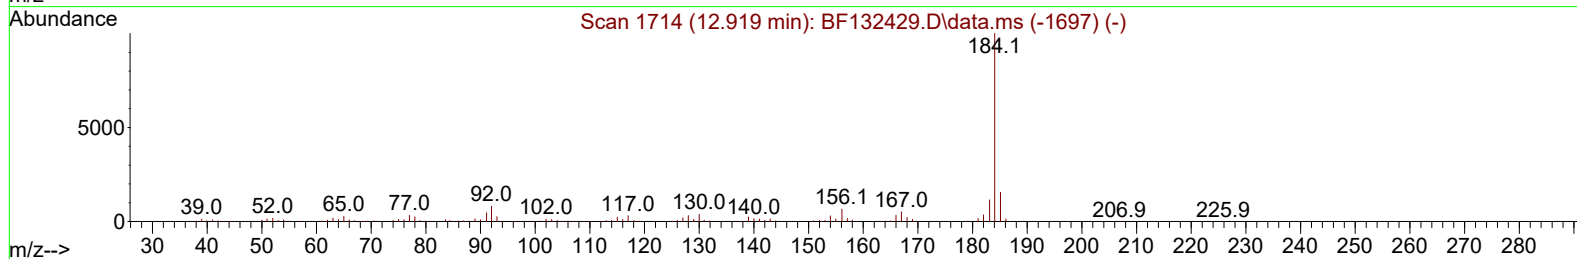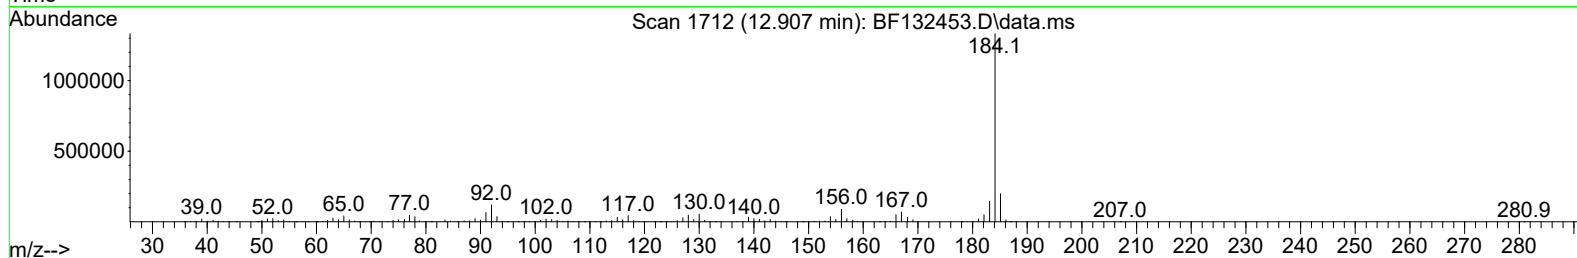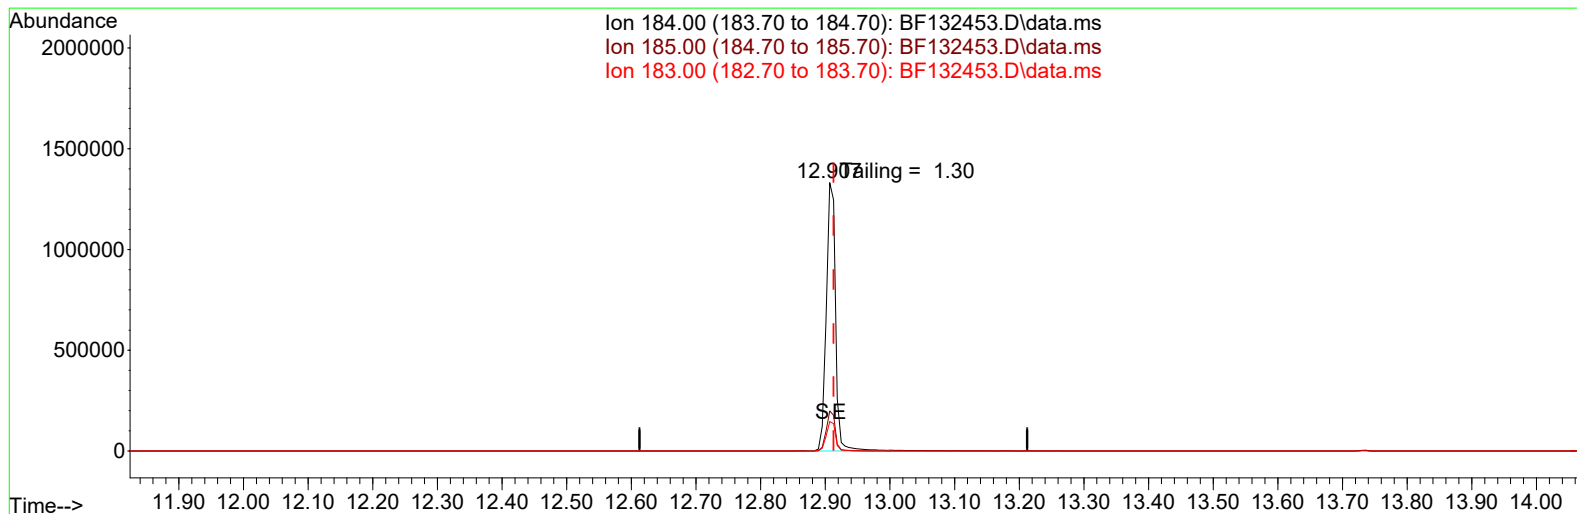

TIC: BF132453.D\data.ms

(77) Benzidine**12.907min (-0.006) 1162961.65 ng****response 1337251**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.93
183.00	11.50	11.01
0.00	0.00	0.00