


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021723\
Data File : BF132446.D
Acq On : 17 Feb 2023 09:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Feb 18 00:58:25 2023

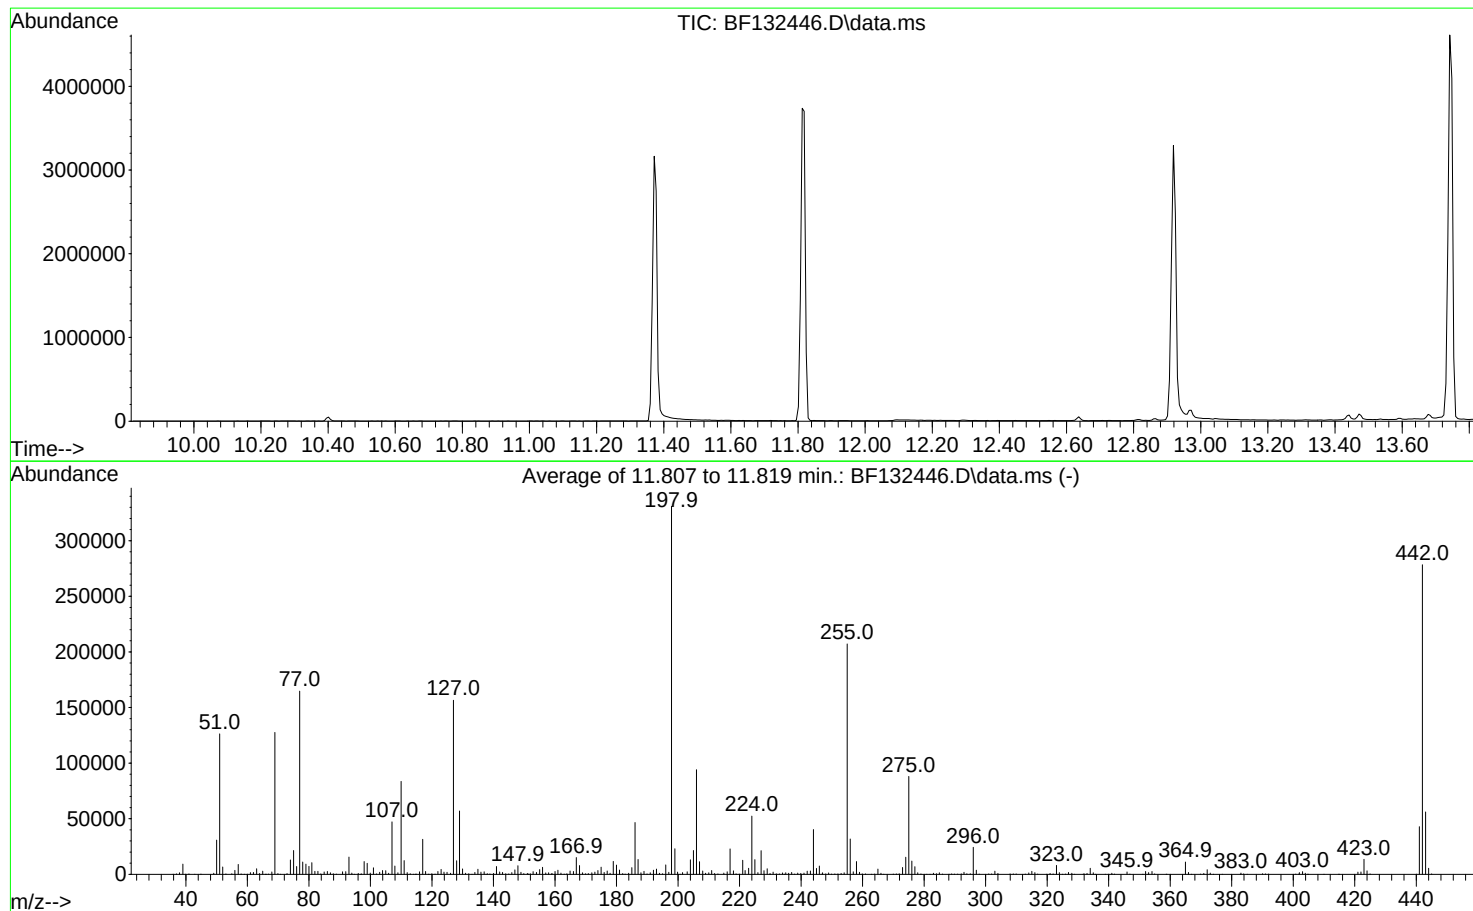




AutoFind: Scans 1525, 1526, 1527; Background Corrected with Scan 1520

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	126312	PASS
68	69	0.00	2	1.6	2039	PASS
69	198	0.00	100	38.5	127536	PASS
70	69	0.00	2	0.5	698	PASS
127	198	10	80	47.3	156440	PASS
197	198	0.00	2	0.6	1845	PASS
198	198	100	100	100.0	330837	PASS
199	198	5	9	6.9	22977	PASS
275	198	10	60	26.6	87995	PASS
365	198	1	100	3.3	10962	PASS
441	198	0.01	100	13.0	42881	PASS
442	442	50	100	100.0	278456	PASS
443	442	15	24	20.1	56019	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021723\
Data File : BF132446.D
Acq On : 17 Feb 2023 09:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 18 04:54:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 18 00:58:25 2023
Response via : Initial Calibration

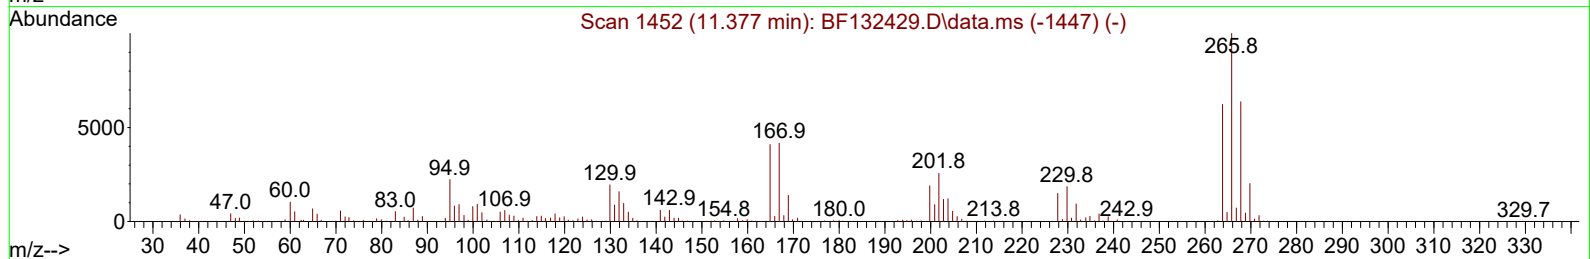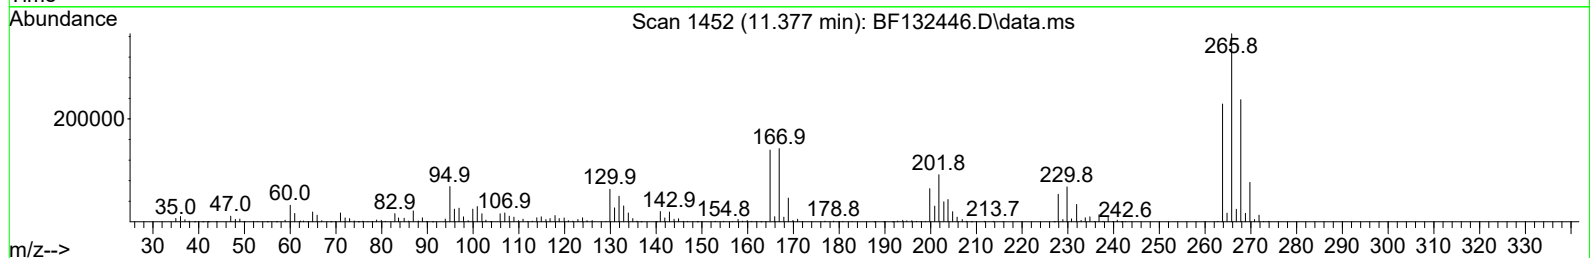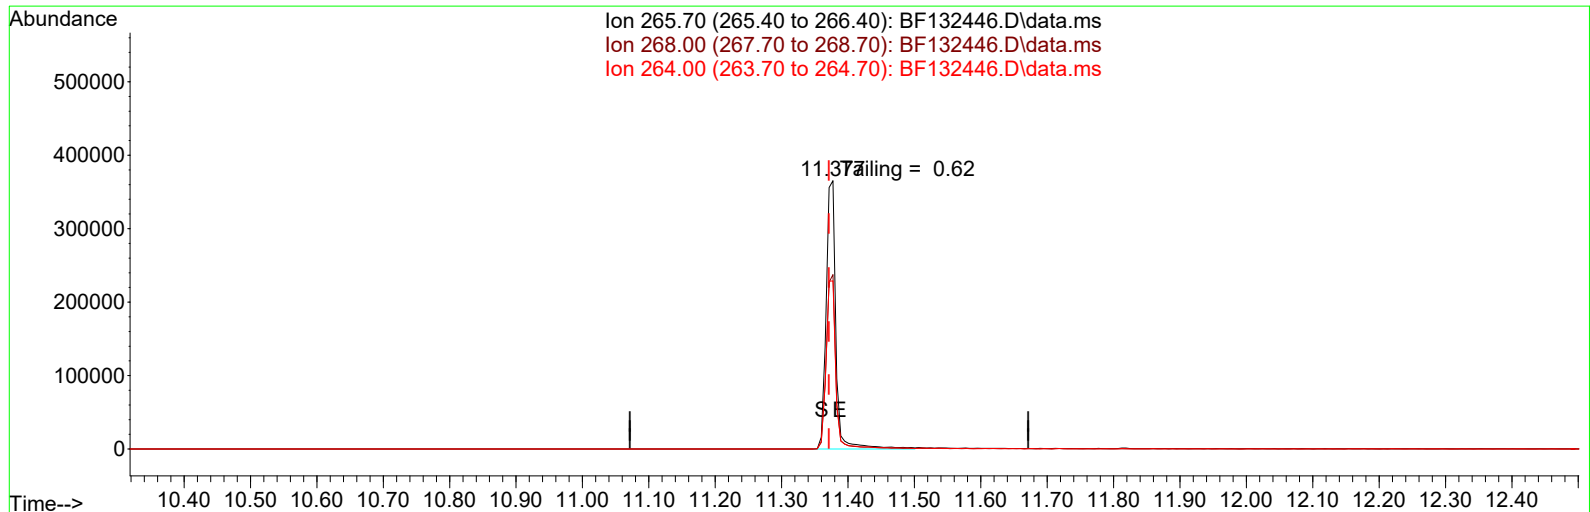

TIC: BF132446.D\data.ms

(70) Pentachlorophenol (C)

11.377min (+ 0.006) 764402.18 ng




response 375684

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.99
264.00	62.20	62.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021723\
 Data File : BF132446.D
 Acq On : 17 Feb 2023 09:35
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 18 04:54:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 18 00:58:25 2023
 Response via : Initial Calibration

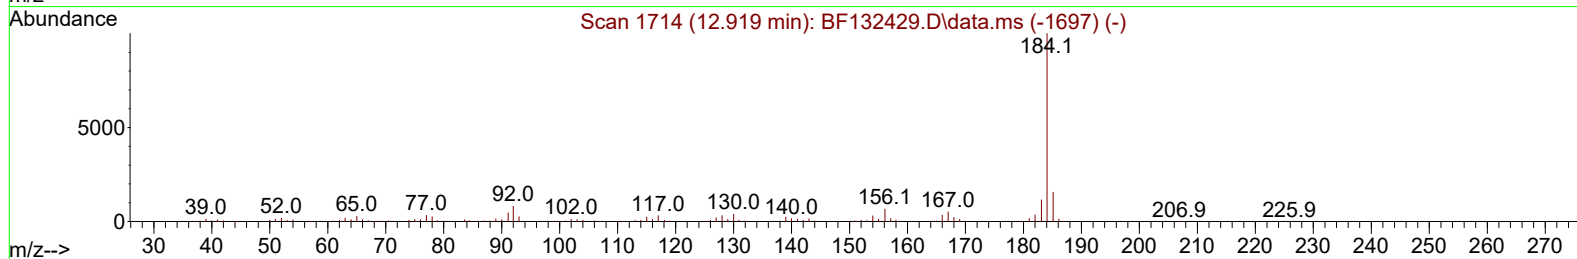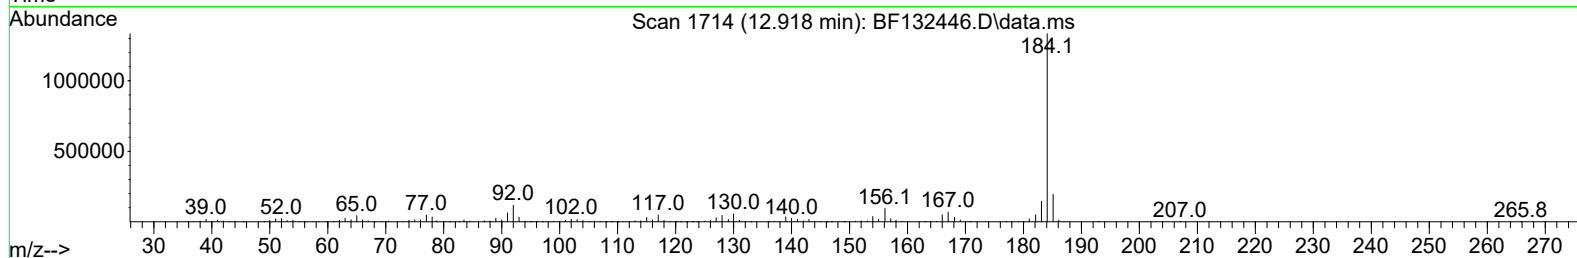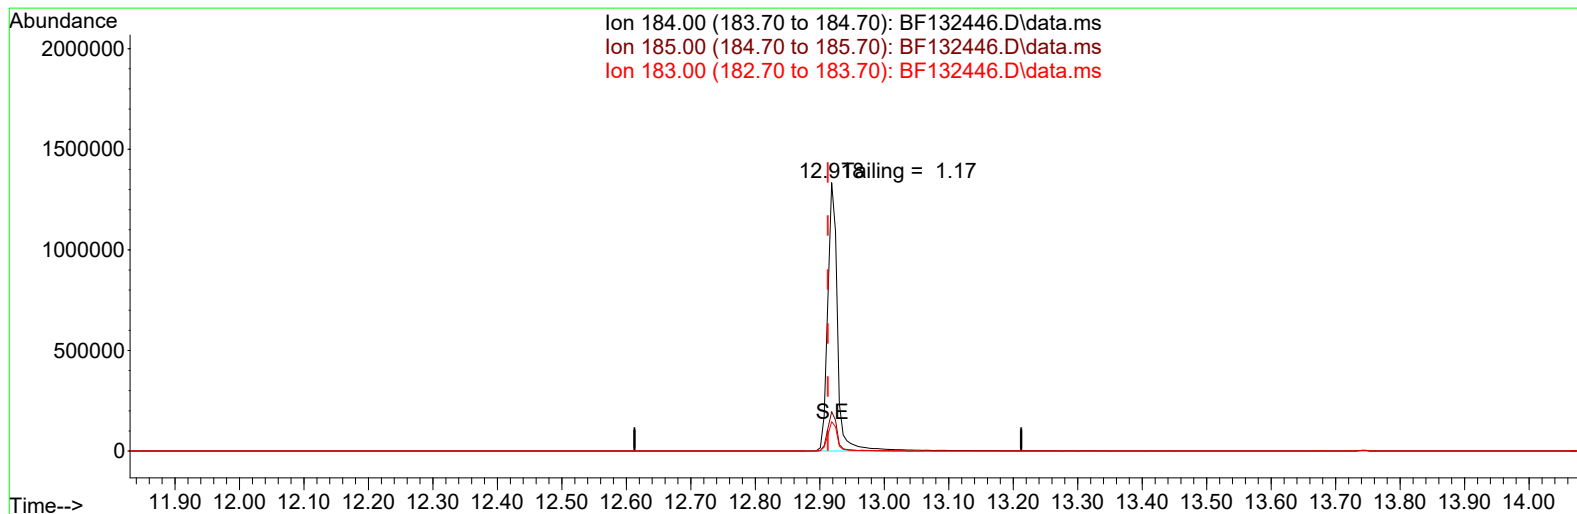

TIC: BF132446.D\data.ms

(77) Benzidine

12.918min (+ 0.006) 0.00 ng

response 1406642

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.69
183.00	11.50	10.94
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/17/2023	BNA_F	<u>BF132446.D</u>
Compound Name	Response	Retention Time
DDT	862049	13.742
DDD	18493	13.442
DDE	462	13.102
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18955	881004	2.15

Instrument :
BNA_F
ClientSampleId :
DFTPP