


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021723\
Data File : BF132453.D
Acq On : 17 Feb 2023 16:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Feb 18 00:58:25 2023

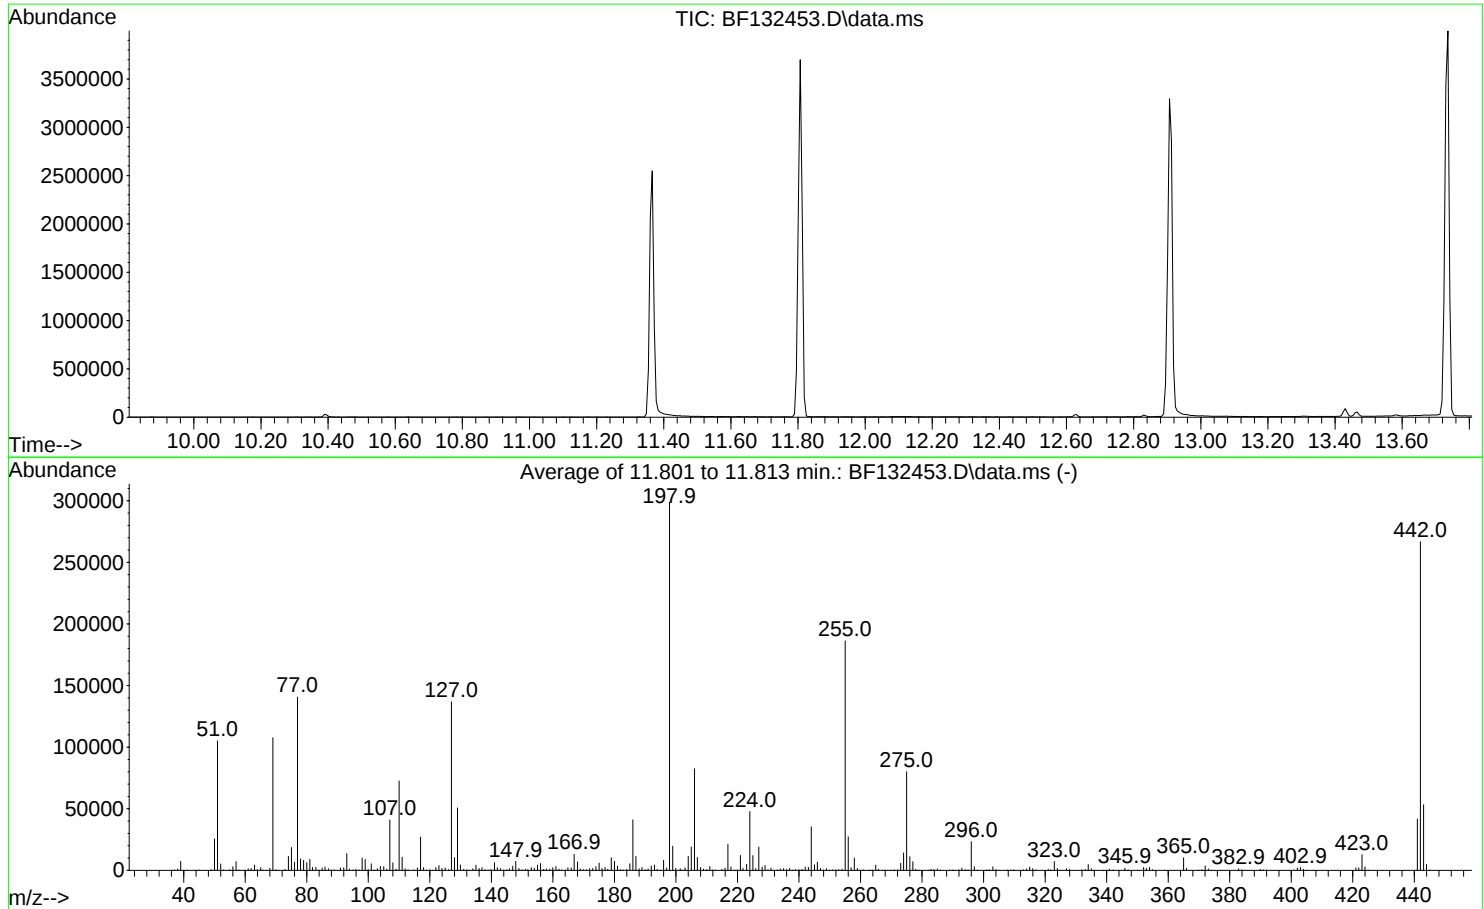




AutoFind: Scans 1524, 1525, 1526; Background Corrected with Scan 1519

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	104997	PASS
68	69	0.00	2	1.6	1762	PASS
69	198	0.00	100	36.0	107573	PASS
70	69	0.00	2	0.5	507	PASS
127	198	10	80	45.8	136656	PASS
197	198	0.00	2	0.6	1860	PASS
198	198	100	100	100.0	298624	PASS
199	198	5	9	6.6	19588	PASS
275	198	10	60	26.8	79995	PASS
365	198	1	100	3.4	10233	PASS
441	198	0.01	100	14.0	41699	PASS
442	442	50	100	100.0	266768	PASS
443	442	15	24	19.9	53205	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021723\
Data File : BF132453.D
Acq On : 17 Feb 2023 16:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 18 04:55:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 18 00:58:25 2023
Response via : Initial Calibration

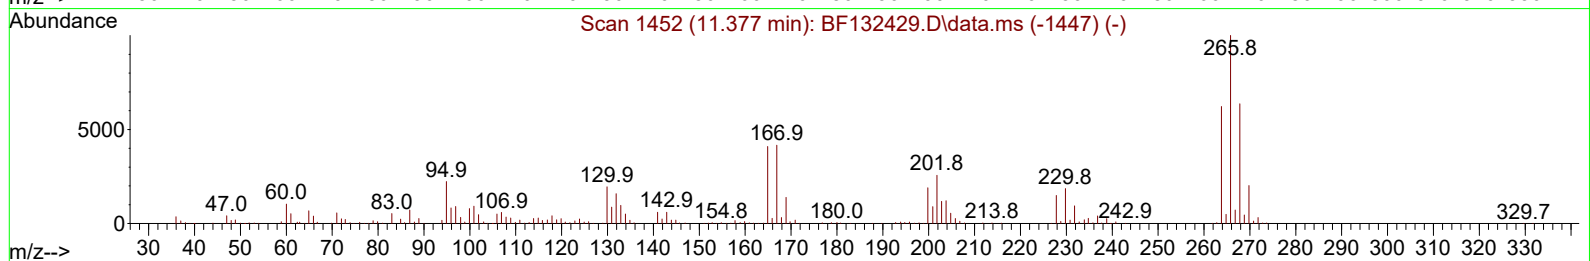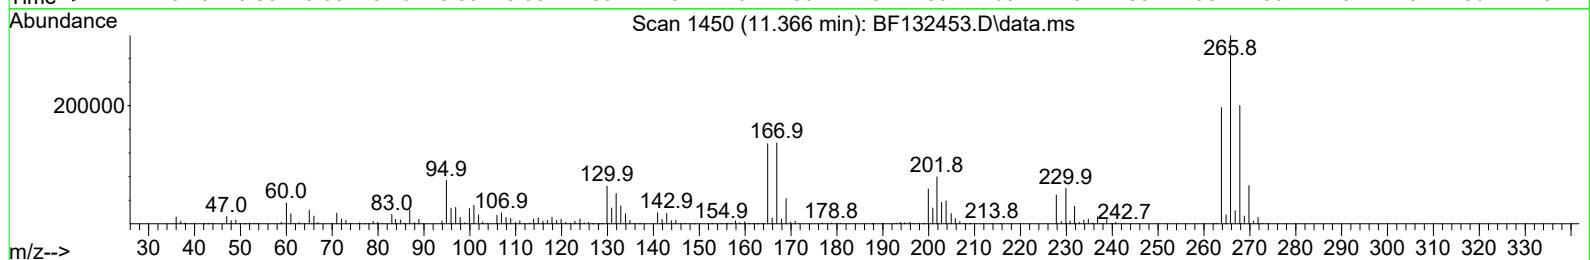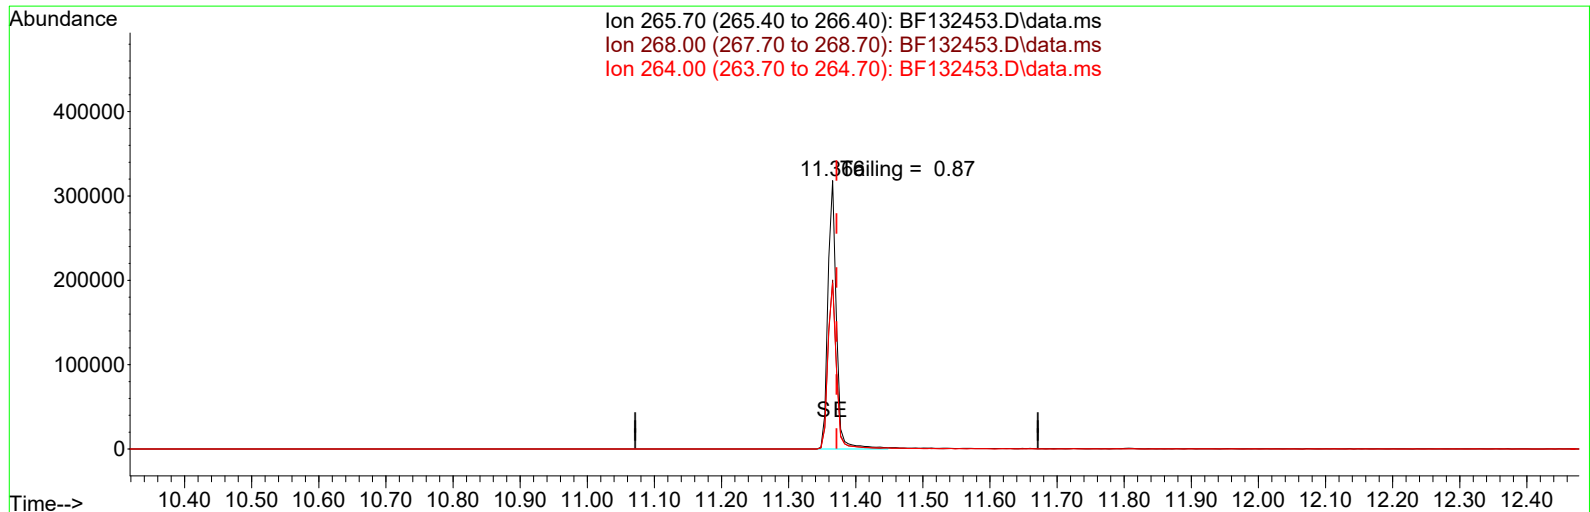

TIC: BF132453.D\data.ms

(70) Pentachlorophenol (C)

11.366min (-0.006) 387755.74 ng




response 284477

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.95
264.00	62.20	61.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021723\
Data File : BF132453.D
Acq On : 17 Feb 2023 16:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 18 04:55:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 18 00:58:25 2023
Response via : Initial Calibration

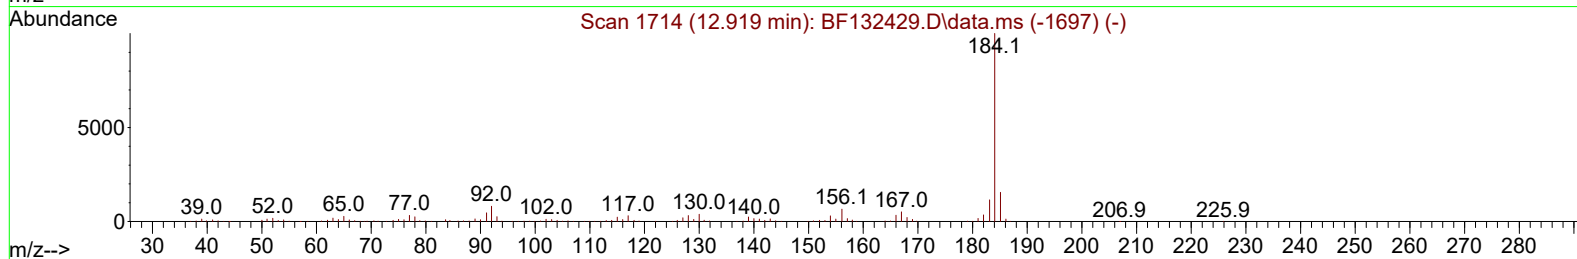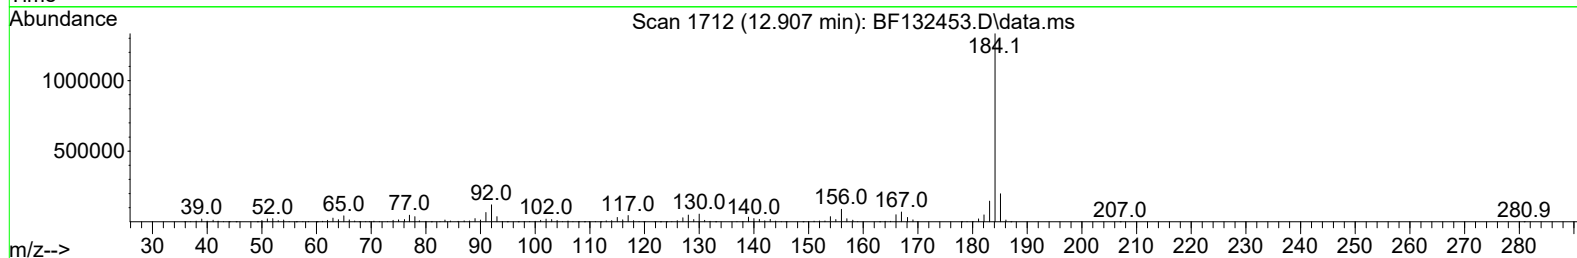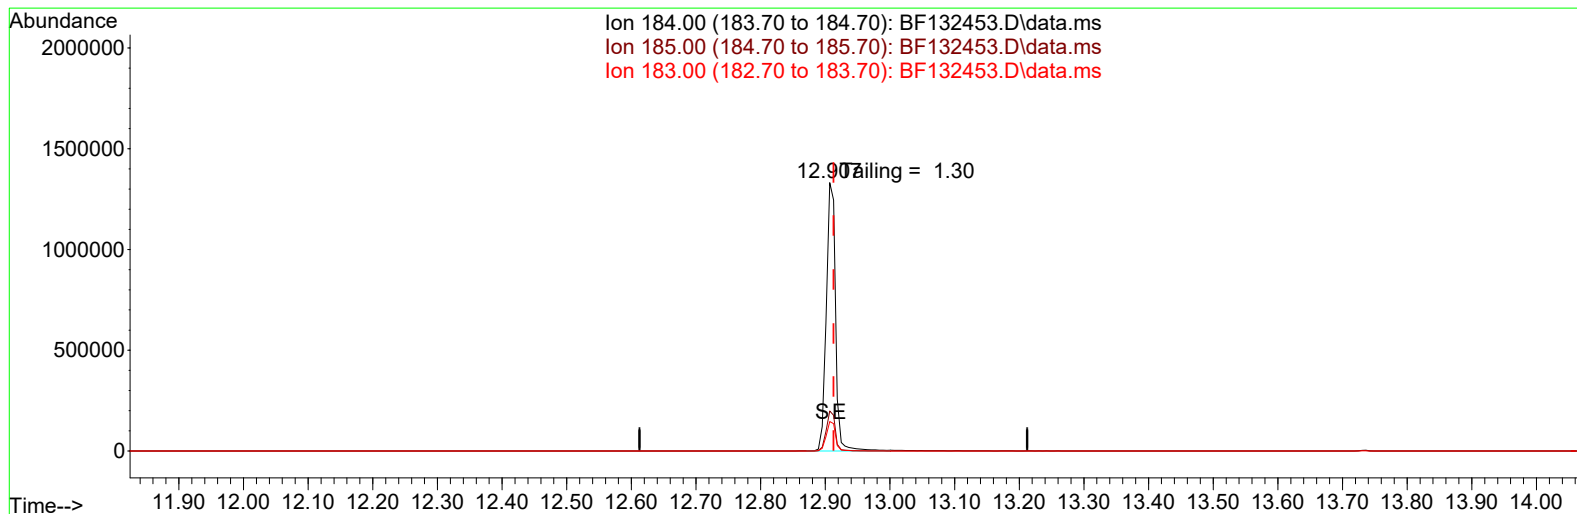

TIC: BF132453.D\data.ms

(77) Benzidine

12.907min (-0.006) 1162961.65 ng

response 1337251

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.93
183.00	11.50	11.01
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/17/2023	BNA_F	<u>BF132453.D</u>
Compound Name	Response	Retention Time
DDT	715855	13.736
DDD	20781	13.43
DDE	387	13.089
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21168	737023	2.87

Instrument :
BNA_F
ClientSampleId :
DFTPP