
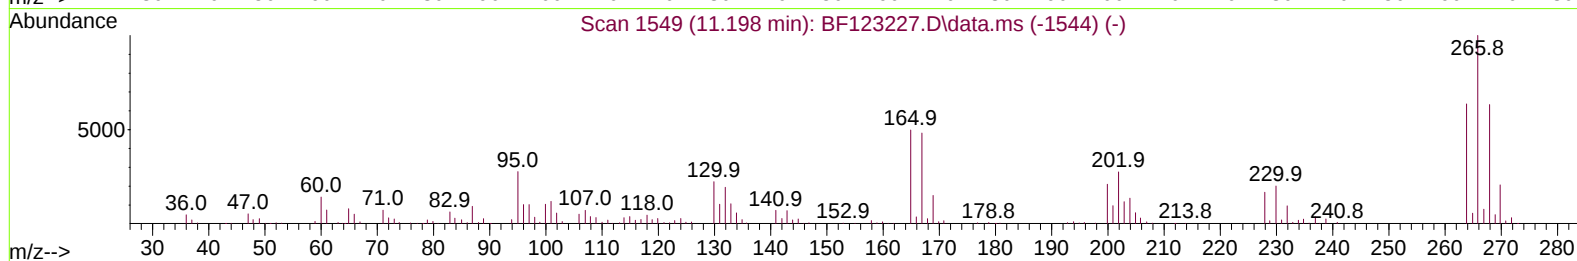
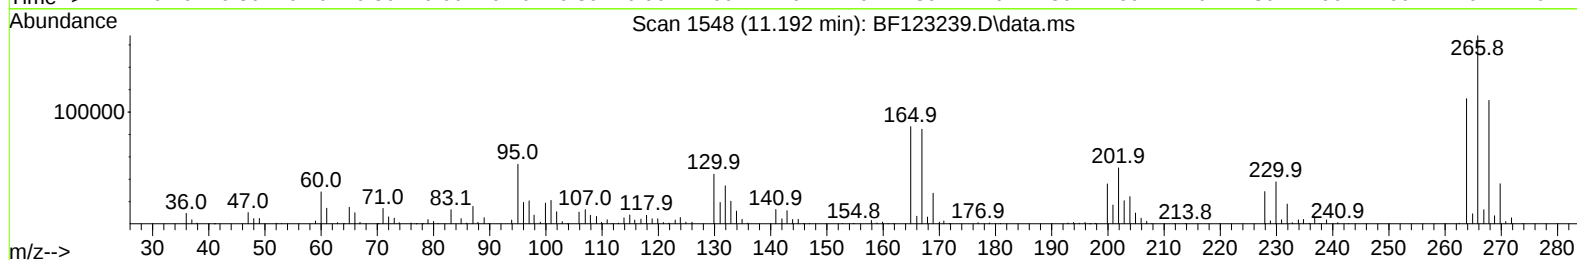


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022021\
Data File : BF123239.D
Acq On : 20 Feb 2021 9:55
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 04:17:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 16:08:53 2021
Response via : Initial Calibration

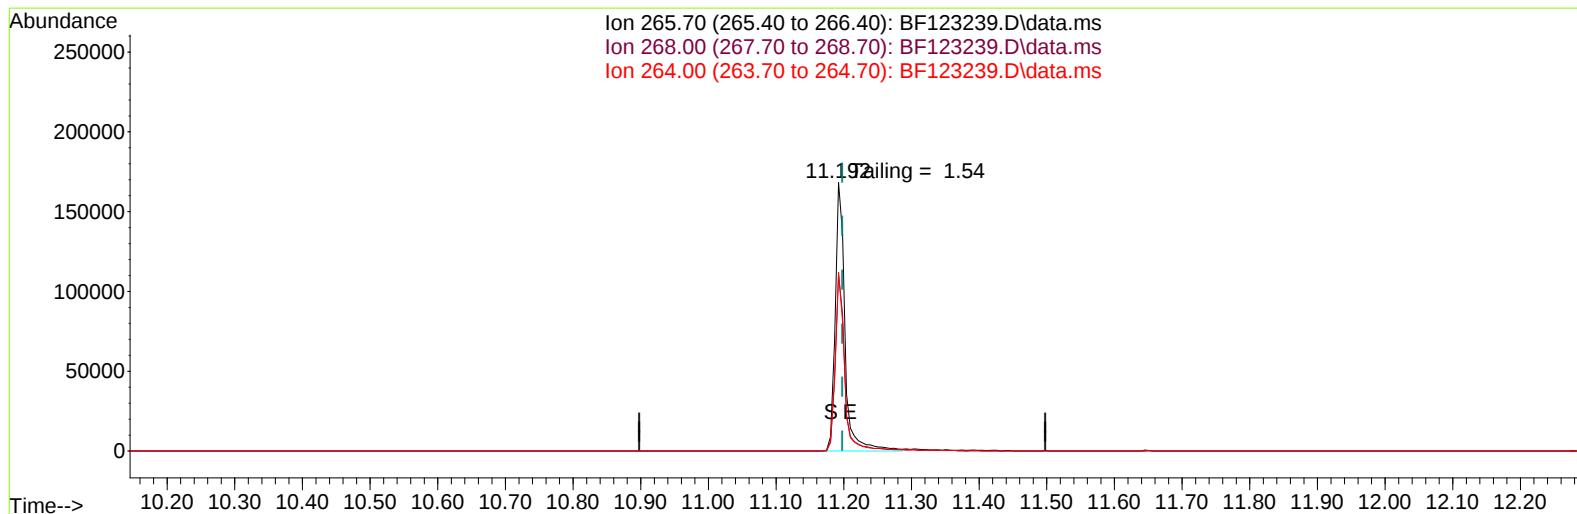

TIC: BF123239.D\data.ms

(70) Pentachlorophenol (C)




11.192min (-0.006) 28457.72 ng

response 168183

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	65.72
264.00	62.30	66.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022021\
Data File : BF123239.D
Acq On : 20 Feb 2021 9:55
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 04:17:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 16:08:53 2021
Response via : Initial Calibration

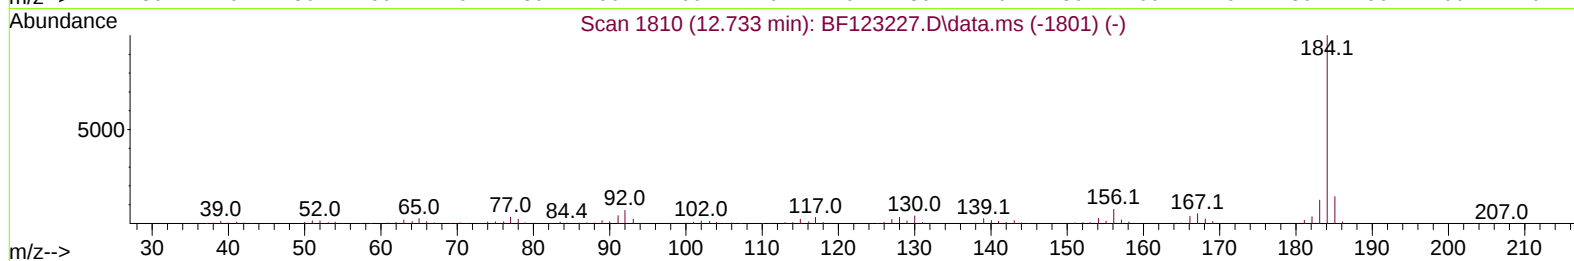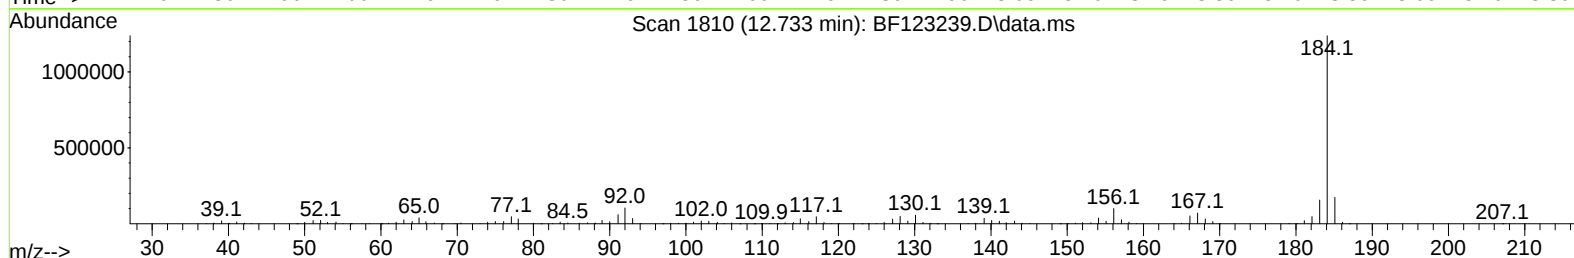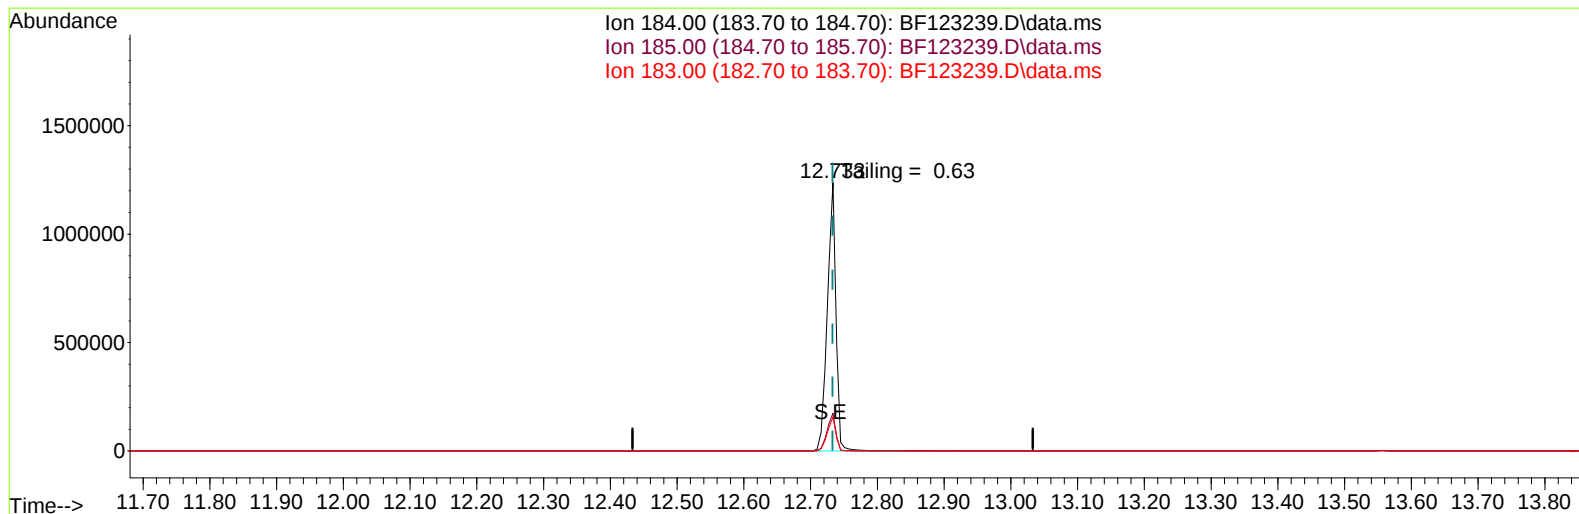

TIC: BF123239.D\data.ms

(77) Benzidine

12.733min (+ 0.000) 0.00 ng

response 1111227

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.09
183.00	12.10	12.63
0.00	0.00	0.00