

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022021\
 Data File : BF123242.D
 Acq On : 20 Feb 2021 11:42
 Operator : JU/CG
 Sample : PB134747TB
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB134747TB

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123242.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.487	573	578	581	rBV	4366644	4424719	72.55%	12.685%
2	6.487	742	748	751	rBV	3980024	4450318	72.97%	12.758%
3	6.857	807	811	814	rBV	969074	874709	14.34%	2.508%
4	7.416	900	906	909	rBV	2476970	2924509	47.95%	8.384%
5	8.139	1024	1029	1032	rBV	1266651	1153534	18.91%	3.307%
6	9.222	1206	1213	1216	rBV	5487421	6099108	100.00%	17.485%
7	9.898	1322	1328	1332	rBV	1928836	1721835	28.23%	4.936%
8	10.692	1457	1463	1466	rBV	3157931	3108686	50.97%	8.912%
9	11.386	1576	1581	1585	rBV	1453273	1398816	22.93%	4.010%
10	12.986	1846	1853	1856	rBV	5834661	5685472	93.22%	16.299%
11	14.039	2027	2032	2035	rBV	1464656	1348941	22.12%	3.867%
12	15.515	2277	2283	2286	rBV	1037258	1339636	21.96%	3.841%
13	15.980	2357	2362	2369	rBV	68662	103019	1.69%	0.295%
14	16.498	2444	2450	2459	rVB	60024	109523	1.80%	0.314%
15	17.092	2546	2551	2557	rVB4	37269	72107	1.18%	0.207%
16	17.804	2666	2672	2681	rVB4	26667	66650	1.09%	0.191%




Sum of corrected areas: 34881582

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022021\
Data File : BF123242.D
Acq On : 20 Feb 2021 11:42
Operator : JU/CG
Sample : PB134747TB
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134747TB

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

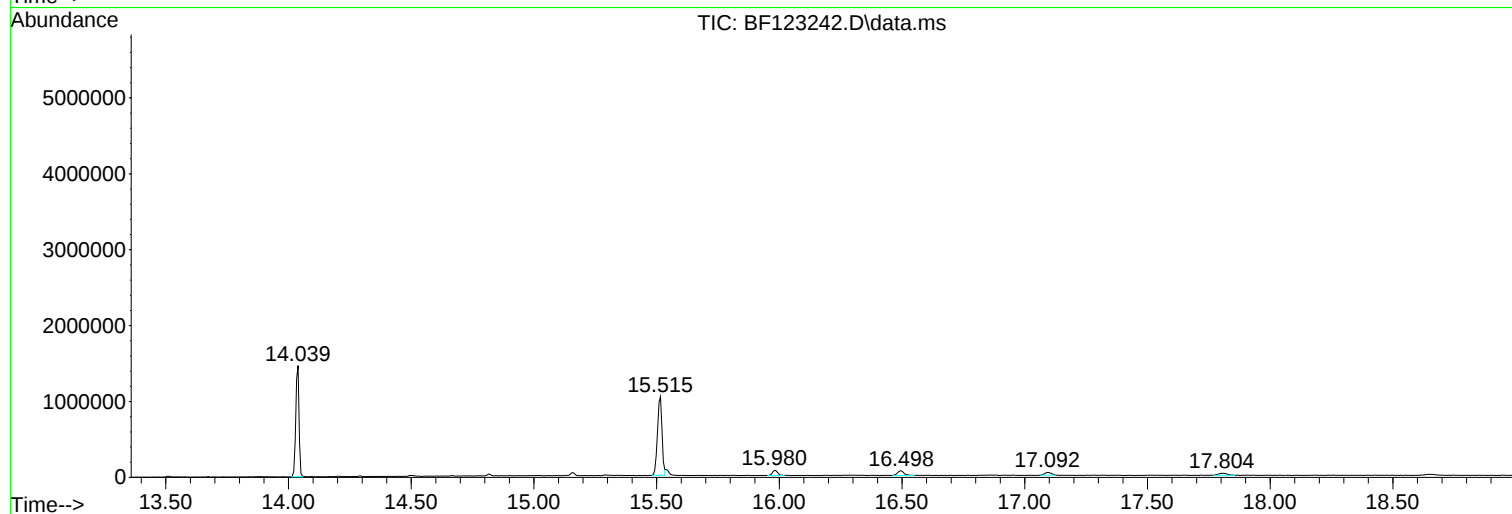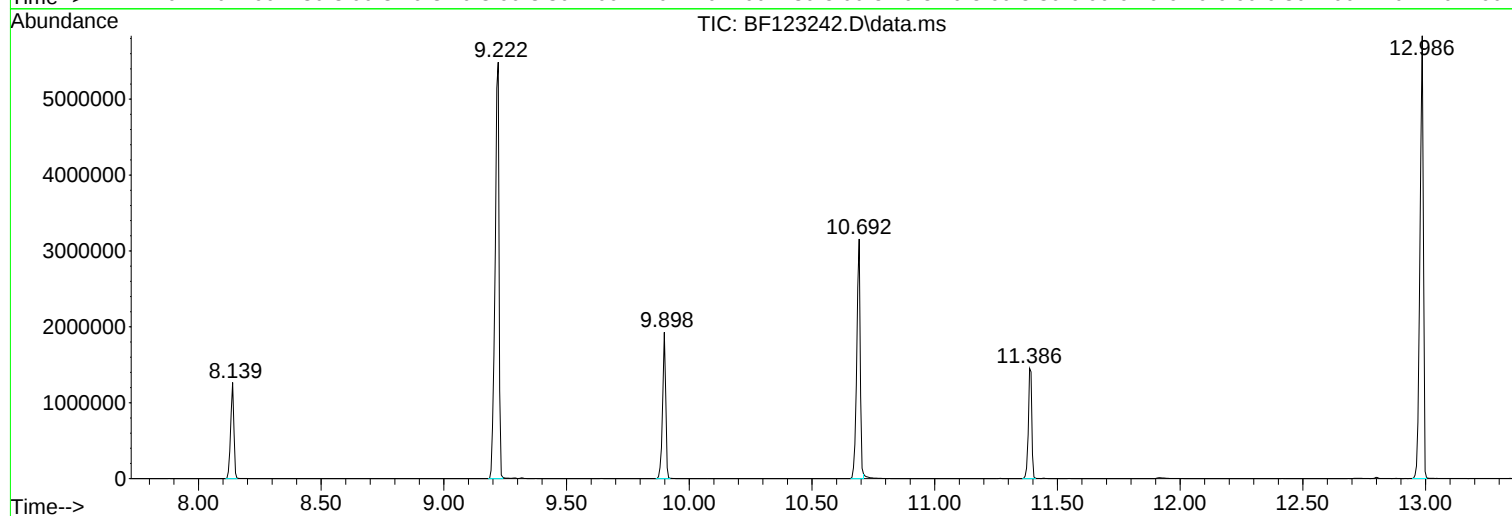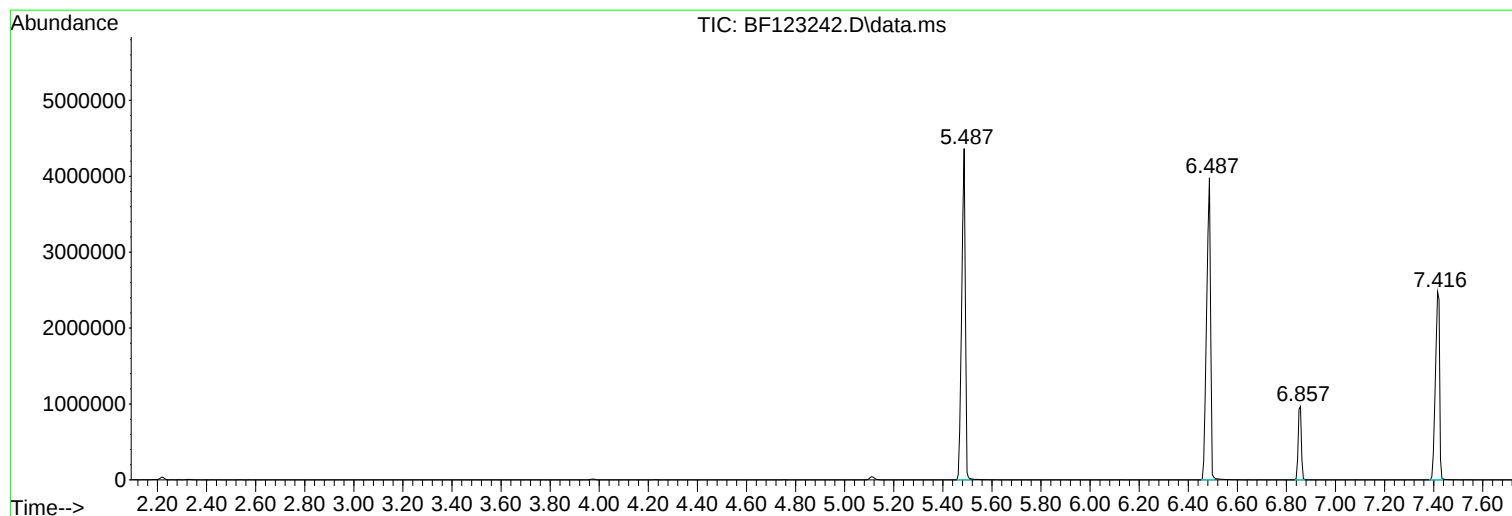

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022021\
Data File : BF123242.D
Acq On : 20 Feb 2021 11:42
Operator : JU/CG
Sample : PB134747TB
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134747TB

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022021\
Data File : BF123242.D
Acq On : 20 Feb 2021 11:42
Operator : JU/CG
Sample : PB134747TB
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134747TB

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------