


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022021\
 Data File : BF123239.D
 Acq On : 20 Feb 2021 9:55
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 19 16:08:53 2021

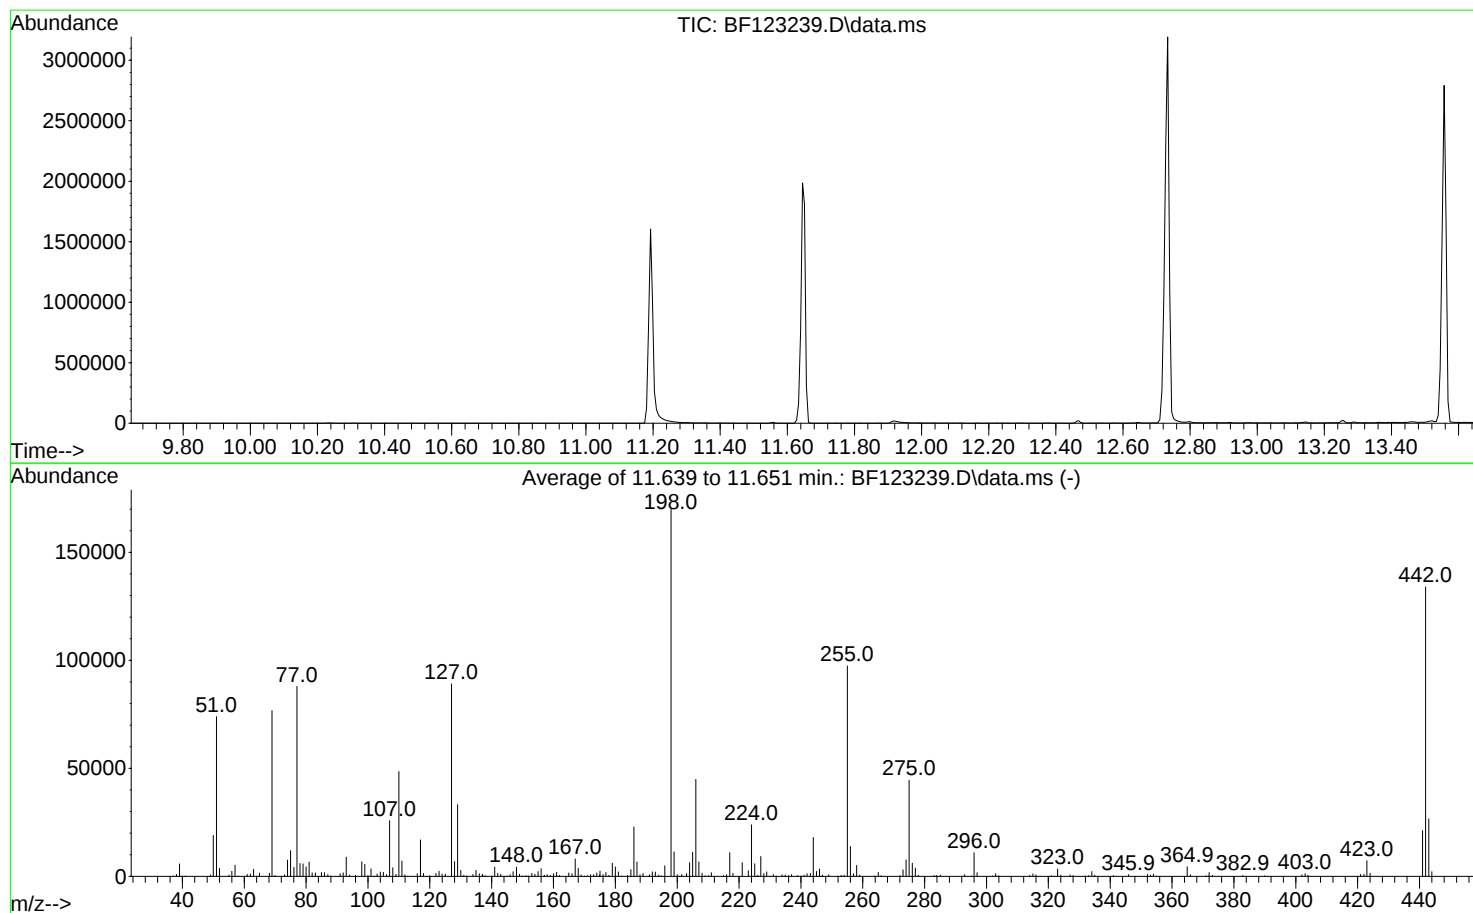




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.4	73909	PASS
68	69	0.00	2	1.8	1416	PASS
69	198	0.00	100	45.1	76723	PASS
70	69	0.00	2	0.6	468	PASS
127	198	10	80	52.3	89115	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	170269	PASS
199	198	5	9	6.7	11334	PASS
275	198	10	60	26.1	44451	PASS
365	198	1	100	2.6	4464	PASS
441	198	0.01	100	12.5	21199	PASS
442	442	50	100	100.0	133957	PASS
443	442	15	24	19.8	26580	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022021\
Data File : BF123239.D
Acq On : 20 Feb 2021 9:55
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 22 04:17:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 16:08:53 2021
Response via : Initial Calibration

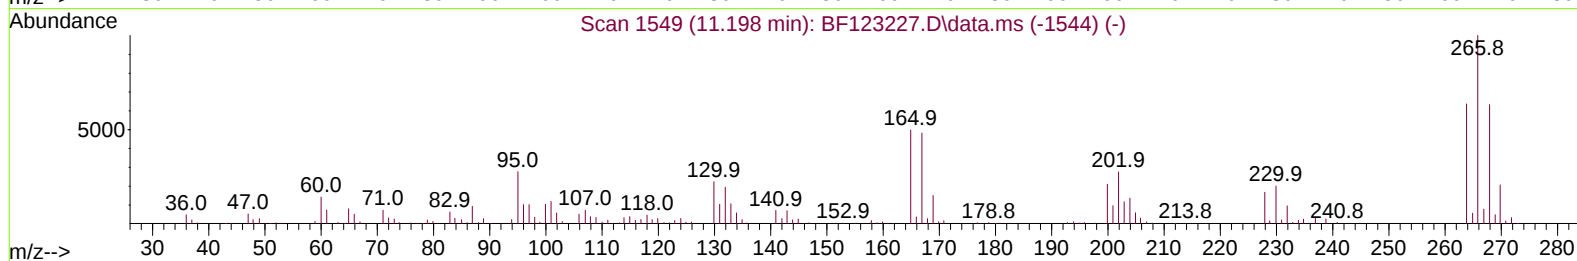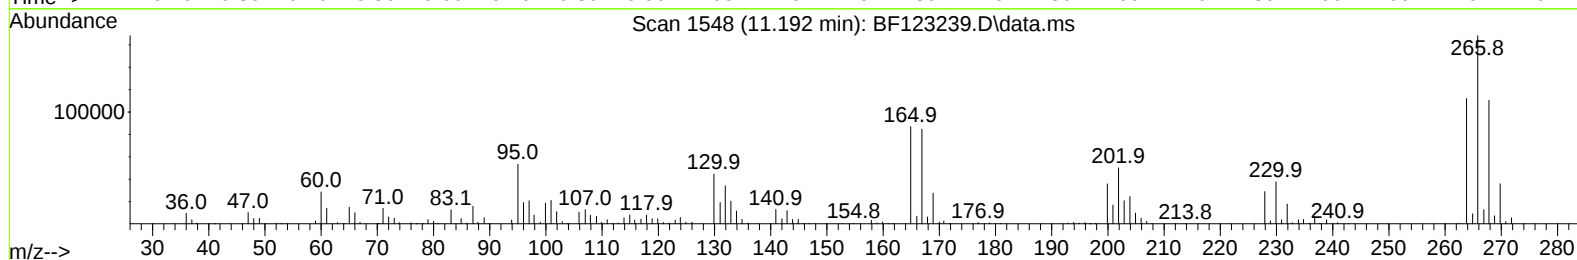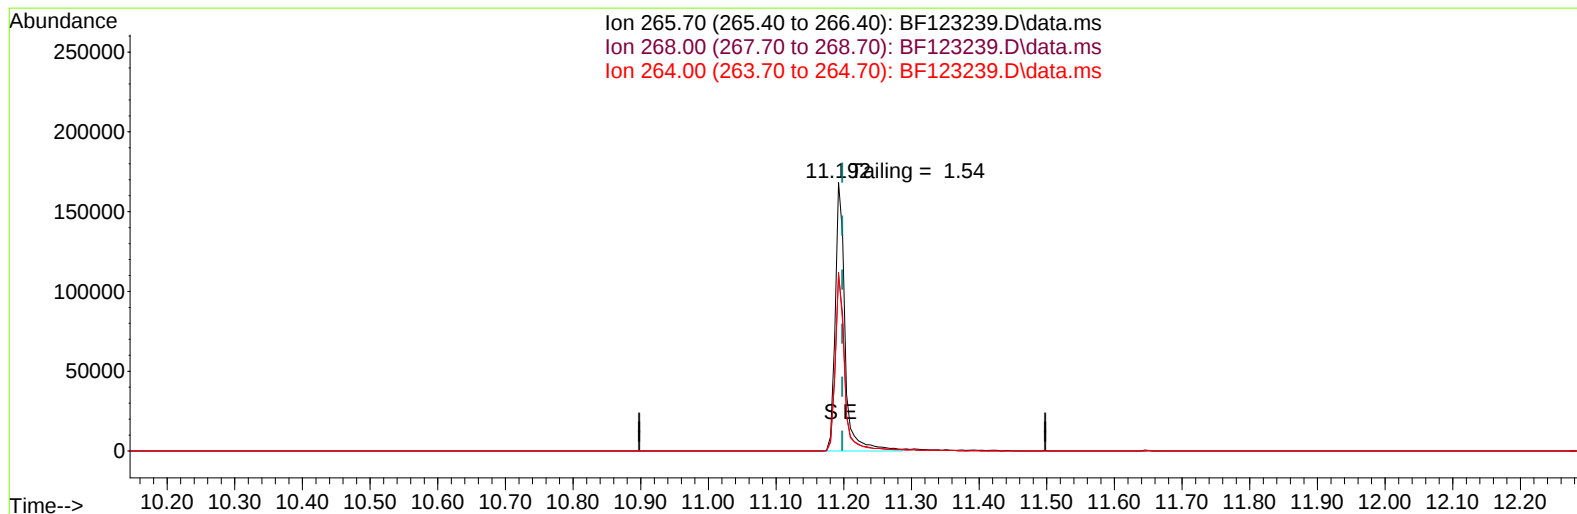

TIC: BF123239.D\data.ms

(70) Pentachlorophenol (C)

11.192min (-0.006) 28457.72 ng




response 168183

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	65.72
264.00	62.30	66.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022021\
 Data File : BF123239.D
 Acq On : 20 Feb 2021 9:55
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 22 04:17:10 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 19 16:08:53 2021
 Response via : Initial Calibration

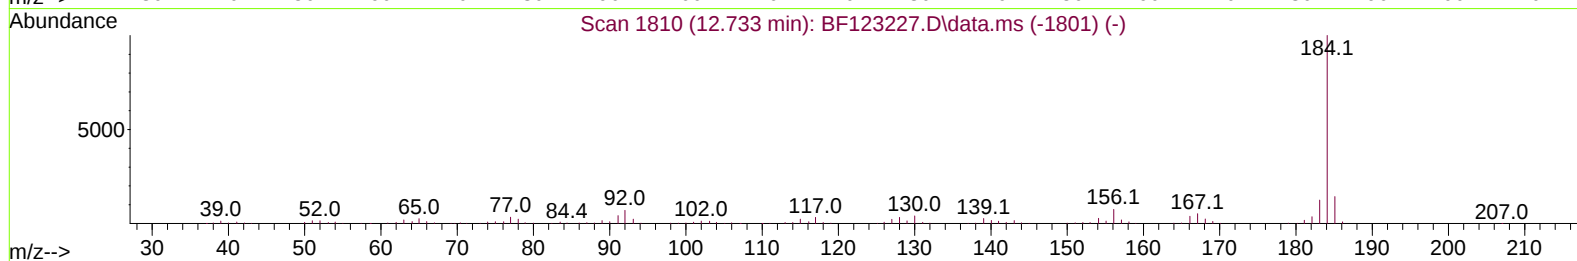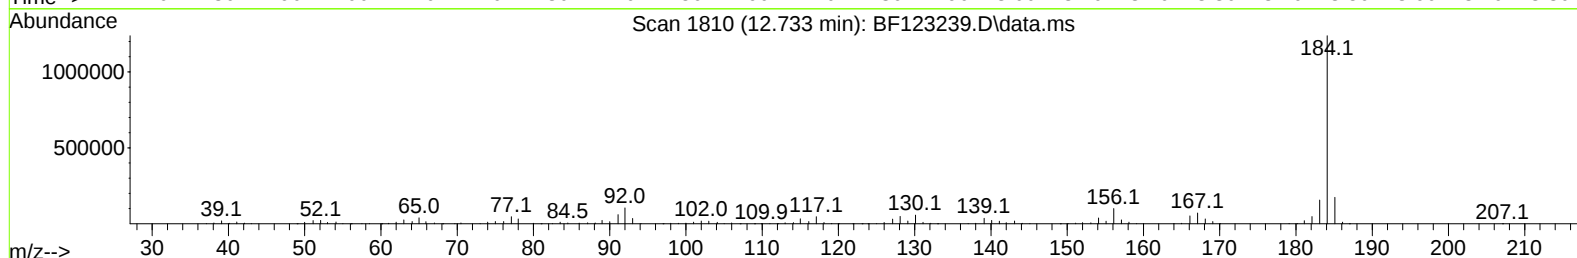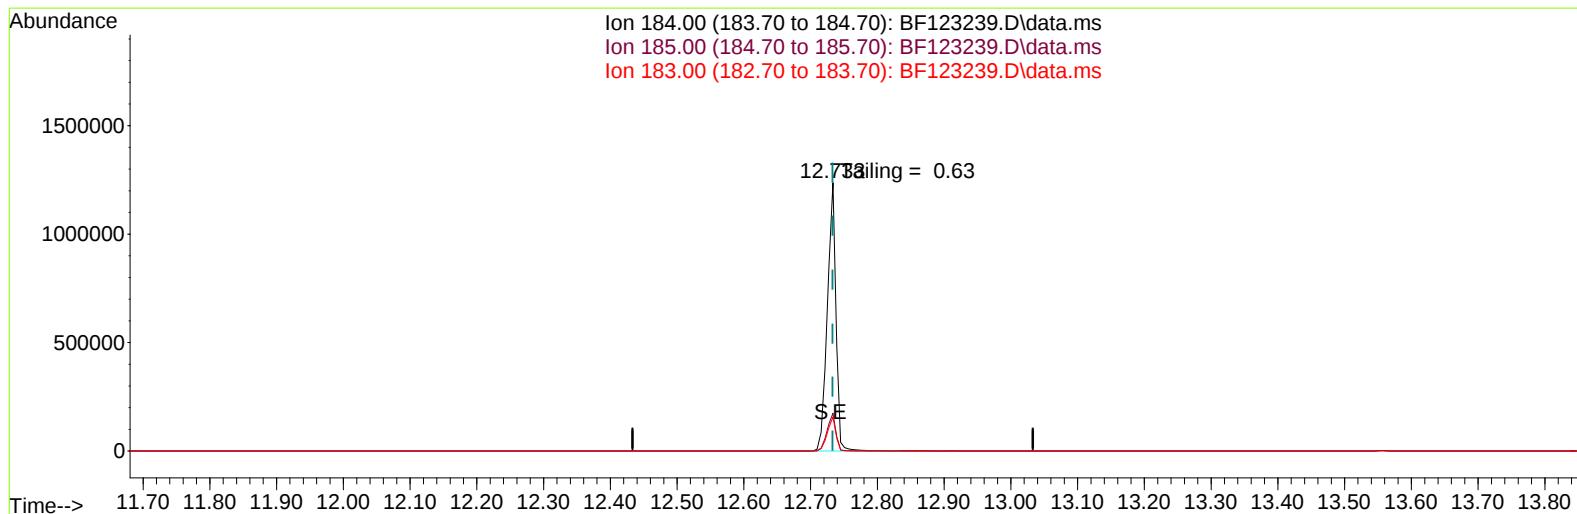

TIC: BF123239.D\data.ms

(77) Benzidine

12.733min (+ 0.000) 0.00 ng

response 1111227

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.09
183.00	12.10	12.63
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_F
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
02/20/2021	BNA_F	<u>BF123239.D</u>
Compound Name	Response	Retention Time
DDT	447174	13.557
DDD	5837	13.257
DDE	1111	12.922
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6948	454122	1.53