
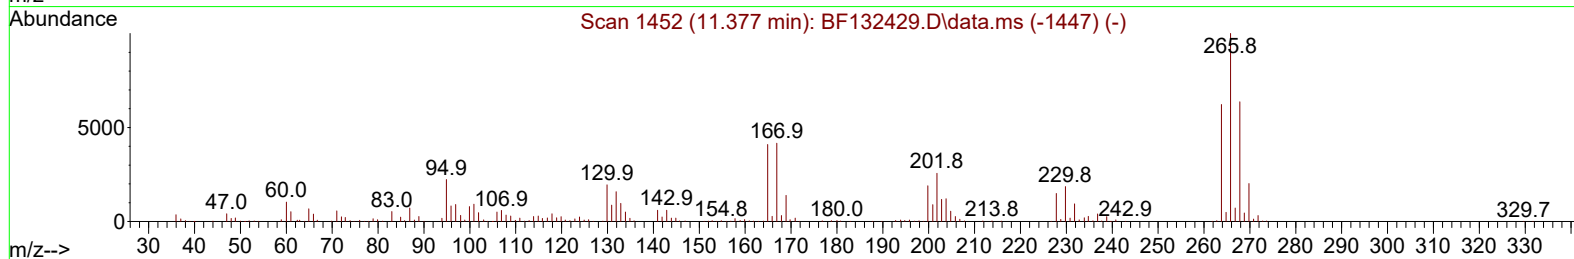
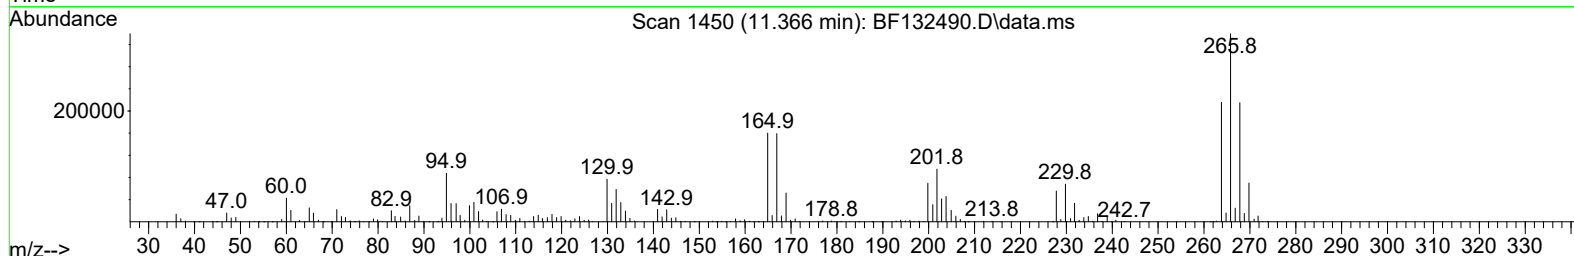


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022123\
Data File : BF132490.D
Acq On : 21 Feb 2023 11:06
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 03:10:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 21 16:43:07 2023
Response via : Initial Calibration

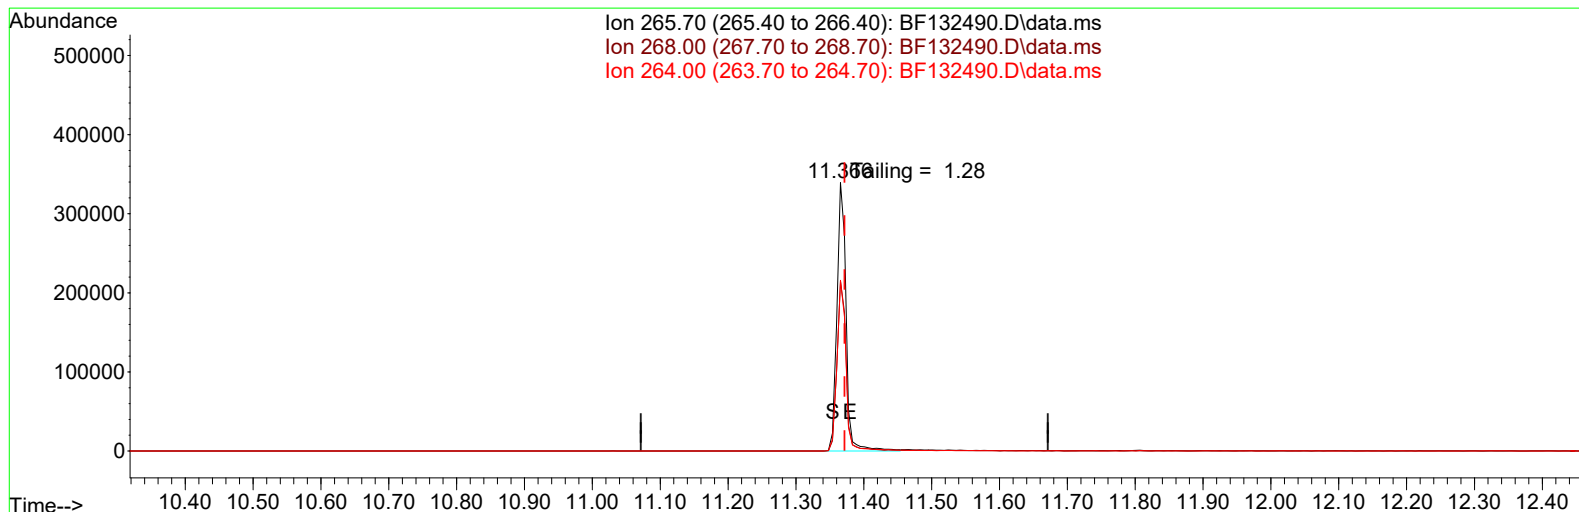

TIC: BF132490.D\data.ms

(70) Pentachlorophenol (C)




11.366min (-0.006) 232858.39 ng

response 316794

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.33
264.00	62.20	63.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022123\
Data File : BF132490.D
Acq On : 21 Feb 2023 11:06
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 03:10:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 21 16:43:07 2023
Response via : Initial Calibration

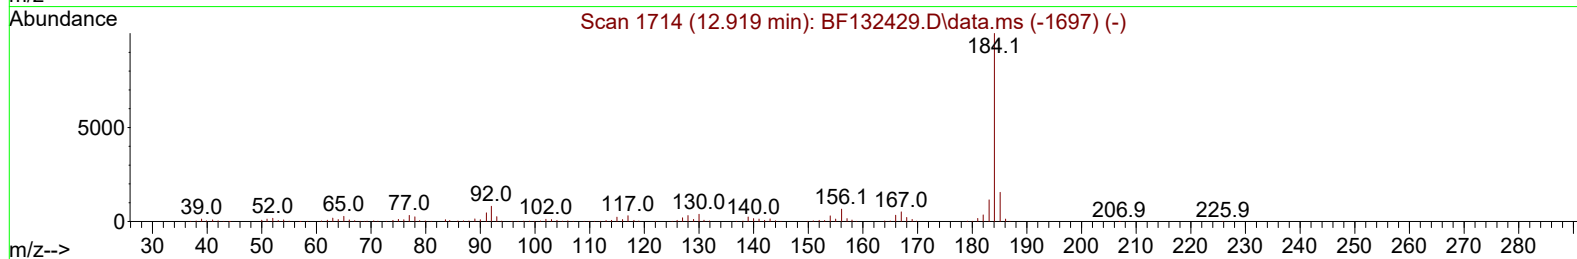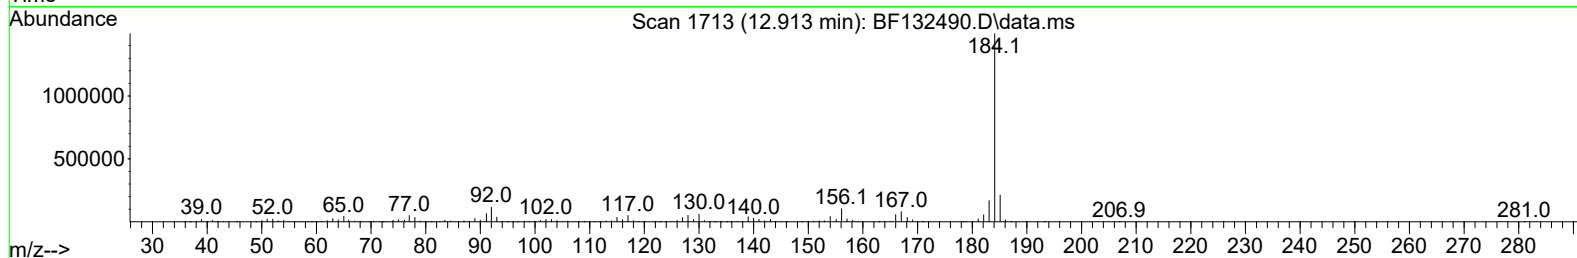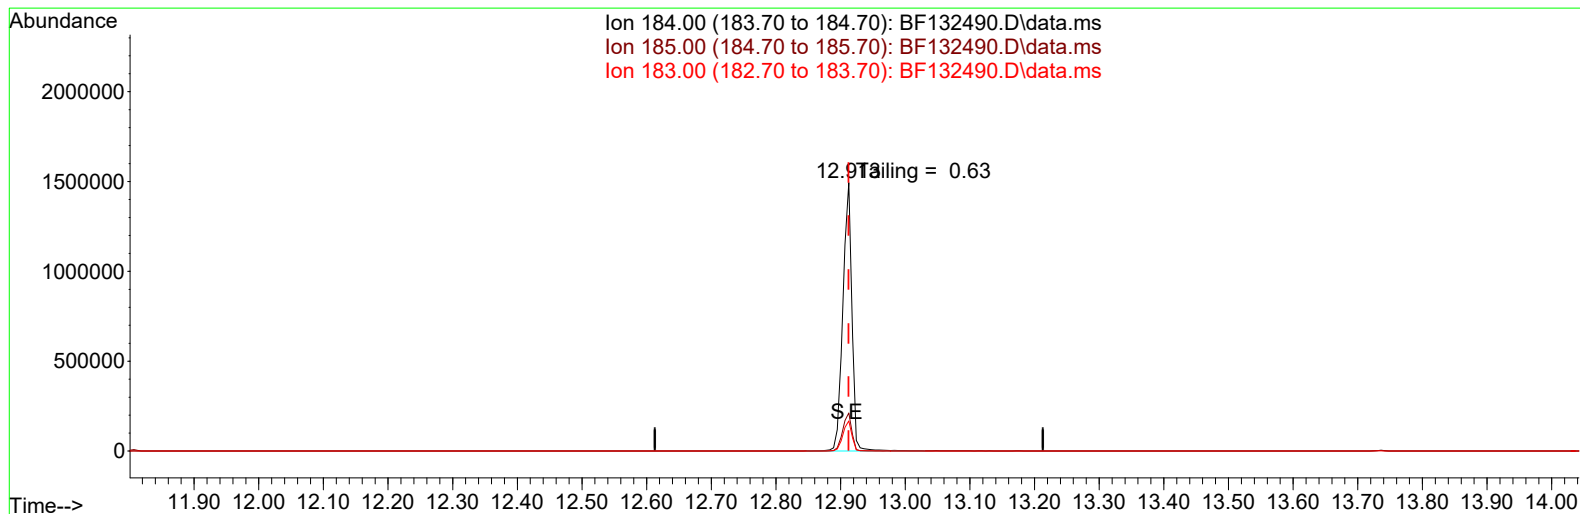

TIC: BF132490.D\data.ms

(77) Benzidine

12.913min (0.000) 1218376.08 ng

response 1452858

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.20
183.00	11.50	11.21
0.00	0.00	0.00