


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022123\
Data File : BF132490.D
Acq On : 21 Feb 2023 11:06
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 21 16:43:07 2023

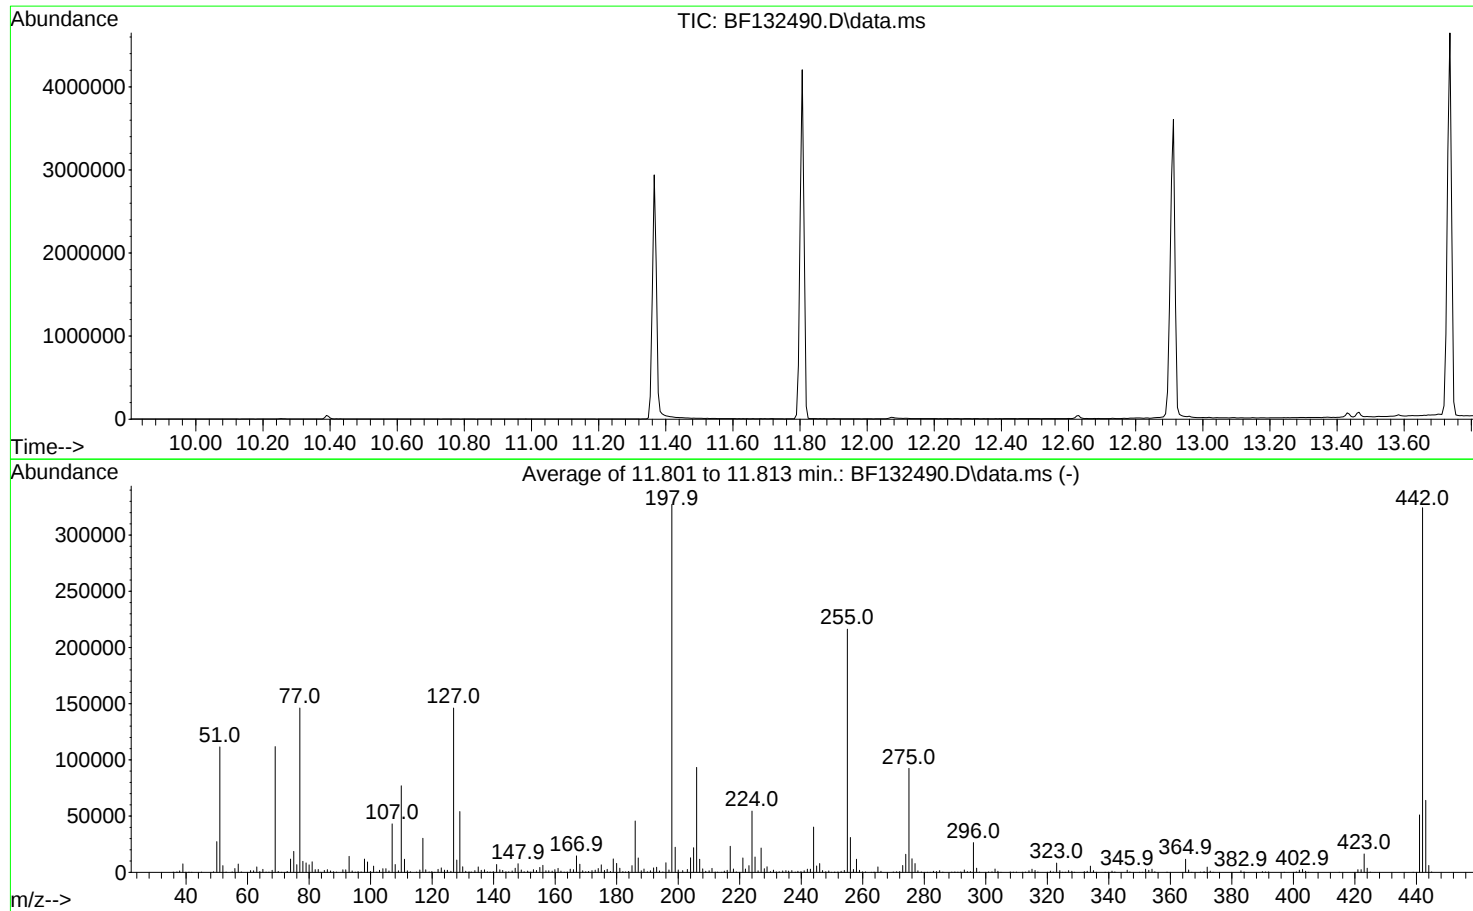




AutoFind: Scans 1524, 1525, 1526; Background Corrected with Scan 1519

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	111573	PASS
68	69	0.00	2	1.6	1790	PASS
69	198	0.00	100	34.1	111760	PASS
70	69	0.00	2	0.7	729	PASS
127	198	10	80	44.6	146099	PASS
197	198	0.00	2	0.7	2140	PASS
198	198	100	100	100.0	327275	PASS
199	198	5	9	6.8	22248	PASS
275	198	10	60	28.2	92424	PASS
365	198	1	100	3.5	11574	PASS
441	198	0.01	100	15.6	51019	PASS
442	442	50	100	100.0	324309	PASS
443	442	15	24	19.7	63941	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022123\
 Data File : BF132490.D
 Acq On : 21 Feb 2023 11:06
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 22 03:10:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 21 16:43:07 2023
 Response via : Initial Calibration

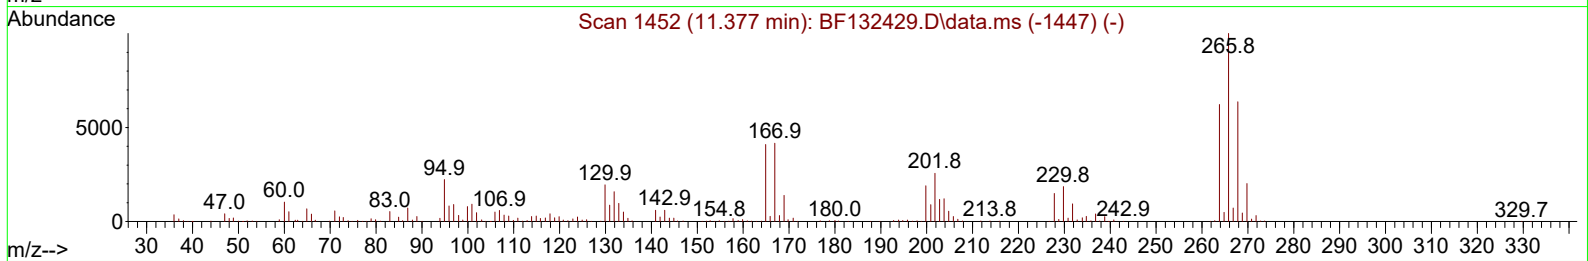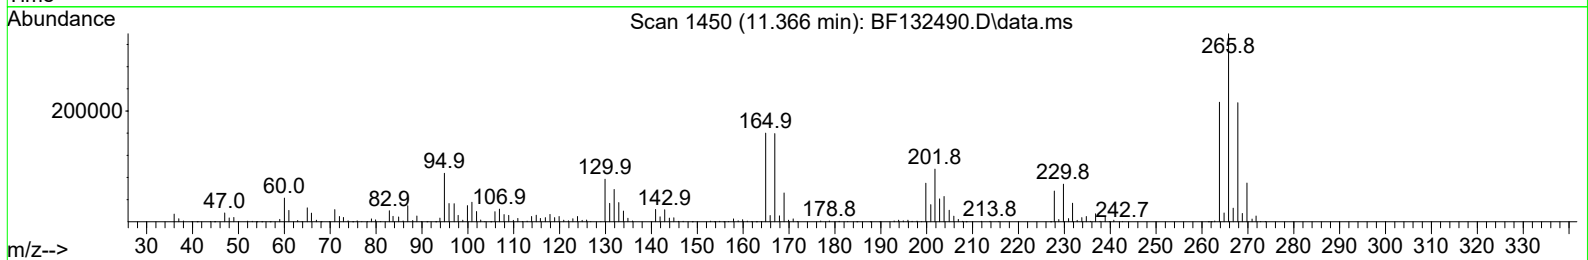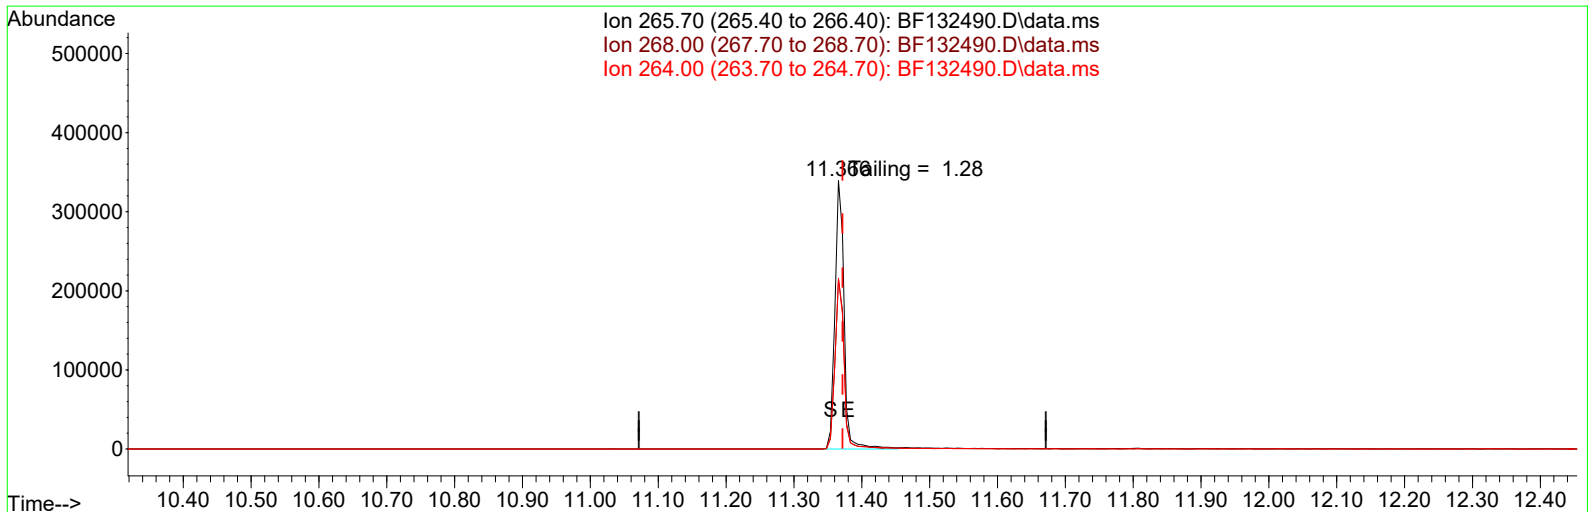

TIC: BF132490.D\data.ms

(70) Pentachlorophenol (C)

11.366min (-0.006) 232858.39 ng




response 316794

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.33
264.00	62.20	63.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022123\
Data File : BF132490.D
Acq On : 21 Feb 2023 11:06
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 22 03:10:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 21 16:43:07 2023
Response via : Initial Calibration

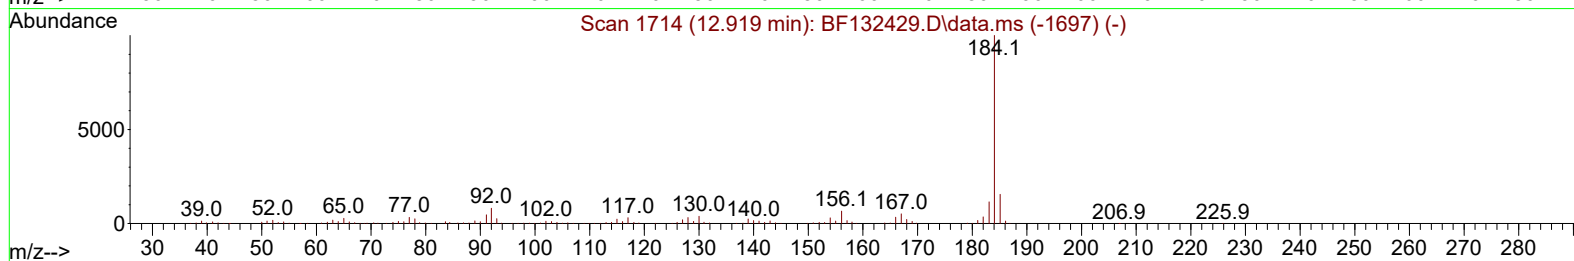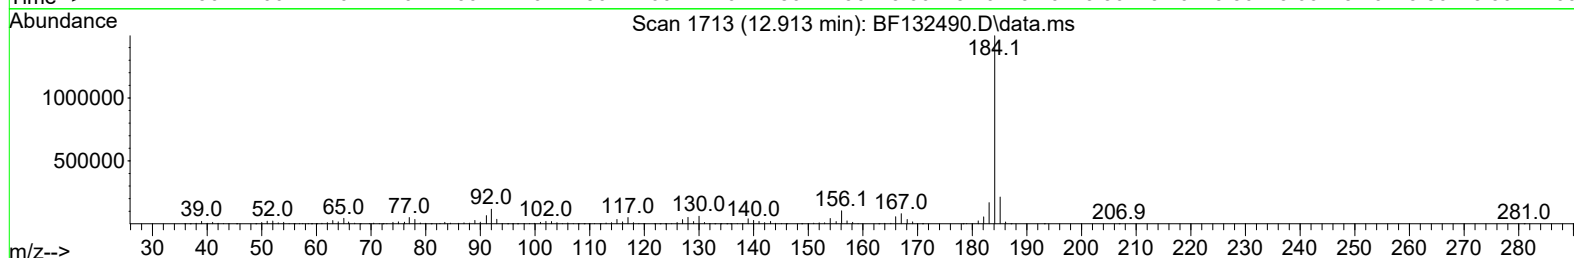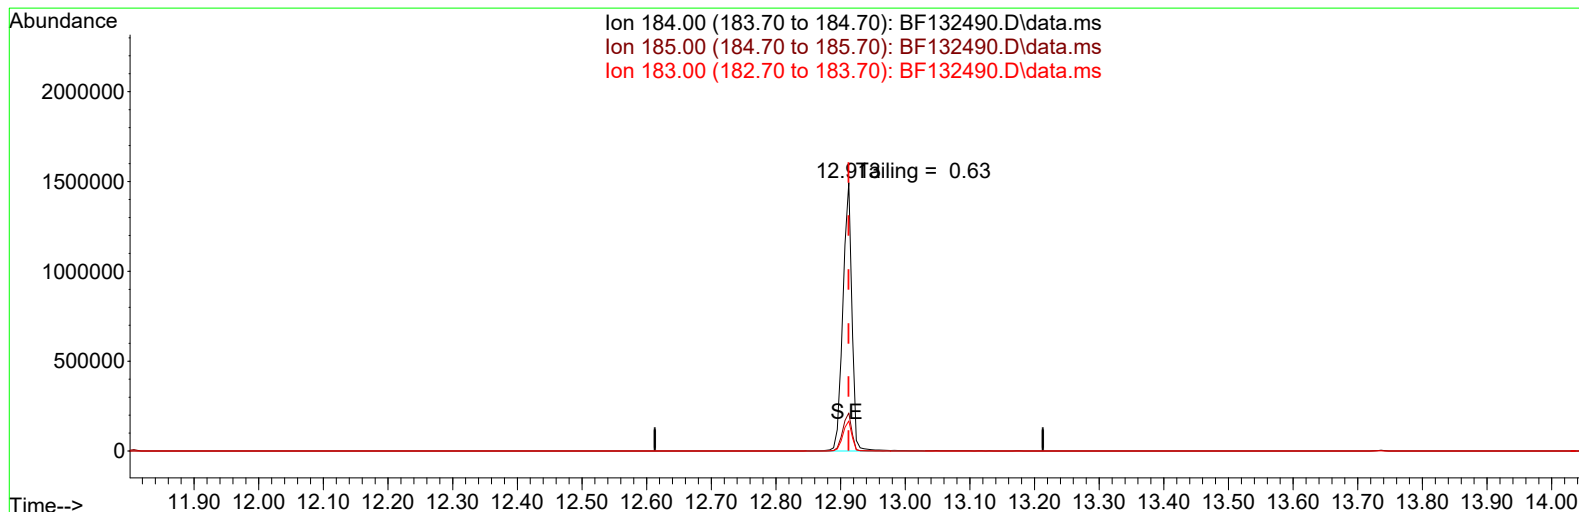

TIC: BF132490.D\data.ms

(77) Benzidine

12.913min (0.000) 1218376.08 ng

response 1452858

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.20
183.00	11.50	11.21
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/21/2023	BNA_F	<u>BF132490.D</u>
Compound Name	Response	Retention Time
DDT	813235	13.736
DDD	18523	13.465
DDE	496	13.095
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19019	832254	2.29

Instrument :
BNA_F
ClientSampleId :
DFTPP