
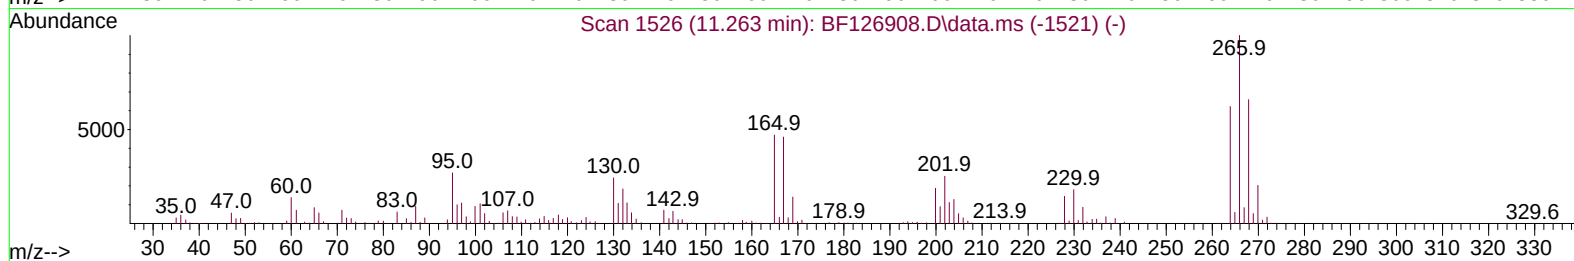
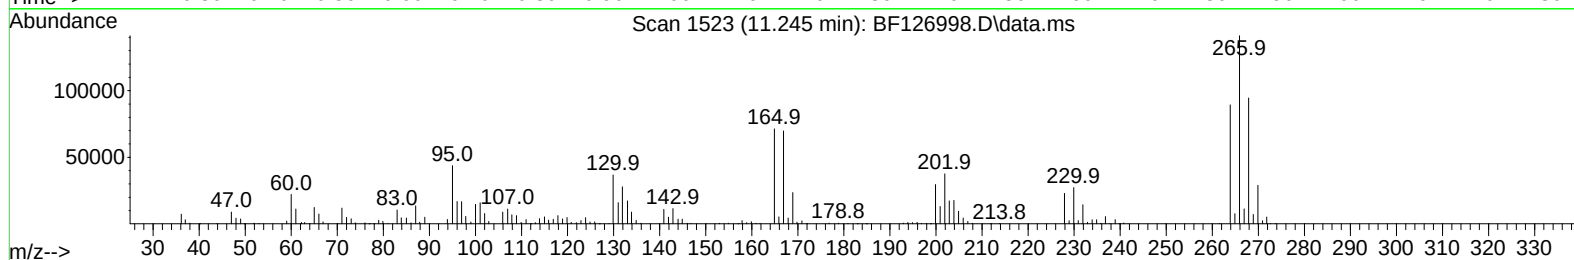


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022222\
 Data File : BF126998.D
 Acq On : 22 Feb 2022 09:36
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 12:22:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 21 13:16:57 2022
 Response via : Initial Calibration

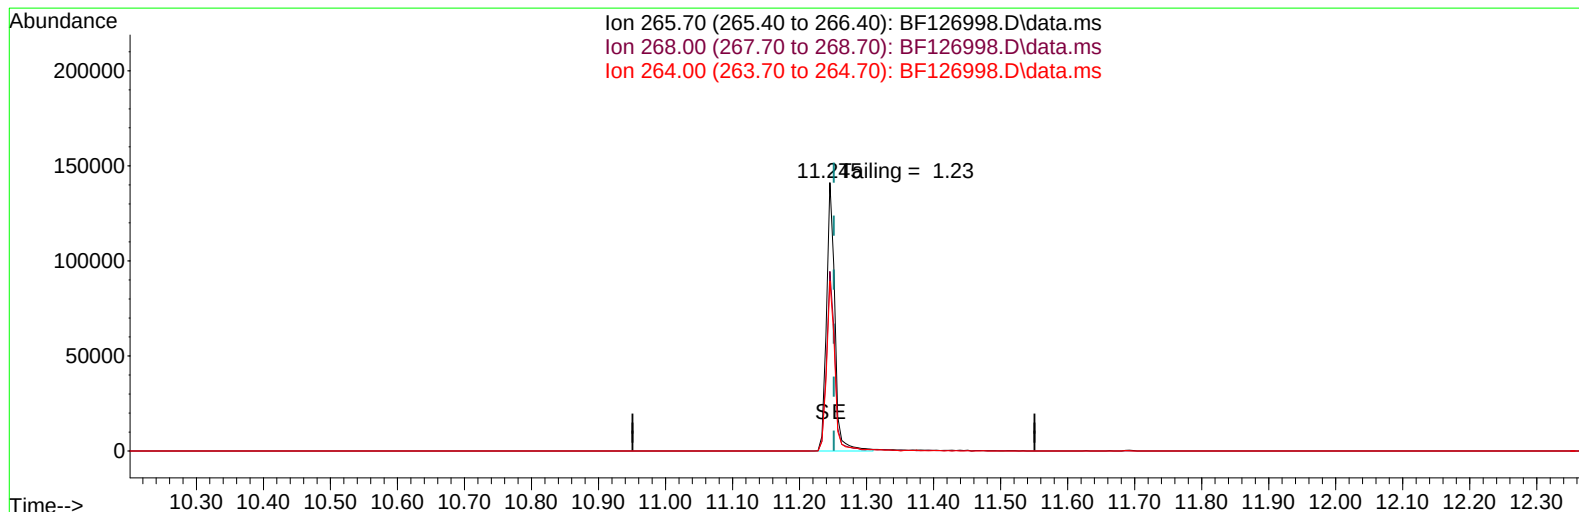

TIC: BF126998.D\data.ms

(70) Pentachlorophenol (C)




11.245min (-0.006) 24013.22 ng

response 124244

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.90
264.00	63.00	63.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022222\
 Data File : BF126998.D
 Acq On : 22 Feb 2022 09:36
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 12:22:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 21 13:16:57 2022
 Response via : Initial Calibration

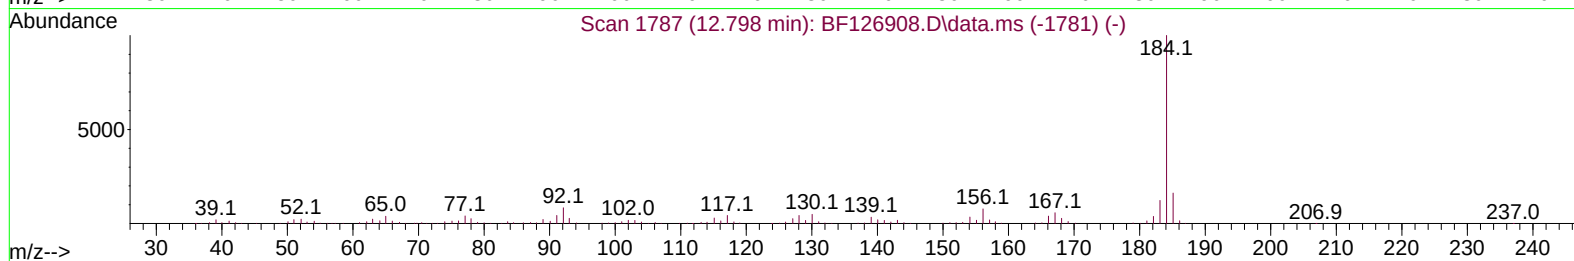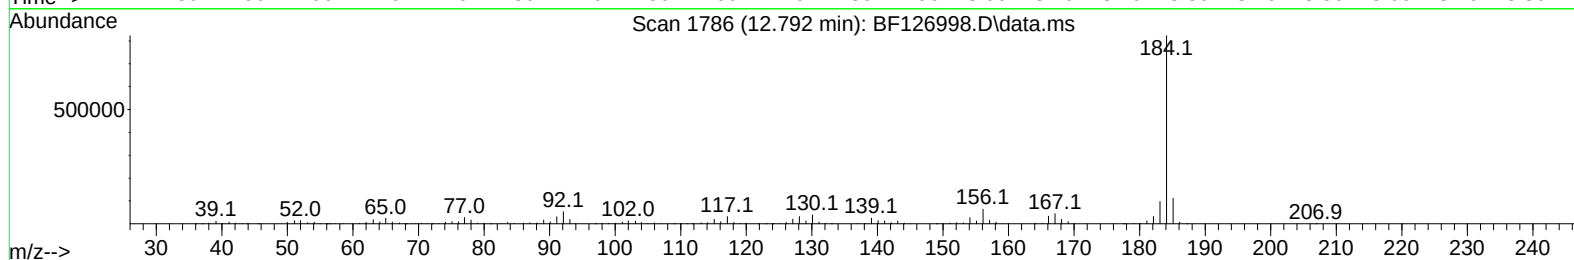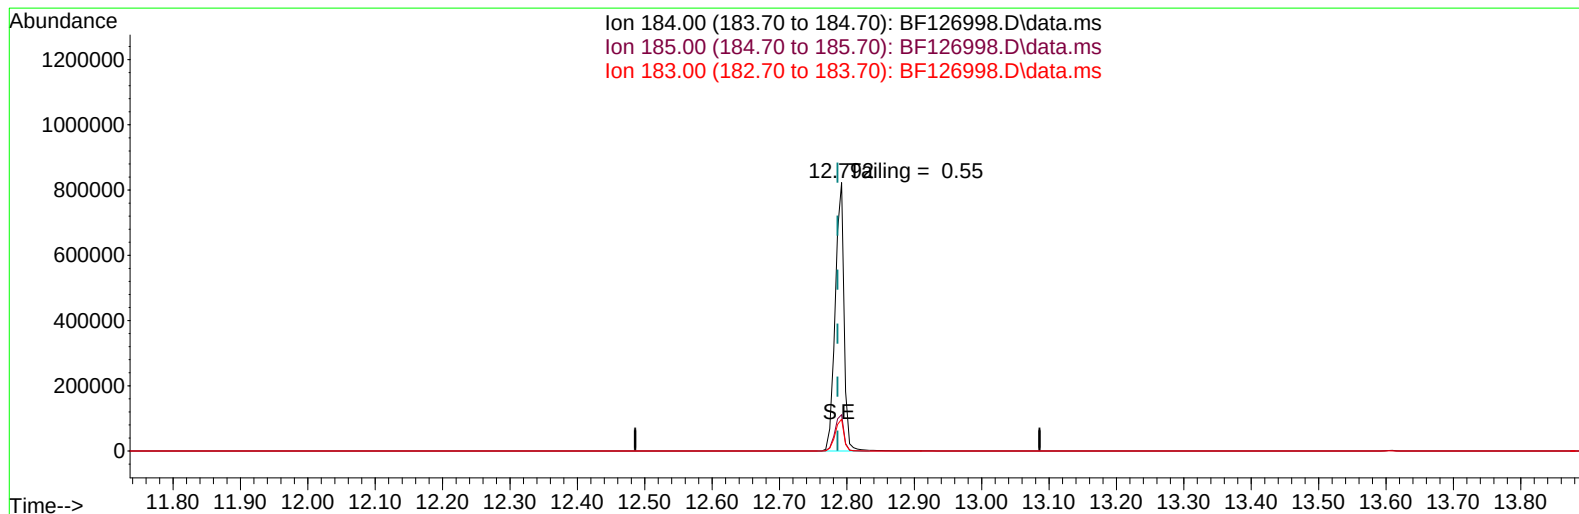

TIC: BF126998.D\data.ms

(77) Benzidine

12.792min (+ 0.006) 0.00 ng

response 748291

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.57
183.00	10.20	11.88
0.00	0.00	0.00