
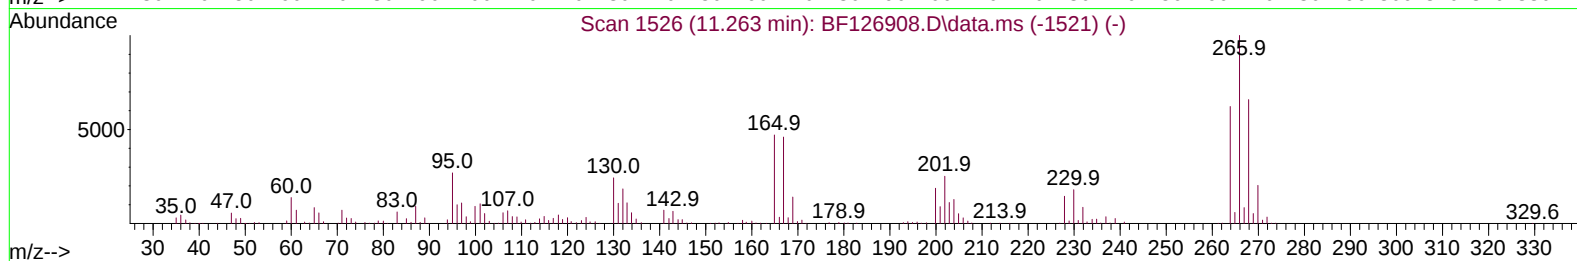
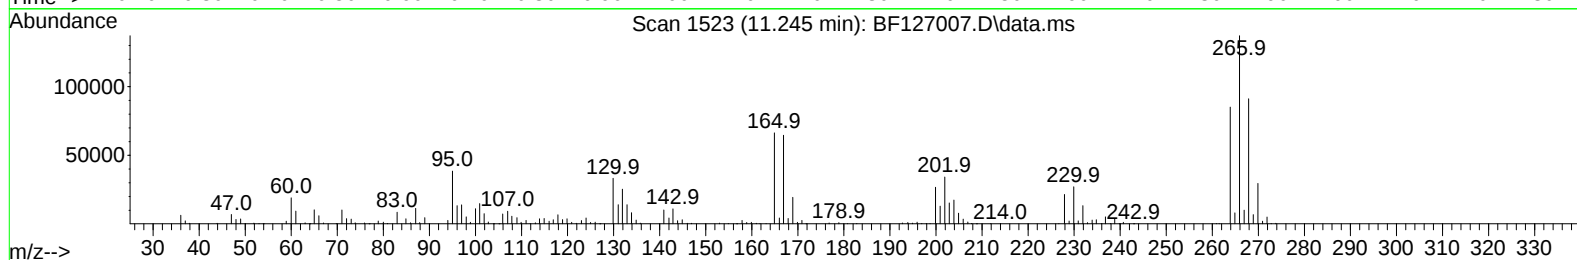


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022222\
Data File : BF127007.D
Acq On : 22 Feb 2022 14:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 07:38:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 21 13:16:57 2022
Response via : Initial Calibration

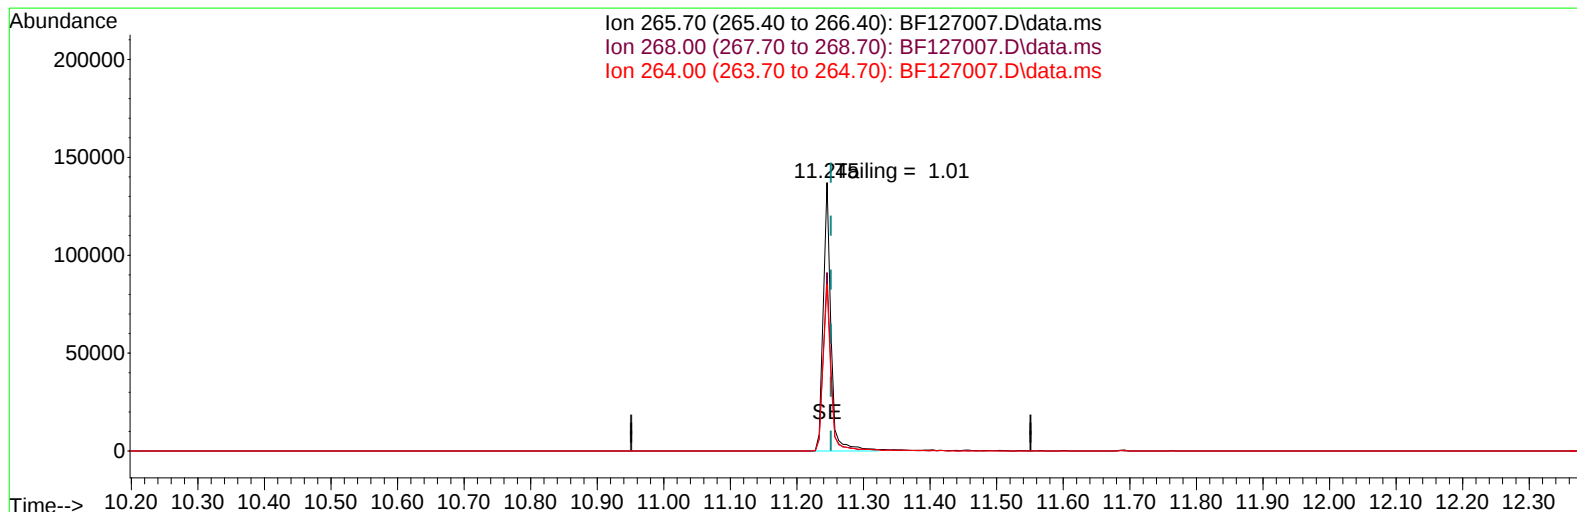

TIC: BF127007.D\data.ms

(70) Pentachlorophenol (C)




11.245min (-0.006) 27438.08 ng

response 112058

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.48
264.00	63.00	62.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022222\
Data File : BF127007.D
Acq On : 22 Feb 2022 14:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 07:38:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 21 13:16:57 2022
Response via : Initial Calibration

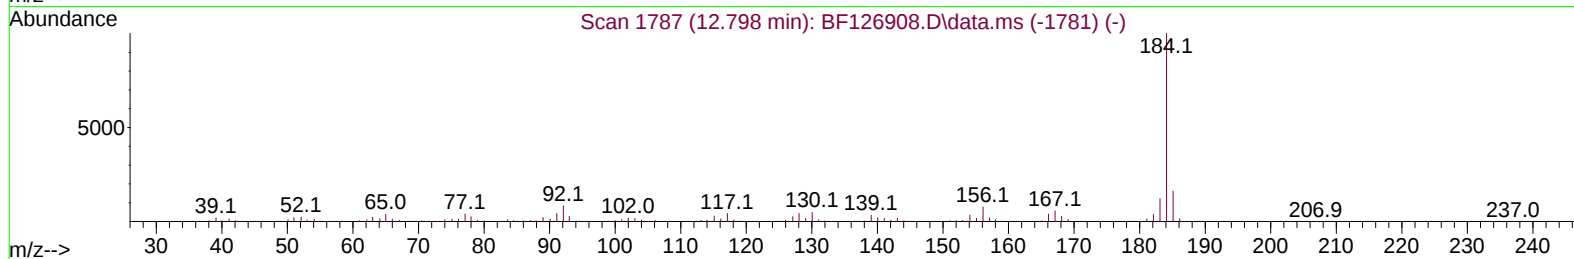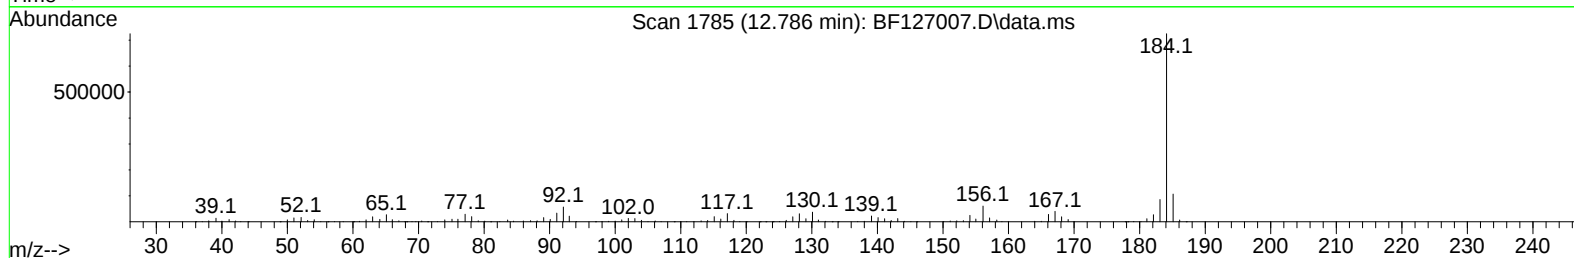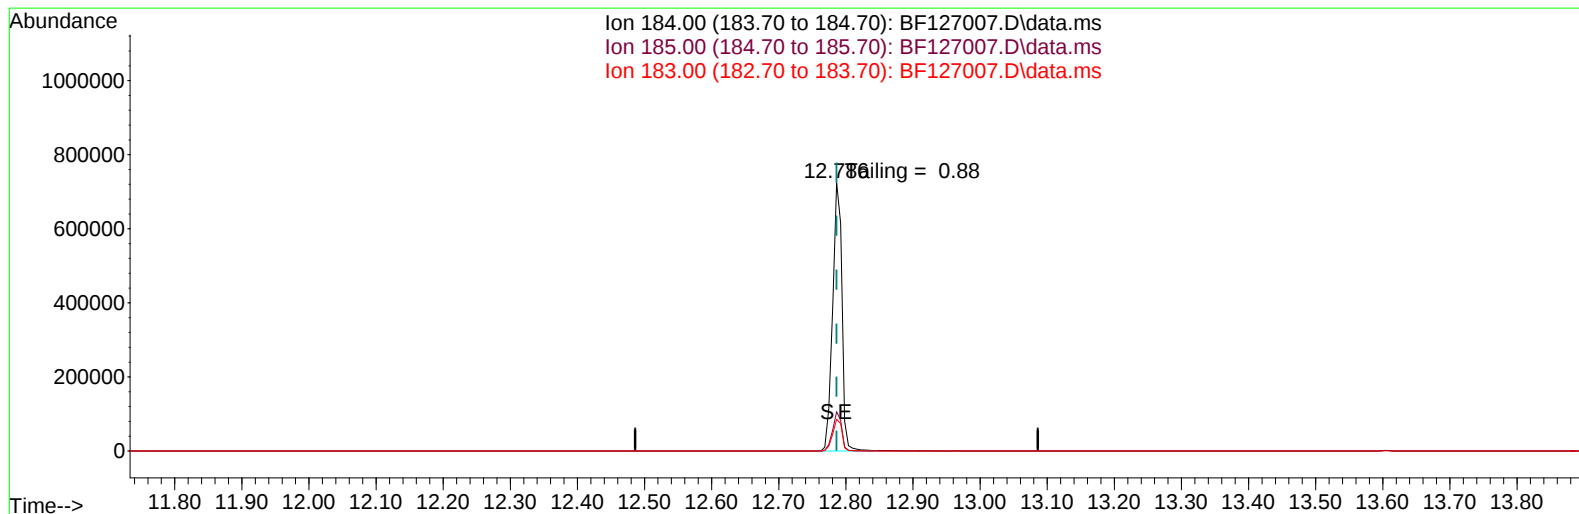

TIC: BF127007.D\data.ms

(77) Benzidine

12.786min (+ 0.000) 0.00 ng

response 700828

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.71
183.00	10.20	11.89
0.00	0.00	0.00