

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022222\
 Data File : BF127003.D
 Acq On : 22 Feb 2022 11:56
 Operator : CG\JU
 Sample : PB142794BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB142794BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127003.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.546	549	554	557	rBV	2965008	3012081	68.53%	12.447%
2	6.540	717	723	726	rBV	2659695	3085983	70.22%	12.752%
3	6.916	783	787	790	rBV	787174	615589	14.01%	2.544%
4	7.481	877	883	886	rBV	2082360	2090069	47.56%	8.637%
5	8.198	1000	1005	1008	rBV	970759	829847	18.88%	3.429%
6	9.275	1182	1188	1191	rBV	3815488	3674200	83.60%	15.183%
7	9.957	1299	1304	1307	rBV	1109771	915998	20.84%	3.785%
8	10.751	1433	1439	1442	rBV	2573650	2528881	57.54%	10.450%
9	11.445	1553	1557	1560	rBV	1269673	1001312	22.78%	4.138%
10	12.839	1791	1794	1798	rBV	78694	65306	1.49%	0.270%
11	13.039	1822	1828	1831	rBV	4708221	4395030	100.00%	18.162%
12	13.545	1911	1914	1919	rVB2	57339	49524	1.13%	0.205%
13	14.086	2002	2006	2010	rBV	1007293	892751	20.31%	3.689%
14	15.204	2192	2196	2200	rBV	47595	48012	1.09%	0.198%
15	15.586	2255	2261	2271	rBV	642773	860556	19.58%	3.556%
16	16.051	2334	2340	2348	rBV2	44514	67968	1.55%	0.281%
17	16.580	2423	2430	2438	rBV2	36113	66477	1.51%	0.275%




Sum of corrected areas: 24199584

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022222\
Data File : BF127003.D
Acq On : 22 Feb 2022 11:56
Operator : CG\JU
Sample : PB142794BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142794BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

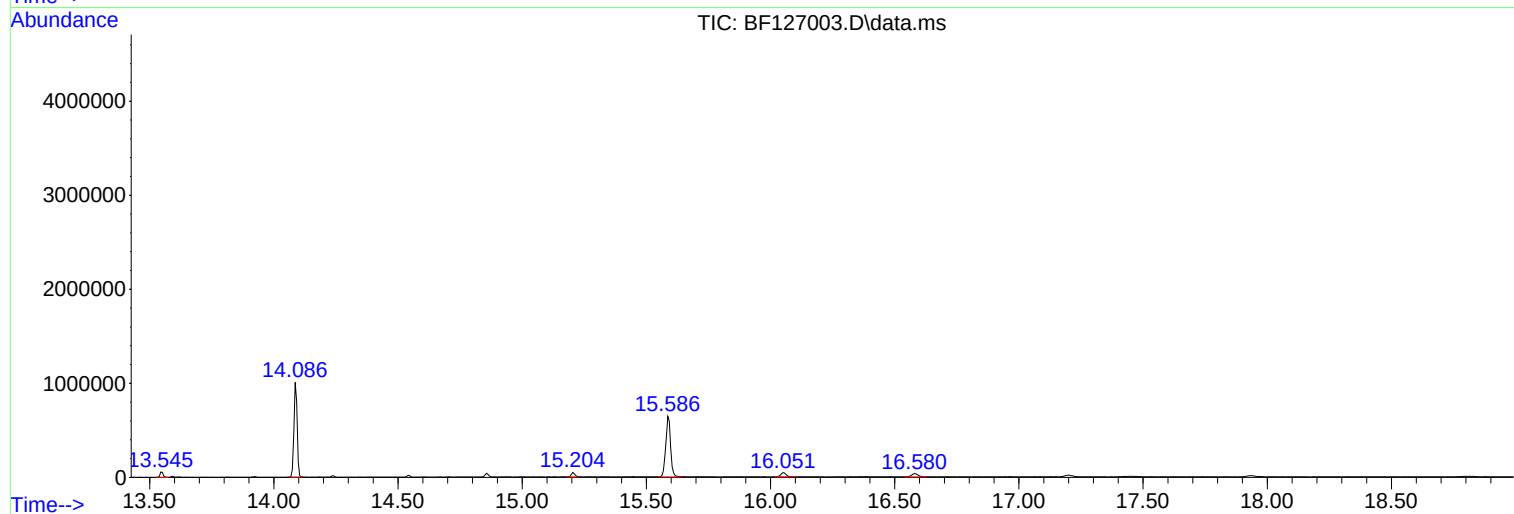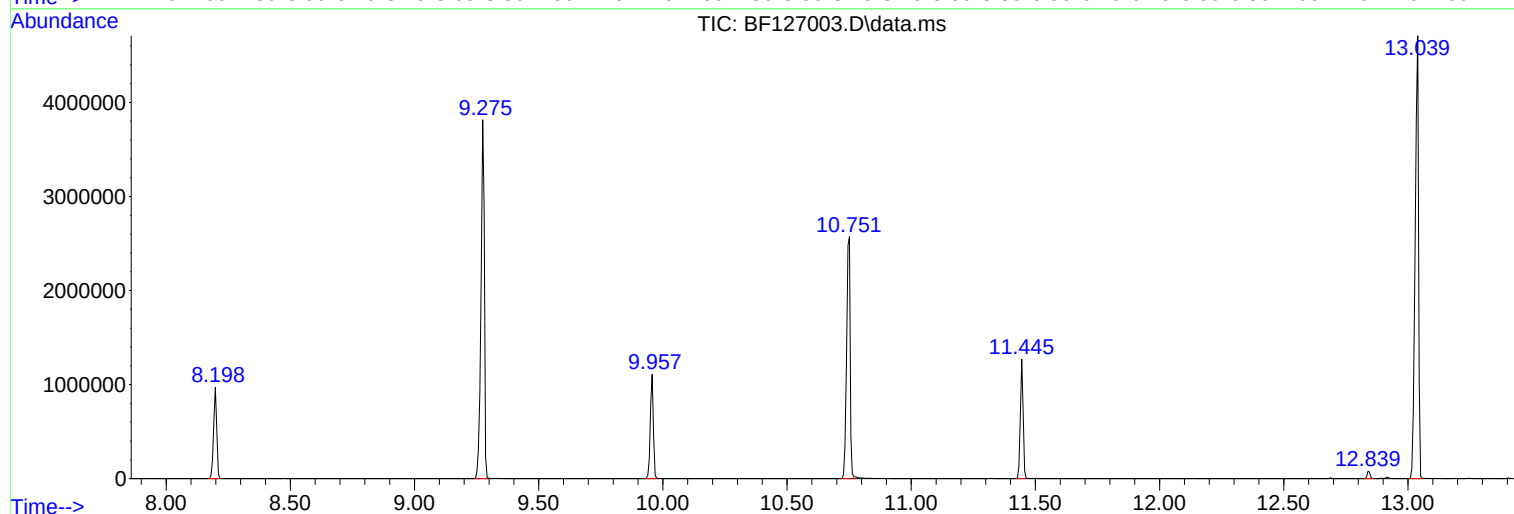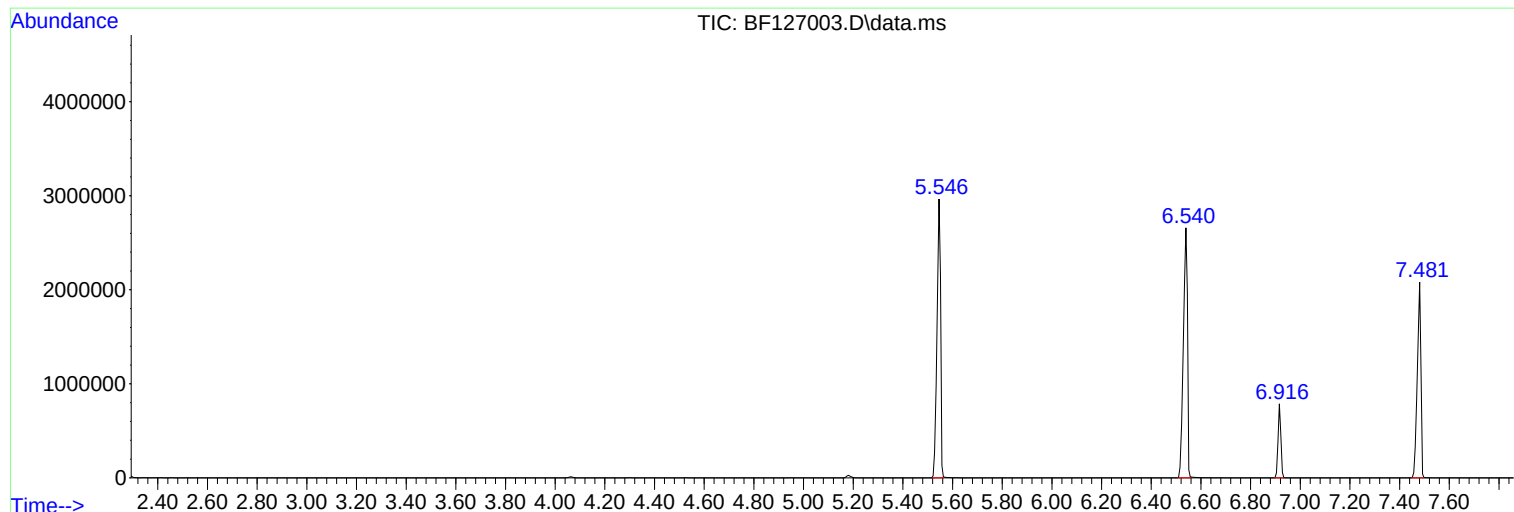

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022222\
Data File : BF127003.D
Acq On : 22 Feb 2022 11:56
Operator : CG\JU
Sample : PB142794BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142794BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022222\
Data File : BF127003.D
Acq On : 22 Feb 2022 11:56
Operator : CG\JU
Sample : PB142794BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142794BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------