

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022222\
 Data File : BF127006.D
 Acq On : 22 Feb 2022 13:50
 Operator : CG\JU
 Sample : PB142770BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB142770BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127006.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.546	549	554	557	rBV	2851345	2977490	67.83%	12.485%
2	6.540	717	723	726	rBV	2752754	3017926	68.76%	12.655%
3	6.916	783	787	790	rBV	796123	603508	13.75%	2.531%
4	7.481	877	883	886	rBV	2101492	2059506	46.92%	8.636%
5	8.198	1000	1005	1008	rBV	958916	814680	18.56%	3.416%
6	9.275	1182	1188	1191	rBV	3960986	3631982	82.74%	15.230%
7	9.957	1299	1304	1307	rBV	1061878	901963	20.55%	3.782%
8	10.745	1433	1438	1442	rBV	2553260	2500426	56.97%	10.485%
9	11.445	1553	1557	1560	rBV	1286042	1005120	22.90%	4.215%
10	12.839	1791	1794	1798	rBV	79611	65896	1.50%	0.276%
11	13.039	1822	1828	1831	rBV	4505879	4389381	100.00%	18.405%
12	13.545	1911	1914	1918	rBV	57768	48826	1.11%	0.205%
13	14.086	2002	2006	2010	rBV	981891	875198	19.94%	3.670%
14	15.204	2192	2196	2203	rBV	44519	51630	1.18%	0.216%
15	15.586	2255	2261	2273	rVB	591740	779508	17.76%	3.269%
16	16.051	2334	2340	2347	rBV2	42826	63552	1.45%	0.266%
17	16.574	2423	2429	2437	rBV3	30980	61725	1.41%	0.259%




Sum of corrected areas: 23848317

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022222\
Data File : BF127006.D
Acq On : 22 Feb 2022 13:50
Operator : CG\JU
Sample : PB142770BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142770BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

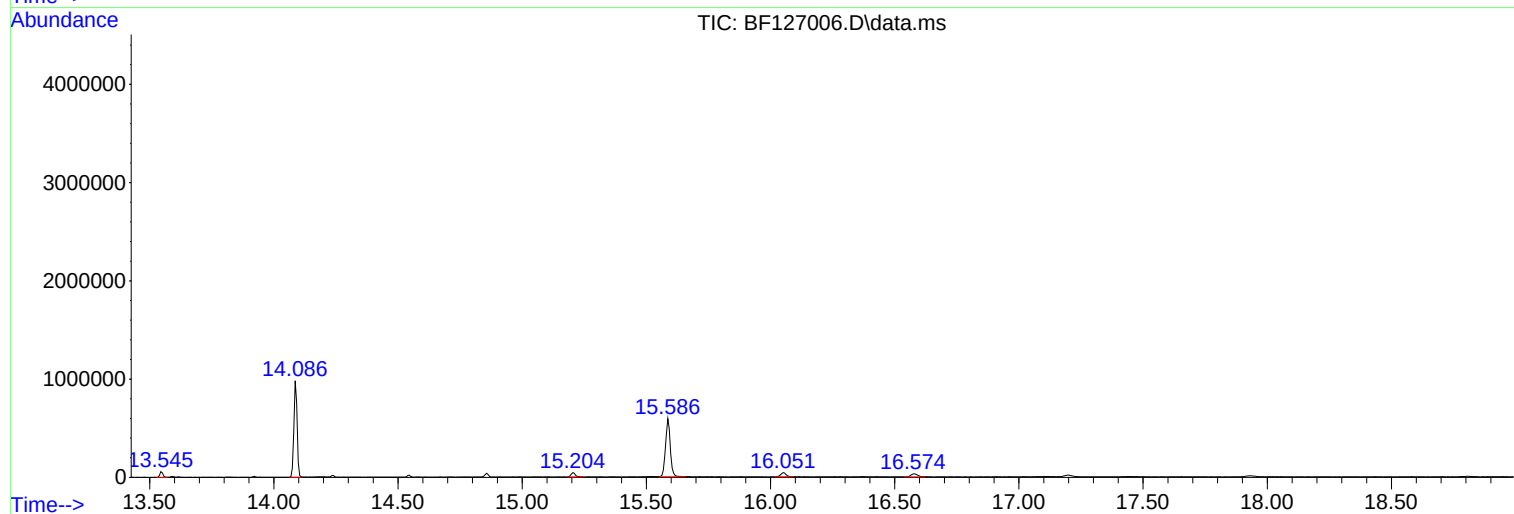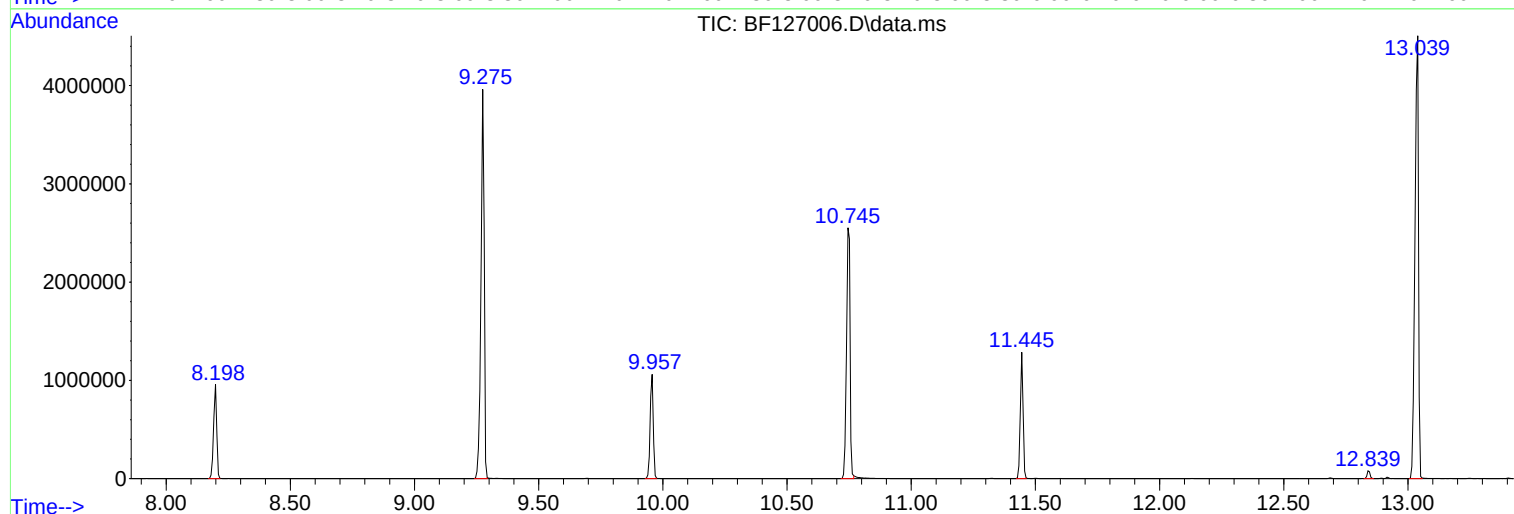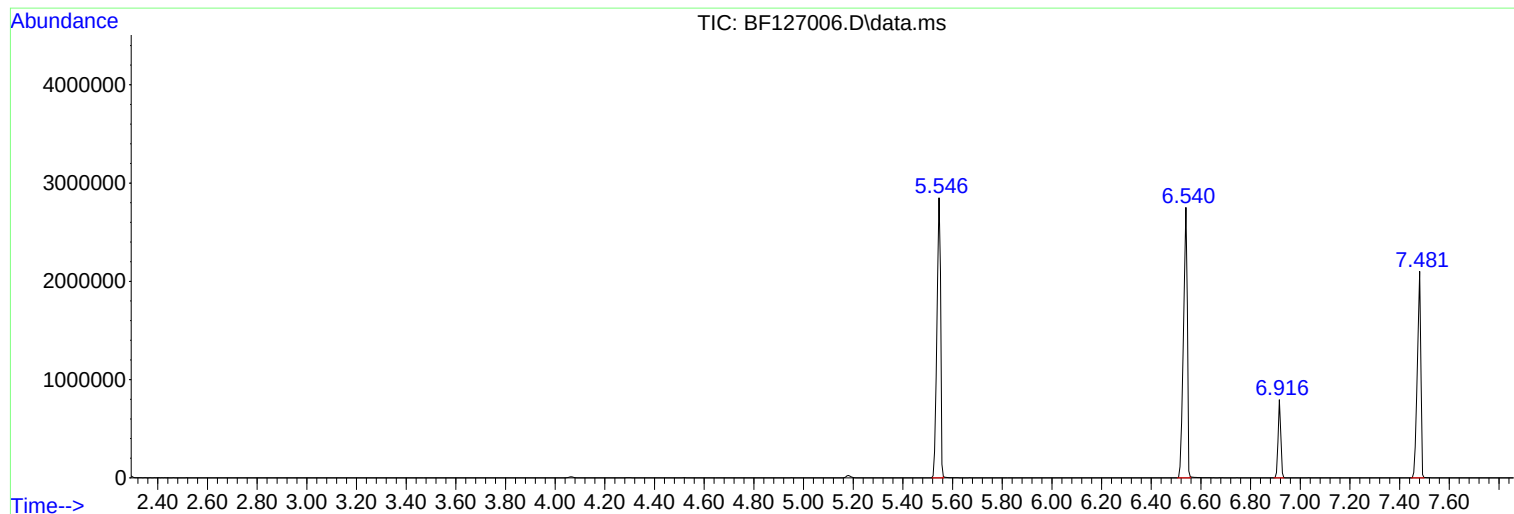

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022222\
Data File : BF127006.D
Acq On : 22 Feb 2022 13:50
Operator : CG\JU
Sample : PB142770BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142770BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022222\
Data File : BF127006.D
Acq On : 22 Feb 2022 13:50
Operator : CG\JU
Sample : PB142770BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142770BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------