

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022222\
 Data File : BF127009.D
 Acq On : 22 Feb 2022 15:22
 Operator : CG\JU
 Sample : PB142832BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB142832BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127009.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.545	549	554	557	rBV	2980449	3024560	68.40%	12.480%
2	6.539	717	723	726	rBV	2749683	3111087	70.36%	12.837%
3	6.916	783	787	790	rBV	797807	620502	14.03%	2.560%
4	7.481	877	883	886	rBV	2081391	2127932	48.13%	8.780%
5	8.198	1000	1005	1008	rBV	1021358	843730	19.08%	3.481%
6	9.274	1182	1188	1191	rBV	3959825	3717343	84.07%	15.339%
7	9.957	1298	1304	1307	rBV	1120894	932852	21.10%	3.849%
8	10.745	1434	1438	1442	rBV	2581665	2516516	56.91%	10.384%
9	11.445	1553	1557	1560	rBV	1239152	1006043	22.75%	4.151%
10	12.839	1791	1794	1798	rVB	75680	61403	1.39%	0.253%
11	13.039	1822	1828	1830	rBV	4462293	4421603	100.00%	18.245%
12	13.545	1911	1914	1919	rBV	55278	46322	1.05%	0.191%
13	14.086	2002	2006	2010	rBV	994935	855874	19.36%	3.532%
14	15.204	2192	2196	2200	rBV	42587	47015	1.06%	0.194%
15	15.586	2255	2261	2273	rBV	580996	769546	17.40%	3.175%
16	16.051	2333	2340	2348	rBV	44187	71012	1.61%	0.293%
17	16.580	2420	2430	2437	rBV	35369	61632	1.39%	0.254%




Sum of corrected areas: 24234972

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022222\
Data File : BF127009.D
Acq On : 22 Feb 2022 15:22
Operator : CG\JU
Sample : PB142832BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142832BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

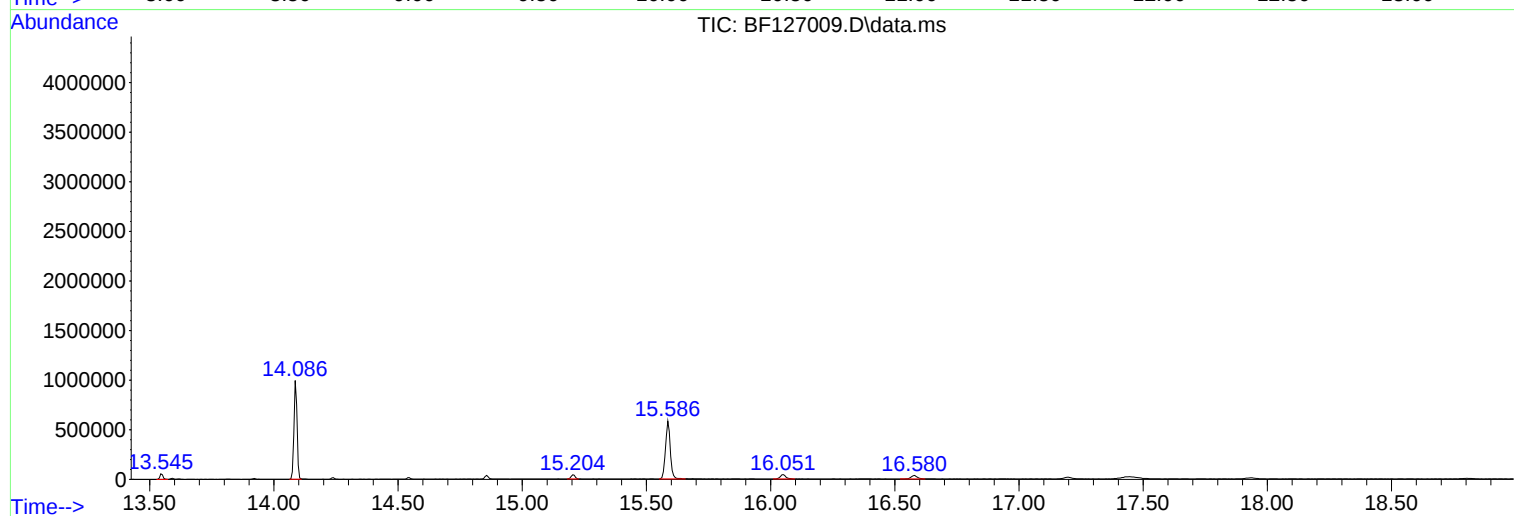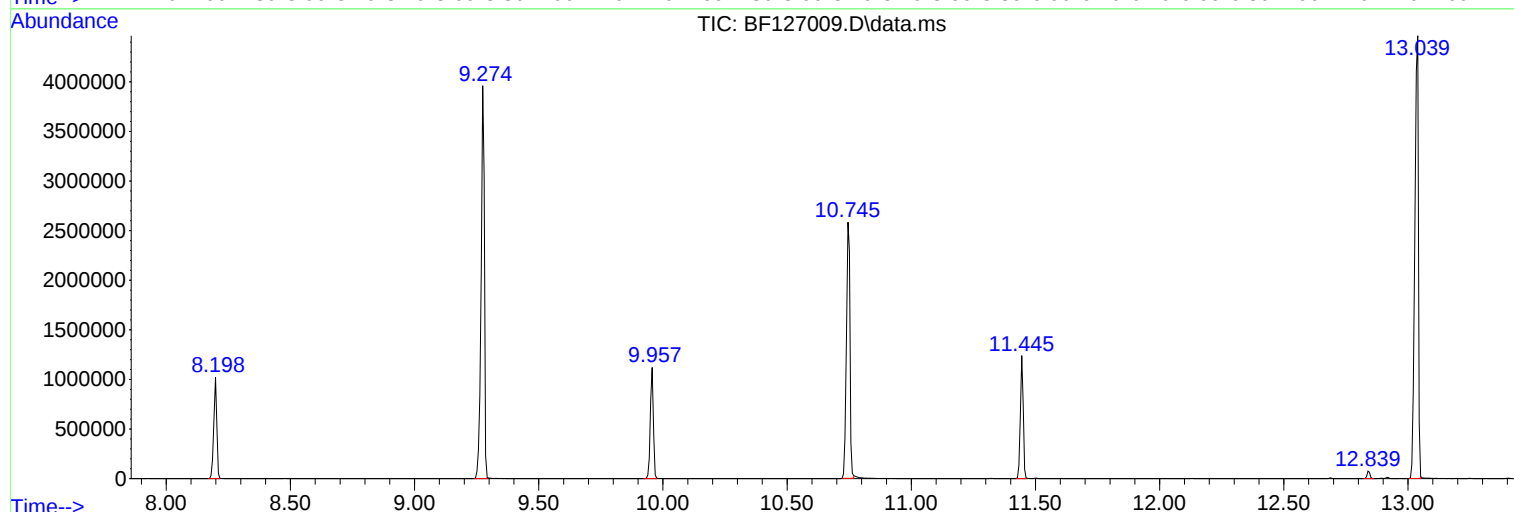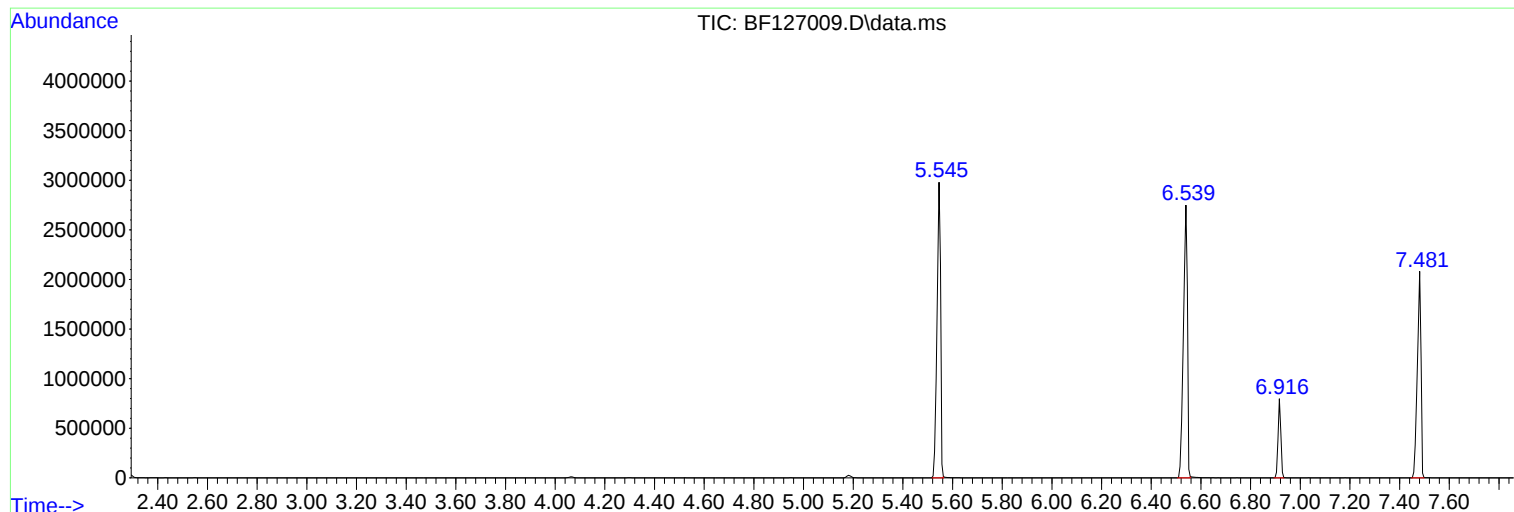

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022222\
Data File : BF127009.D
Acq On : 22 Feb 2022 15:22
Operator : CG\JU
Sample : PB142832BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142832BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022222\
Data File : BF127009.D
Acq On : 22 Feb 2022 15:22
Operator : CG\JU
Sample : PB142832BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142832BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------