
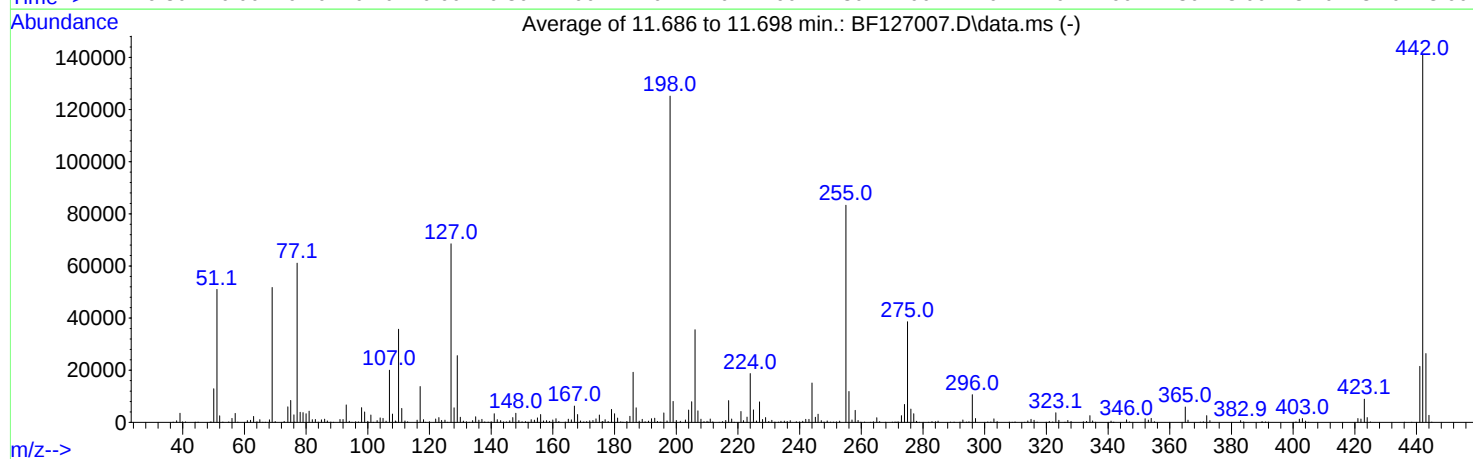


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022222\
 Data File : BF127007.D
 Acq On : 22 Feb 2022 14:19
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 21 13:16:57 2022

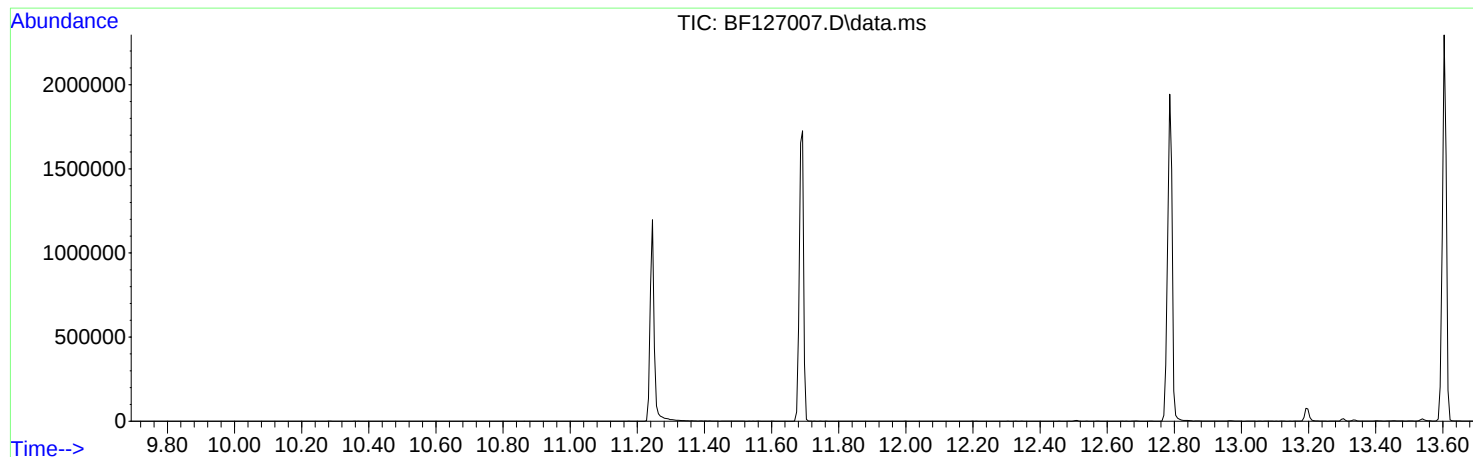




AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.8	51002	PASS
68	69	0.00	2	1.9	976	PASS
69	198	0.00	100	41.4	51762	PASS
70	69	0.00	2	0.6	313	PASS
127	198	10	80	54.7	68511	PASS
197	198	0.00	2	0.4	550	PASS
198	198	100	100	100.0	125144	PASS
199	198	5	9	6.4	8062	PASS
275	198	10	60	30.9	38629	PASS
365	198	1	100	4.7	5917	PASS
441	198	0.01	100	17.2	21499	PASS
442	442	50	100	100.0	141120	PASS
443	442	15	24	18.7	26398	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022222\
 Data File : BF127007.D
 Acq On : 22 Feb 2022 14:19
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 23 07:38:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 21 13:16:57 2022
 Response via : Initial Calibration

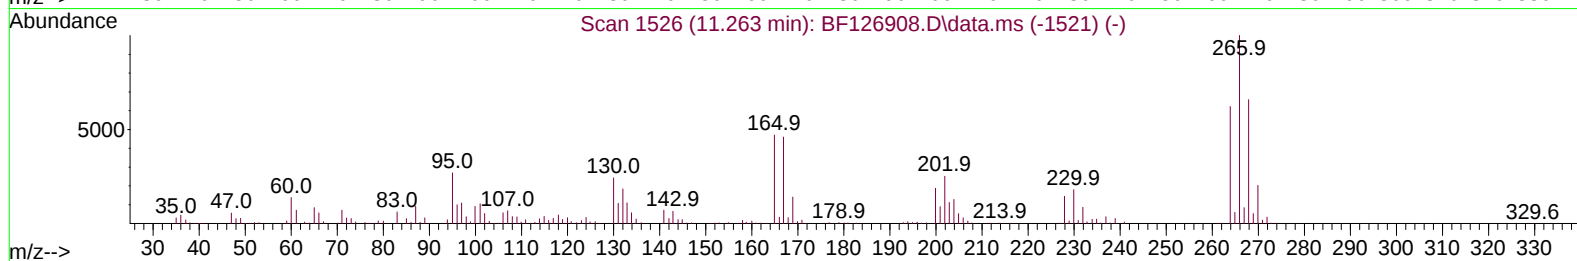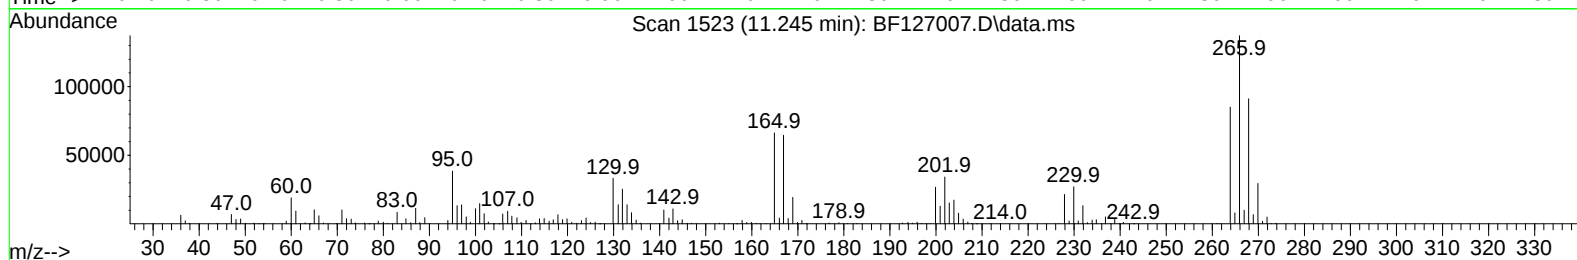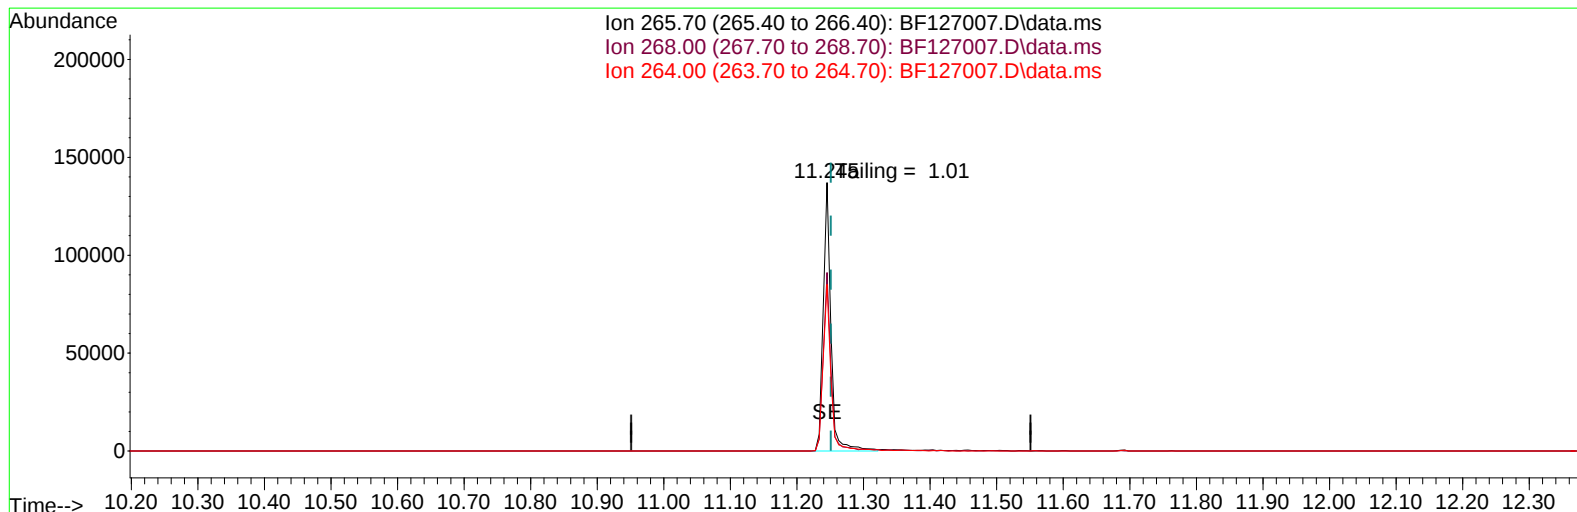

TIC: BF127007.D\data.ms

(70) Pentachlorophenol (C)

11.245min (-0.006) 27438.08 ng




response 112058

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.48
264.00	63.00	62.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022222\
Data File : BF127007.D
Acq On : 22 Feb 2022 14:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 23 07:38:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 21 13:16:57 2022
Response via : Initial Calibration

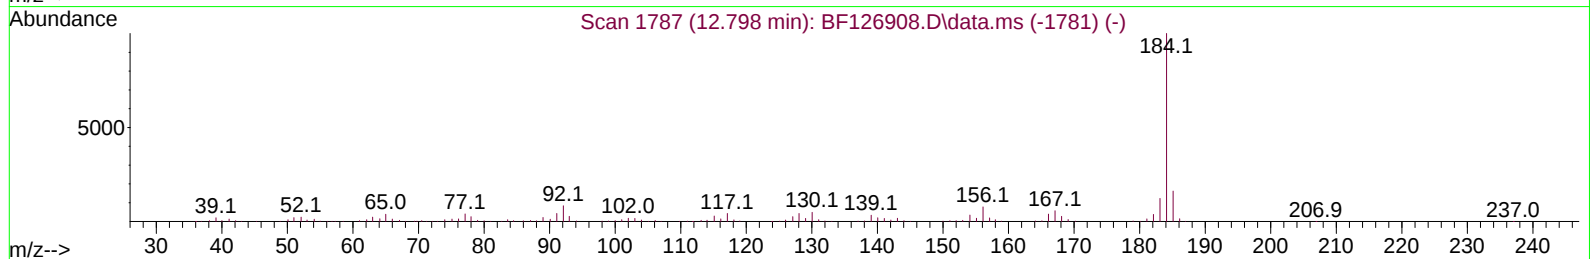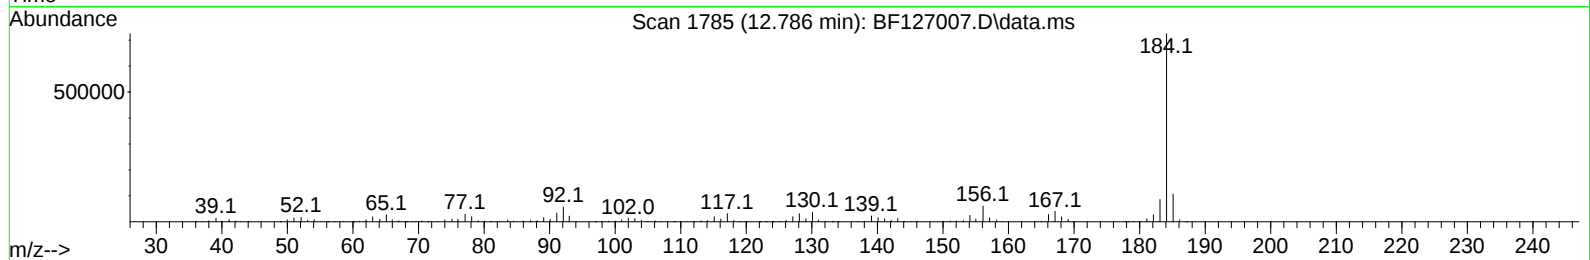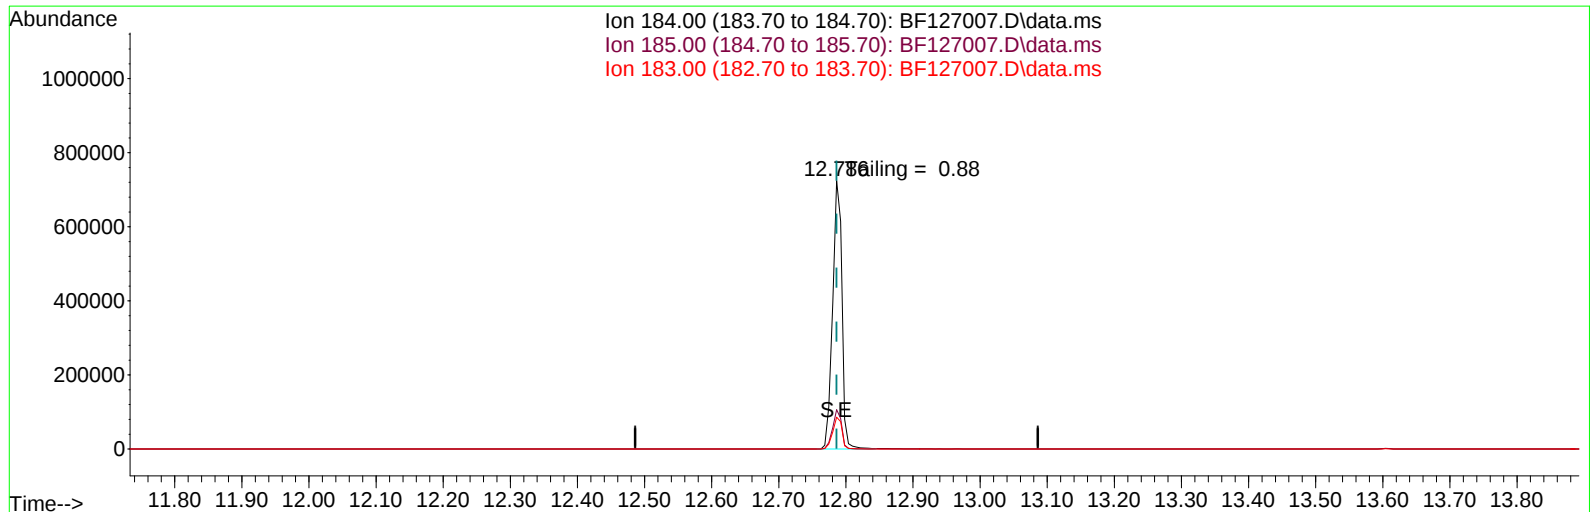

TIC: BF127007.D\data.ms

(77) Benzidine

12.786min (+ 0.000) 0.00 ng

response 700828

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.71
183.00	10.20	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/22/2022	BNA_F	<u>BF127007.D</u>
Compound Name	Response	Retention Time
DDT	340330	13.604
DDD	4174	13.304
DDE	514	12.969
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4688	345018	1.36

Instrument :
BNA_F
ClientSampled :
DFTPP