
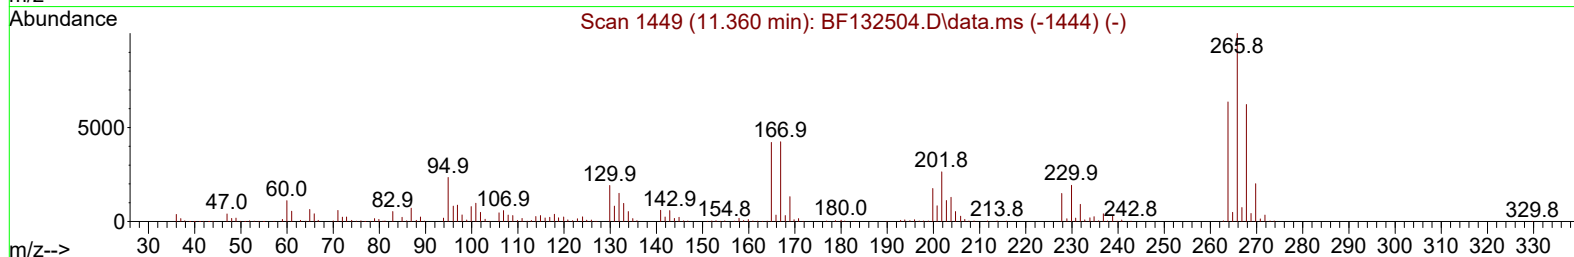
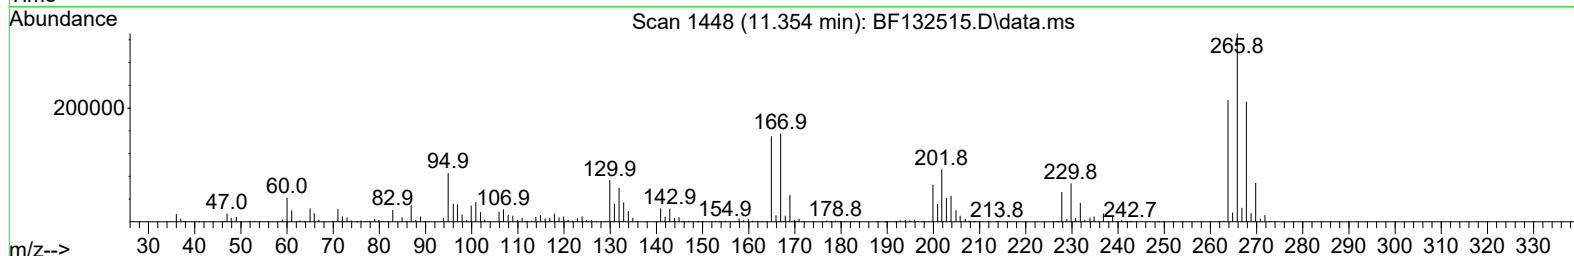


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022323\
Data File : BF132515.D
Acq On : 23 Feb 2023 12:04
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 24 03:29:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 23 00:59:42 2023
Response via : Initial Calibration

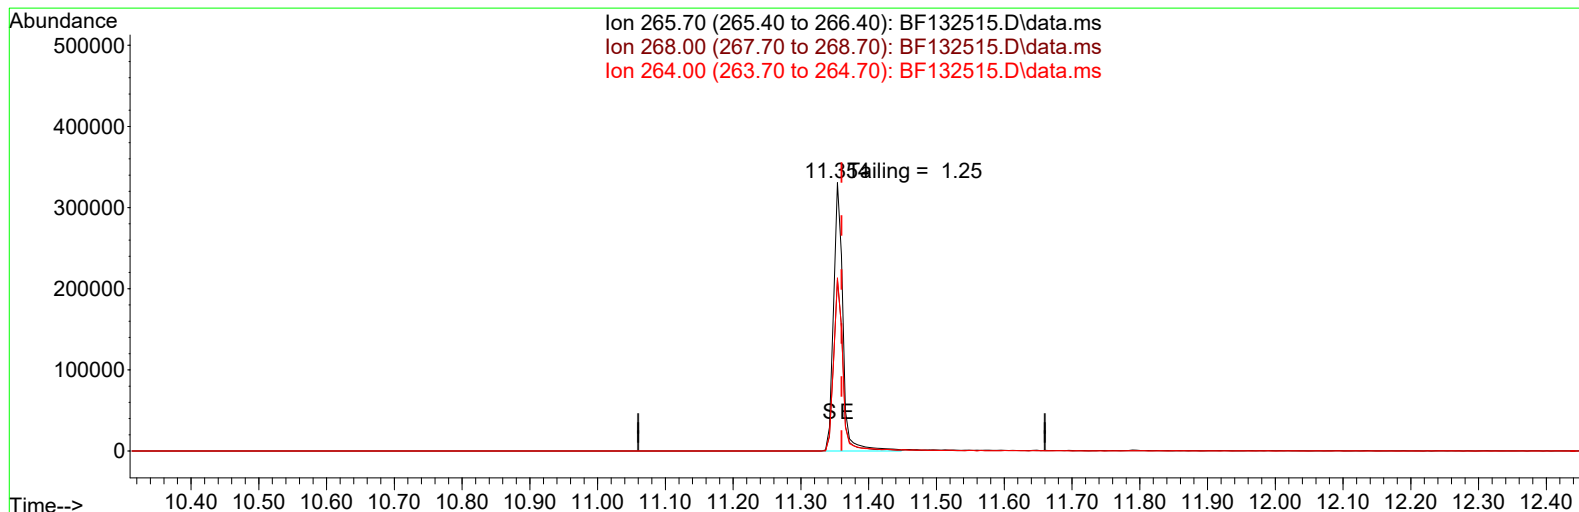

TIC: BF132515.D\data.ms

(70) Pentachlorophenol (C)




11.354min (-0.006) 446437.59 ng

response 316145

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.66
264.00	63.60	64.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022323\
Data File : BF132515.D
Acq On : 23 Feb 2023 12:04
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 24 03:29:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 23 00:59:42 2023
Response via : Initial Calibration

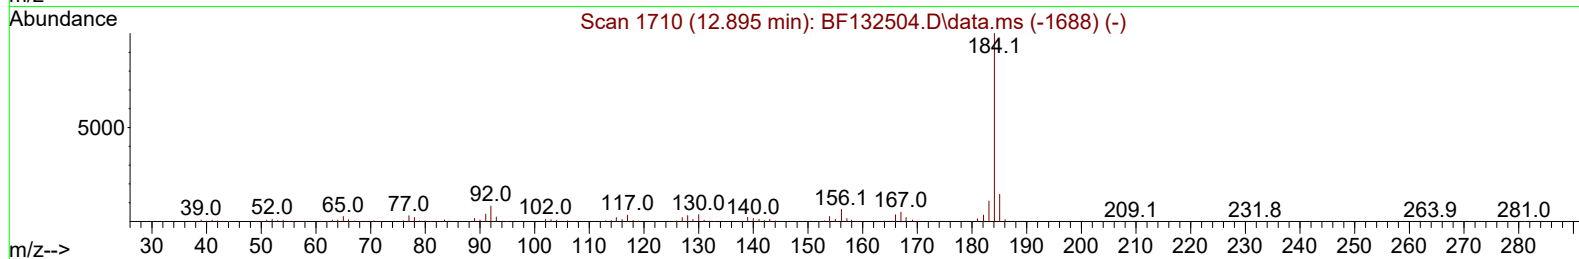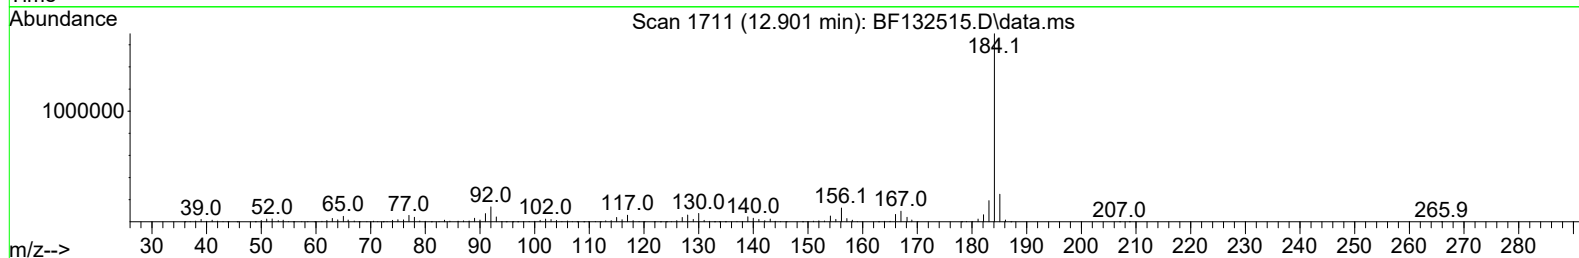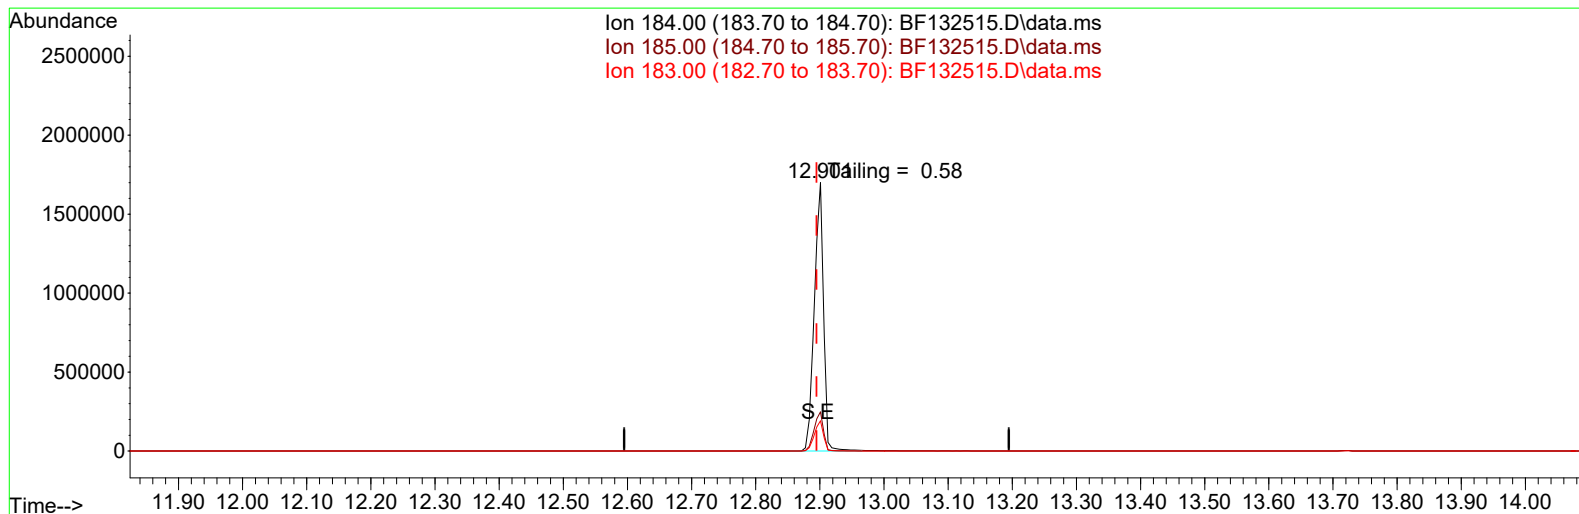

TIC: BF132515.D\data.ms

(77) Benzidine**12.901min (+ 0.006) 1068509.59 ng****response 1716698**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.65
183.00	10.90	11.28
0.00	0.00	0.00