

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022323\
 Data File : BF132519.D
 Acq On : 23 Feb 2023 14:22
 Operator : CG\JU
 Sample : PB151028BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB151028BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF132519.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.660	307	310	319	rBV	72325	87865	1.25%	0.204%
2	5.260	406	412	427	rVB	1872572	2637062	37.61%	6.108%
3	5.648	473	478	481	rBV	5010703	5241465	74.75%	12.140%
4	6.637	641	646	649	rBV	4412428	5276578	75.25%	12.221%
5	7.007	705	709	712	rBV	1411715	1119054	15.96%	2.592%
6	7.572	799	805	808	rBV	3301798	3625622	51.70%	8.397%
7	8.295	923	928	931	rBV	1550424	1444710	20.60%	3.346%
8	9.372	1104	1111	1114	rBV	6649313	6095064	86.92%	14.117%
9	10.054	1223	1227	1231	rBV	2081358	1692162	24.13%	3.919%
10	10.854	1358	1363	1366	rBV	4149679	4149804	59.18%	9.611%
11	11.548	1477	1481	1485	rBV	1989371	1826872	26.05%	4.231%
12	13.148	1747	1753	1756	rBV	6954135	7012354	100.00%	16.241%
13	14.207	1929	1933	1937	rBV	1820622	1626240	23.19%	3.767%
14	15.759	2191	2197	2207	rBV	979885	1341358	19.13%	3.107%




Sum of corrected areas: 43176210

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022323\
Data File : BF132519.D
Acq On : 23 Feb 2023 14:22
Operator : CG\JU
Sample : PB151028BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB151028BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

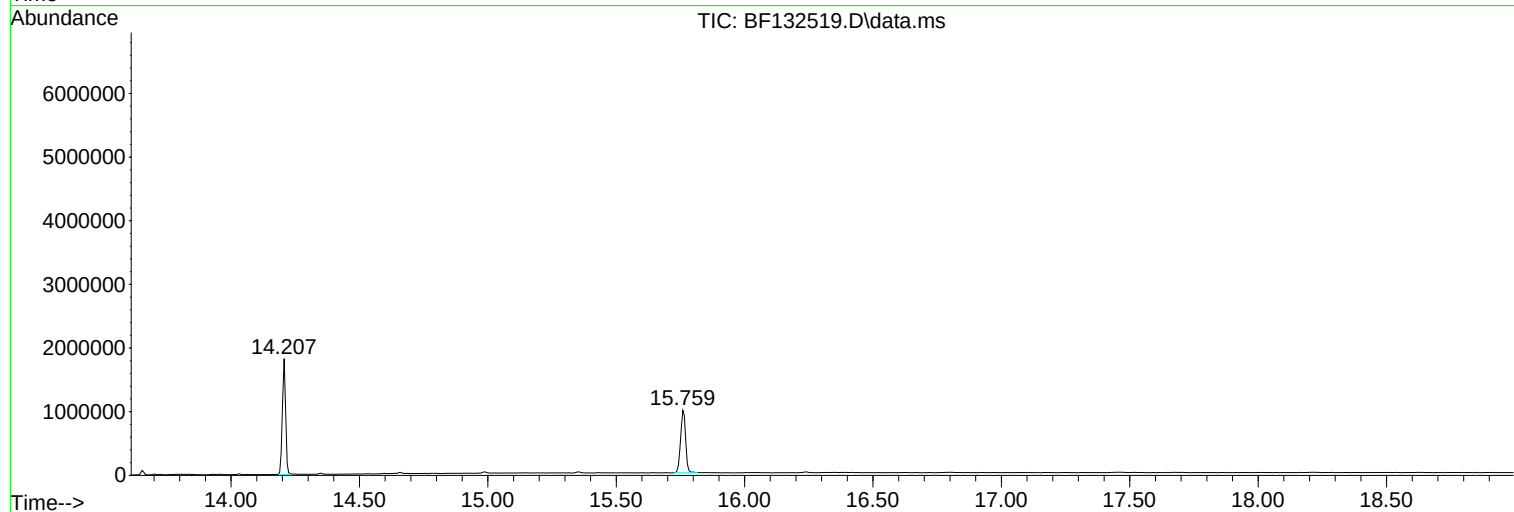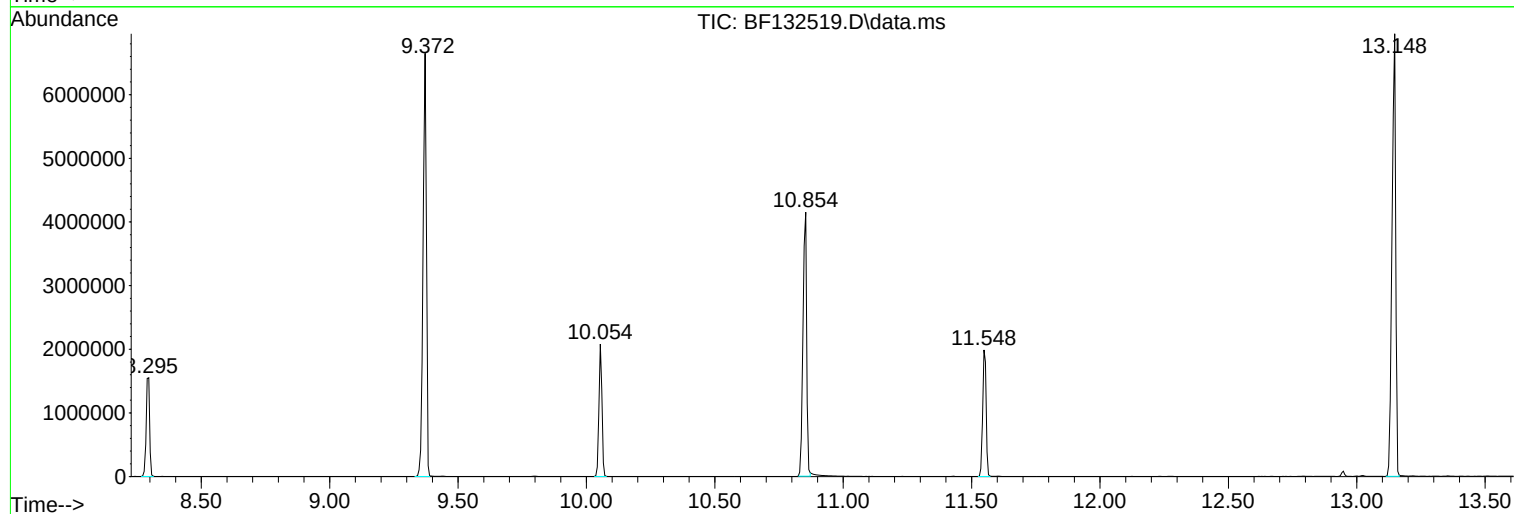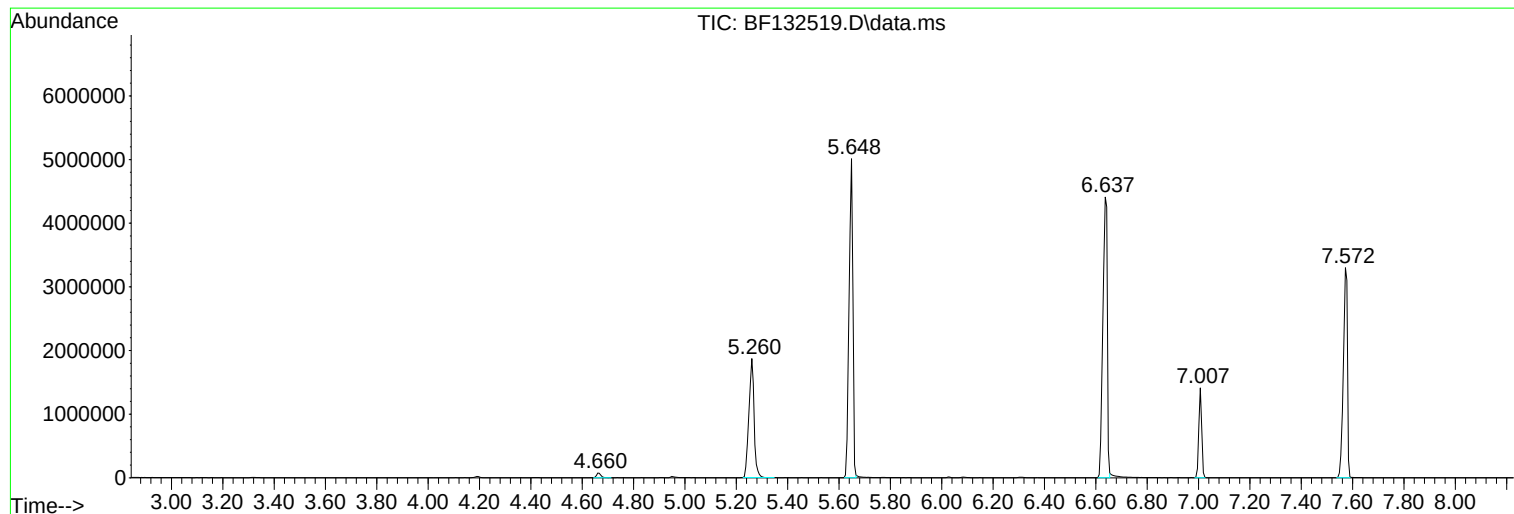

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022323\
Data File : BF132519.D
Acq On : 23 Feb 2023 14:22
Operator : CG\JU
Sample : PB151028BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB151028BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.260	47.13 ng	2637060	1,4-Dichlorobenzene-d4	7.007

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17
3			Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9
4			Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9
5			5-Hexen-2-one	98	C6H10O	000109-49-9	9

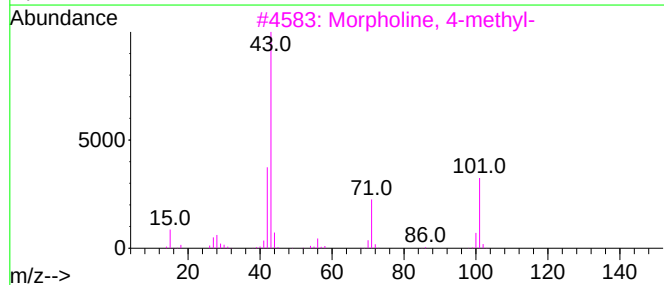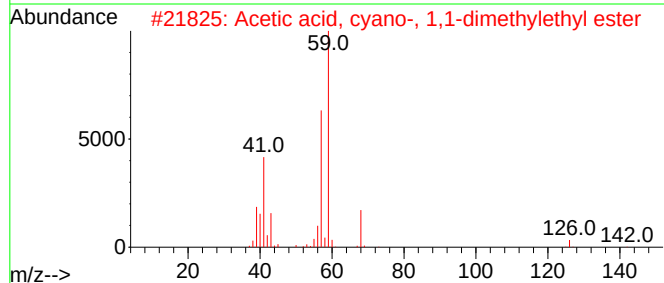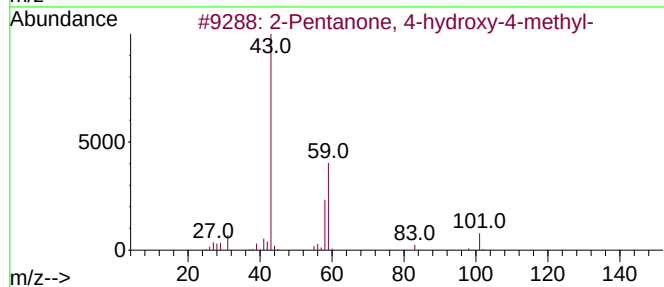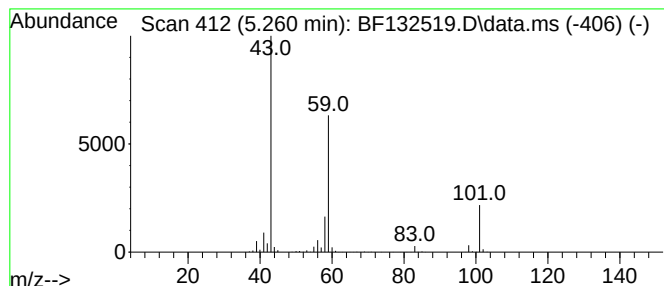

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022323\
Data File : BF132519.D
Acq On : 23 Feb 2023 14:22
Operator : CG\JU
Sample : PB151028BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB151028BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.260	47.1	ng	2637060	1	7.007	1119050	20.0