

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022422\
 Data File : BF127056.D
 Acq On : 24 Feb 2022 14:28
 Operator : CG\JU
 Sample : PB142894BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB142894BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127056.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.534	547	552	555	rBV	2527295	2360011	58.98%	11.886%
2	6.534	717	722	725	rBV	2340825	2448641	61.20%	12.332%
3	6.904	781	785	788	rBV	599939	465436	11.63%	2.344%
4	7.469	875	881	884	rBV	1768221	1686464	42.15%	8.494%
5	8.186	999	1003	1007	rBV	683540	630682	15.76%	3.176%
6	9.263	1181	1186	1189	rBV	3121643	3150678	78.75%	15.868%
7	9.945	1297	1302	1306	rBV	761510	722053	18.05%	3.637%
8	10.745	1431	1438	1441	rBV	2394445	2349201	58.71%	11.832%
9	11.439	1552	1556	1560	rBV	967670	805418	20.13%	4.056%
10	13.033	1822	1827	1830	rBV	4197607	4001036	100.00%	20.151%
11	14.086	2002	2006	2010	rBV	768637	683071	17.07%	3.440%
12	15.592	2257	2262	2267	rVB	444090	552742	13.81%	2.784%




Sum of corrected areas: 19855433

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022422\
Data File : BF127056.D
Acq On : 24 Feb 2022 14:28
Operator : CG\JU
Sample : PB142894BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142894BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

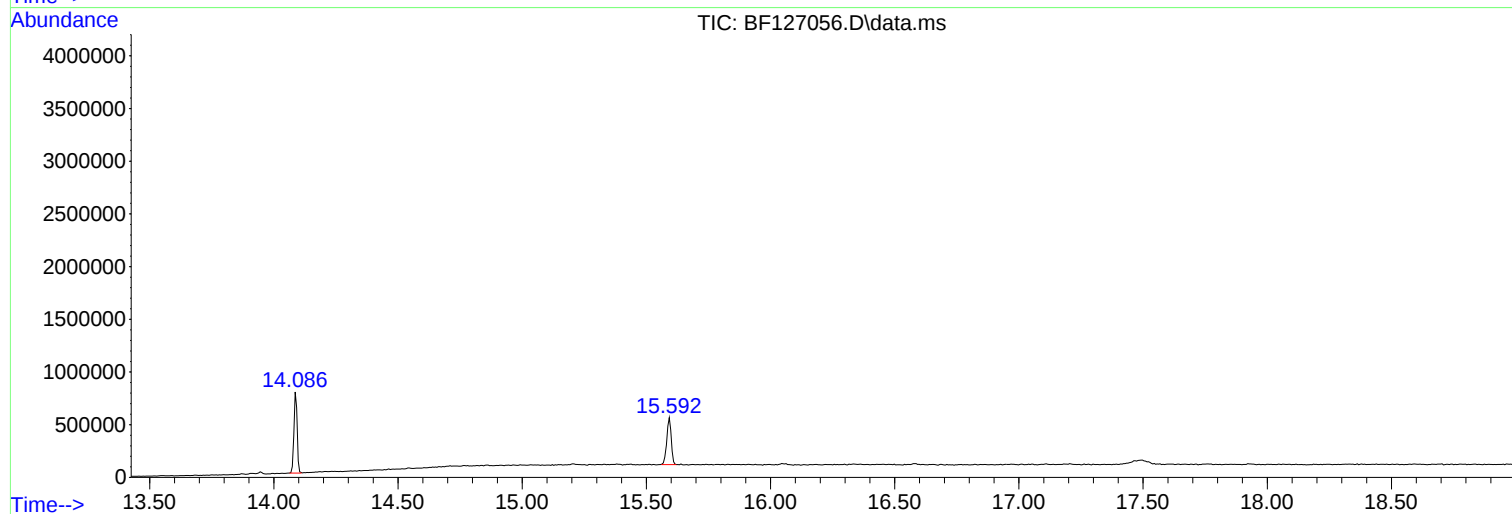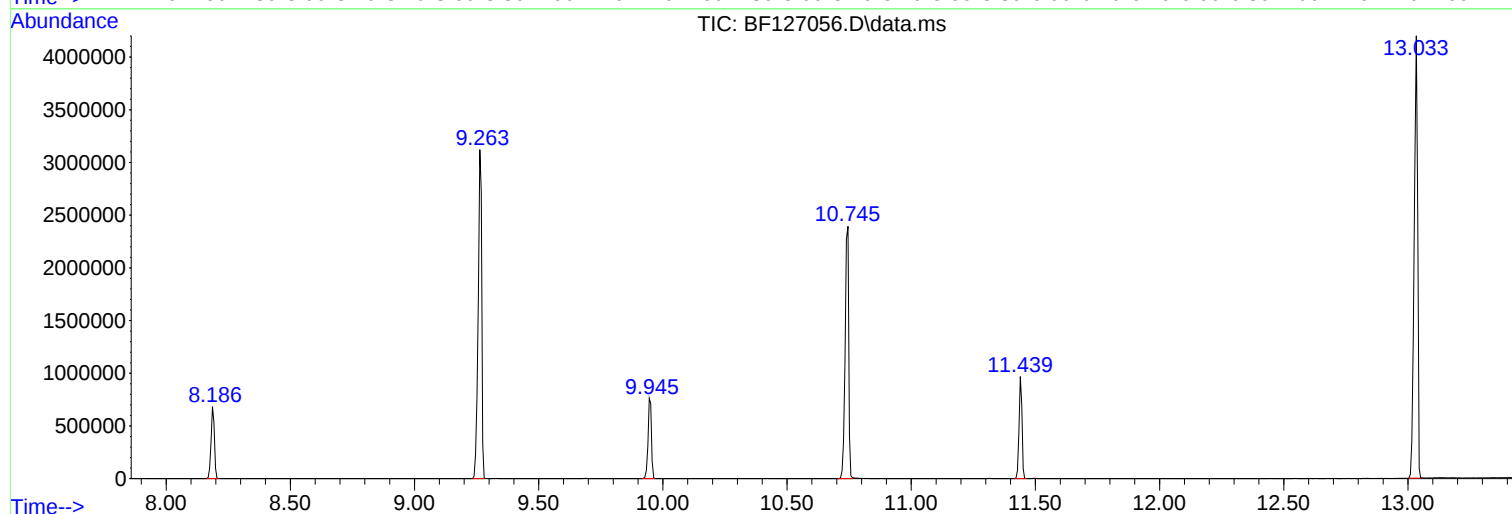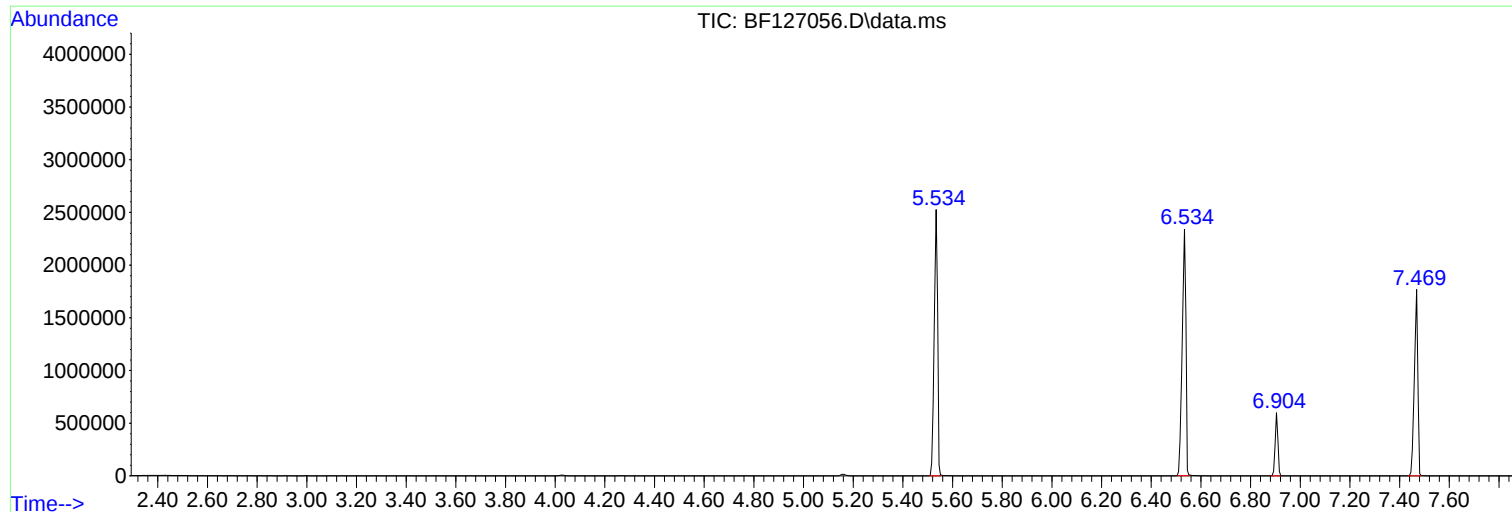

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022422\
Data File : BF127056.D
Acq On : 24 Feb 2022 14:28
Operator : CG\JU
Sample : PB142894BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142894BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022422\
Data File : BF127056.D
Acq On : 24 Feb 2022 14:28
Operator : CG\JU
Sample : PB142894BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142894BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------