
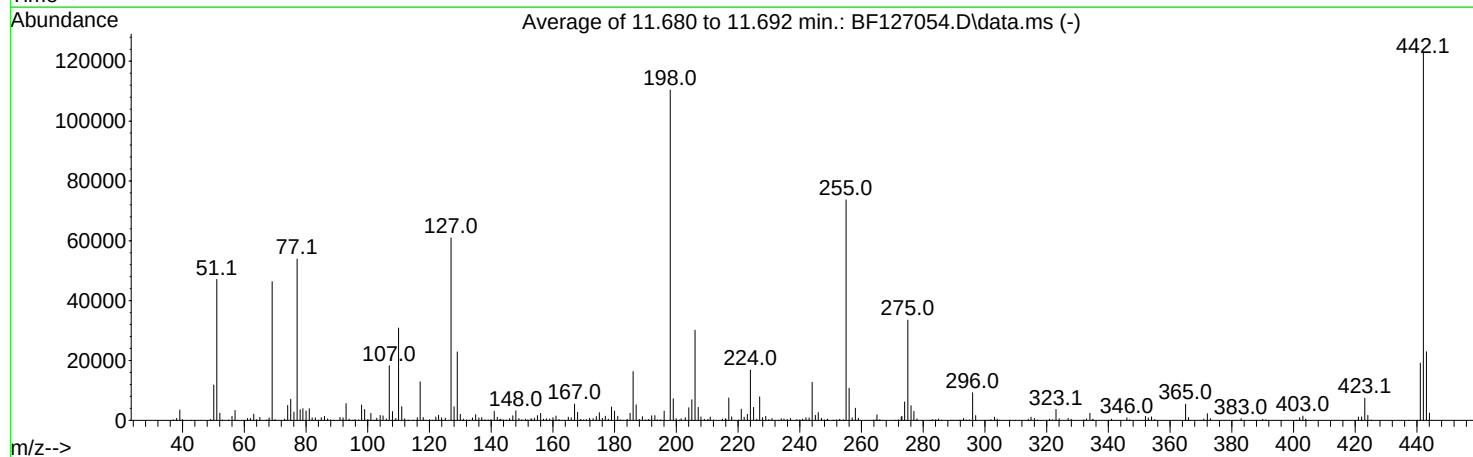


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF-2022\BF-FEB-22\BF022422\
 Data File : BF127054.D
 Acq On : 24 Feb 2022 13:18
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 05 02:16:58 2022

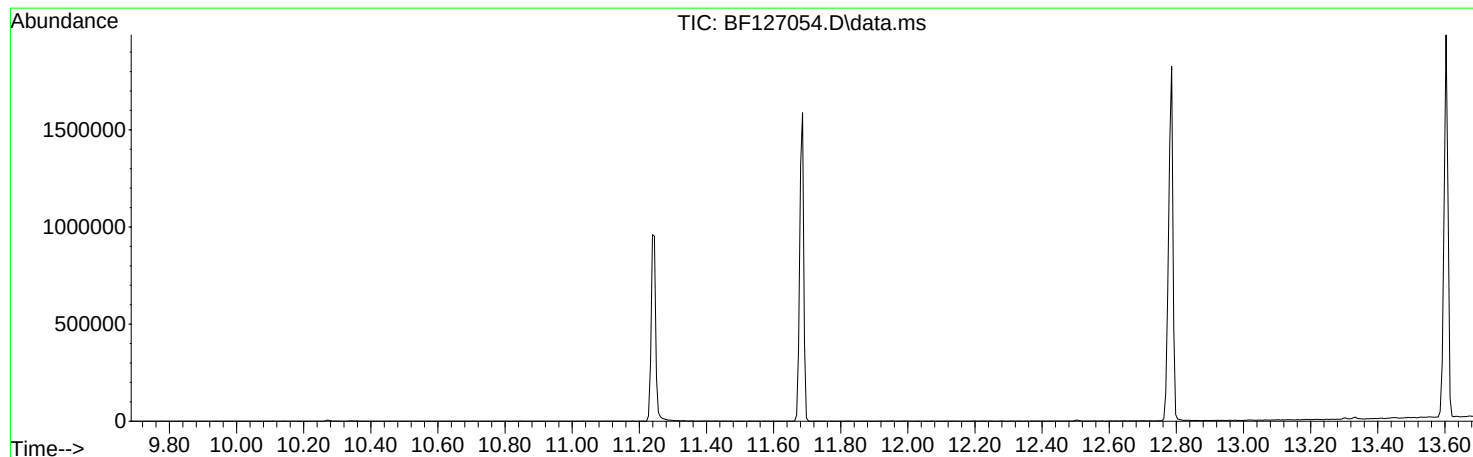




AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	47087	PASS
68	69	0.00	2	1.8	830	PASS
69	198	0.00	100	42.0	46350	PASS
70	69	0.00	2	0.5	245	PASS
127	198	10	80	55.2	60962	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	110344	PASS
199	198	5	9	6.6	7228	PASS
275	198	10	60	30.4	33514	PASS
365	198	1	100	4.9	5431	PASS
441	198	0.01	100	17.3	19125	PASS
442	442	50	100	100.0	122917	PASS
443	442	15	24	18.7	22965	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022422\
Data File : BF127054.D
Acq On : 24 Feb 2022 13:18
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 24 16:30:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 24 02:10:57 2022
Response via : Initial Calibration

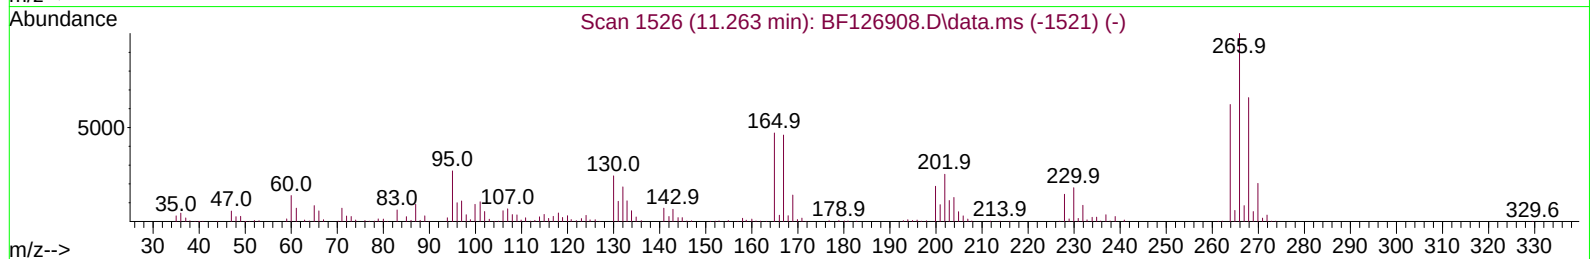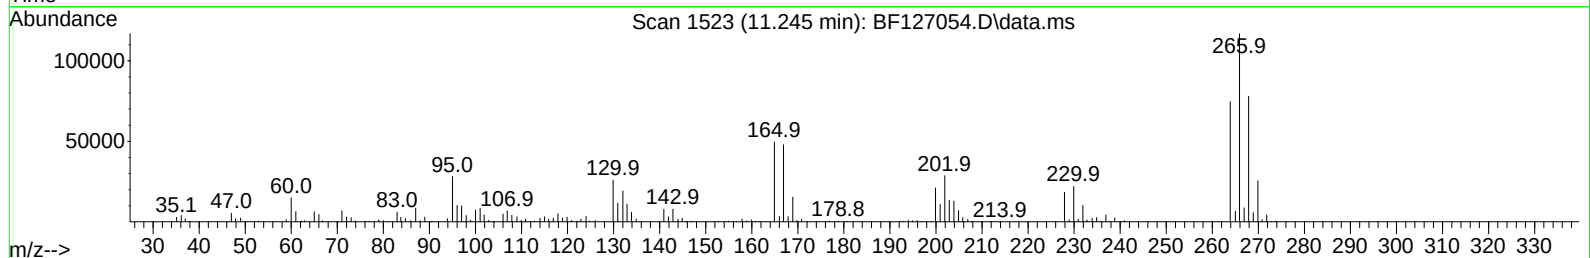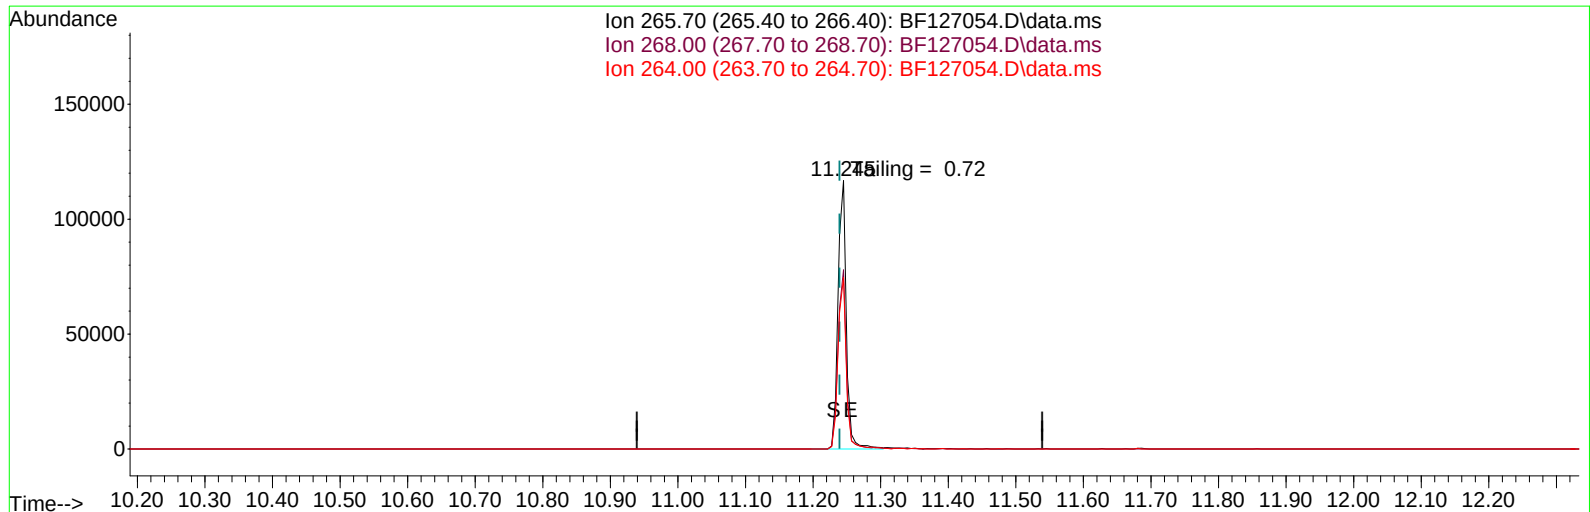

TIC: BF127054.D\data.ms

(70) Pentachlorophenol (C)

11.245min (+ 0.006) 31179.15 ng




response 99904

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.80
264.00	63.00	63.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022422\
Data File : BF127054.D
Acq On : 24 Feb 2022 13:18
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 24 16:30:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 24 02:10:57 2022
Response via : Initial Calibration

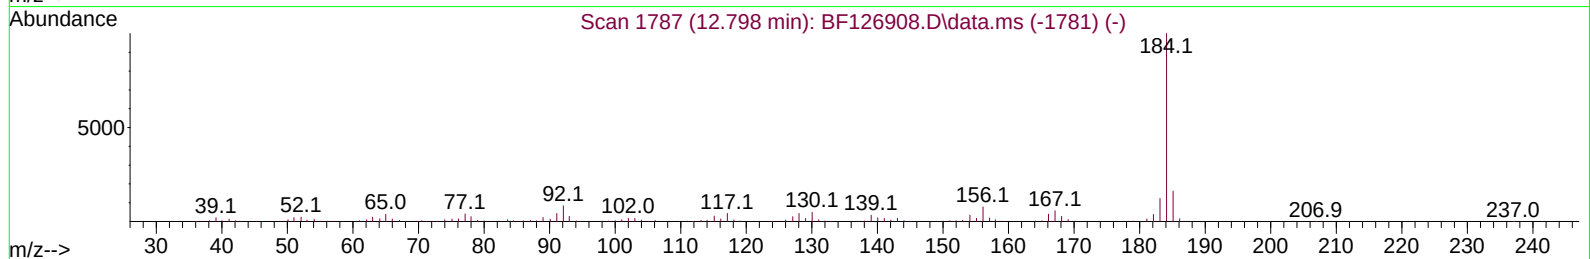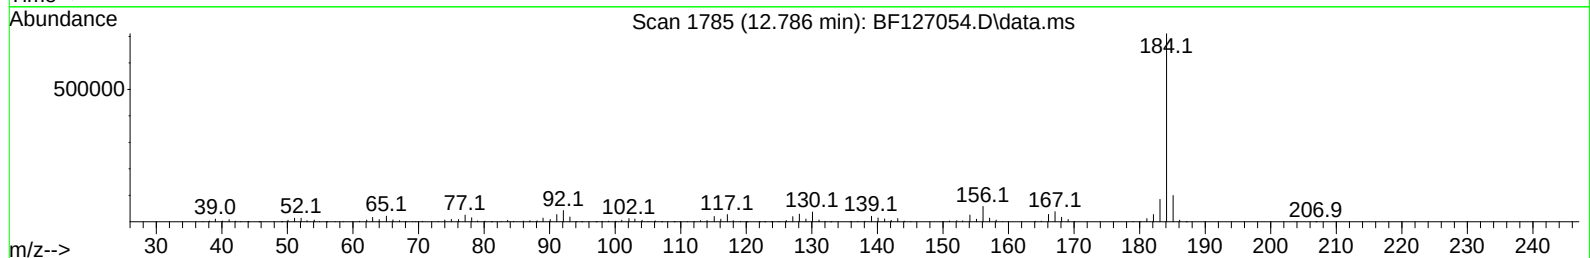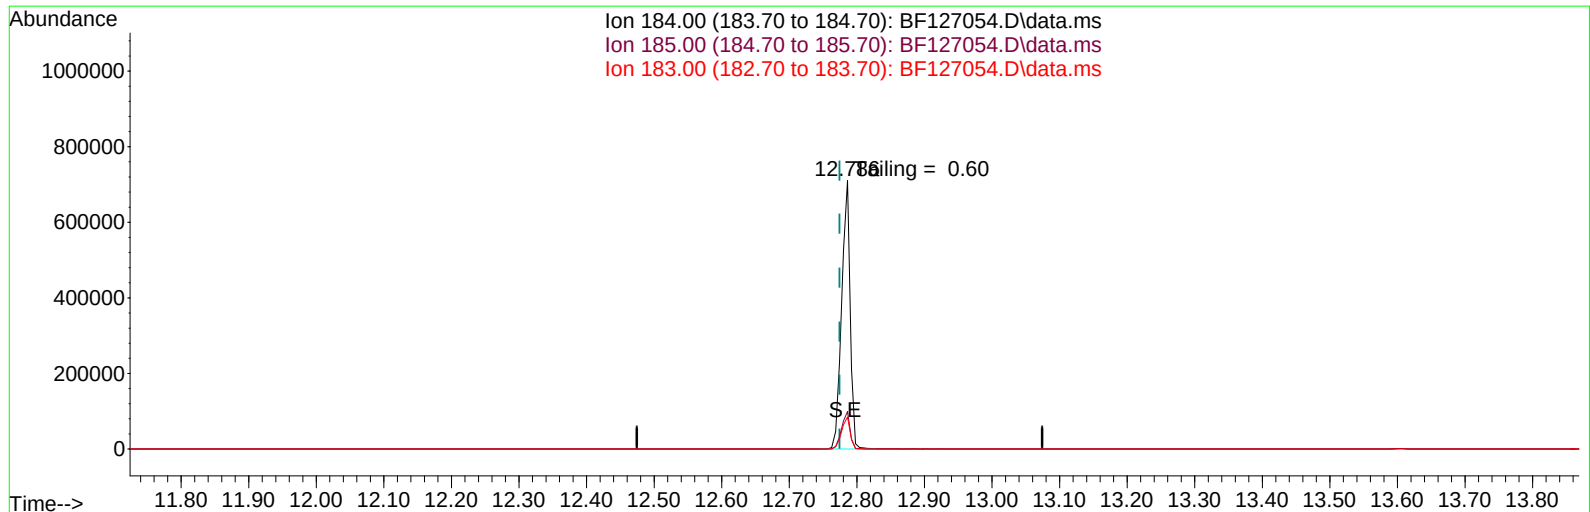

TIC: BF127054.D\data.ms

(77) Benzidine

12.786min (+ 0.012) 0.00 ng

response 620829

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.97
183.00	10.20	11.96
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/24/2022	BNA_F	<u>BF127054.D</u>
Compound Name	Response	Retention Time
DDT	283990	13.6
DDD	1345	13.3
DDE	147	12.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1492	285482	0.52

Instrument :
BNA_F
ClientSampleId :
DFTPP