

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030822\
 Data File : BF127262.D
 Acq On : 08 Mar 2022 17:01
 Operator : CG\JU
 Sample : N1763-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 31-32-SAMPLE-LOCATION-16

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127262.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.116	477	481	489	rVB	18095	25677	1.19%	0.190%
2	5.504	543	547	559	rBV	2137831	2033914	94.19%	15.079%
3	6.516	714	719	732	rBV	1989081	2039998	94.48%	15.124%
4	6.875	777	780	784	rBV	663667	546750	25.32%	4.054%
5	7.445	872	877	880	rBV	1424798	1318891	61.08%	9.778%
6	7.604	901	904	908	rVB	28721	26086	1.21%	0.193%
7	8.163	995	999	1002	rBV	768546	660067	30.57%	4.894%
8	9.239	1176	1182	1185	rBV	2448039	2159263	100.00%	16.009%
9	9.304	1190	1193	1197	rVB	47642	42351	1.96%	0.314%
10	9.798	1271	1277	1280	rBV5	41817	51908	2.40%	0.385%
11	9.922	1294	1298	1301	rBV	799096	683580	31.66%	5.068%
12	10.716	1429	1433	1436	rBV	1173201	1113260	51.56%	8.254%
13	11.227	1518	1520	1522	rVB2	38711	25509	1.18%	0.189%
14	11.410	1548	1551	1554	rBV	553639	510493	23.64%	3.785%
15	12.533	1740	1742	1745	rBV2	79315	67109	3.11%	0.498%
16	12.998	1818	1821	1824	rBV	1503469	1291347	59.80%	9.574%
17	13.874	1968	1970	1973	rVB	185422	155006	7.18%	1.149%
18	14.063	1999	2002	2005	rVB	421763	359176	16.63%	2.663%
19	15.562	2254	2257	2261	rVB	301134	377822	17.50%	2.801%

Sum of corrected areas: 13488207

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030822\
Data File : BF127262.D
Acq On : 08 Mar 2022 17:01
Operator : CG\JU
Sample : N1763-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
31-32-SAMPLE-LOCATION-16










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown12.533 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.533	2.63 ng	67109	Phenanthrene-d10	11.416

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isophthalic acid, 2-fluorophenyl...	386	C23H27FO4	1000344-65-8	27
2			N-Acrylonitril-2,2,6,6-tetrameth...	192	C12H20N2	077376-88-6	25
3			Cyclohexene, 4-(4-ethylcyclohexy...	262	C19H34	301643-32-3	18
4			Bicyclo[3.1.1]heptane-2-methanol...	154	C10H18O	000514-99-8	14
5			Amiphenazole	191	C9H9N3S	000490-55-1	11

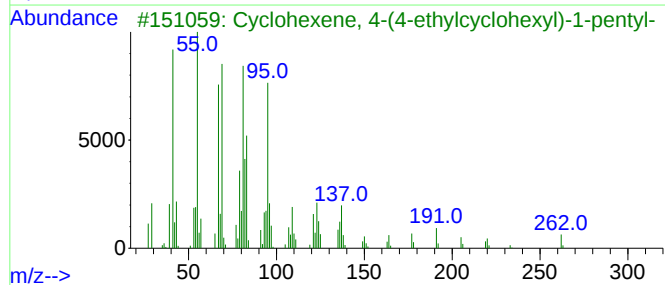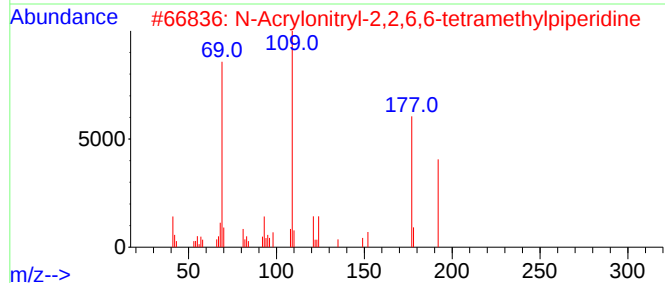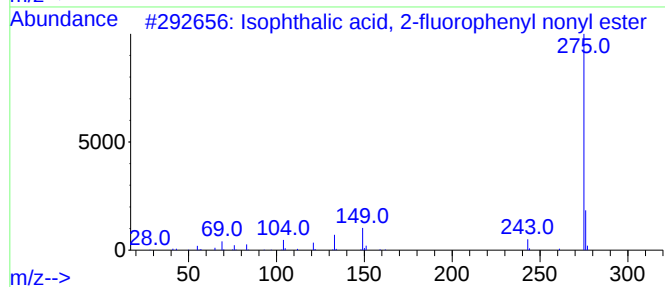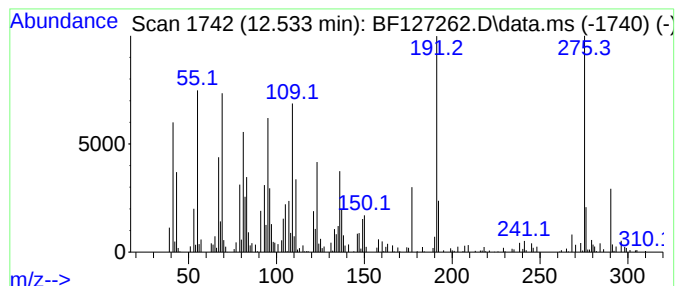

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030822\
Data File : BF127262.D
Acq On : 08 Mar 2022 17:01
Operator : CG\JU
Sample : N1763-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
31-32-SAMPLE-LOCATION-16









Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown13.874 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.874	8.63 ng	155006	Chrysene-d12	14.063

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	4-(1,3,3-Trimethyl-bicyclo[4.1.0...	206	C14H22O	077143-31-8	30		
2	Bicyclo[2.2.1]heptane, 2,2,3-tri...	138	C10H18	020536-41-8	20		
3	5-Hexen-1-one, 1-(1H-imidazol-4-...	192	C11H16N2O	069393-41-5	20		
4	(+)-(Z)-Longipinane	206	C15H26	1000156-12-3	18		
5	Bicyclo[2.2.1]heptane, 2,2,3-tri...	138	C10H18	000473-19-8	18		

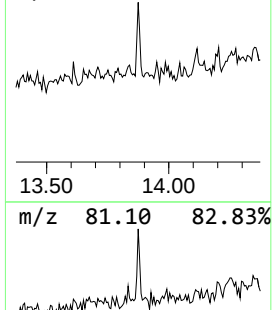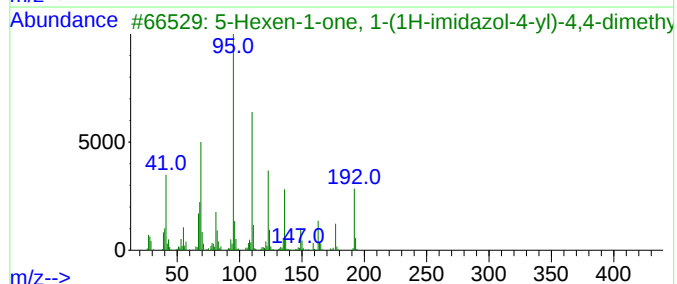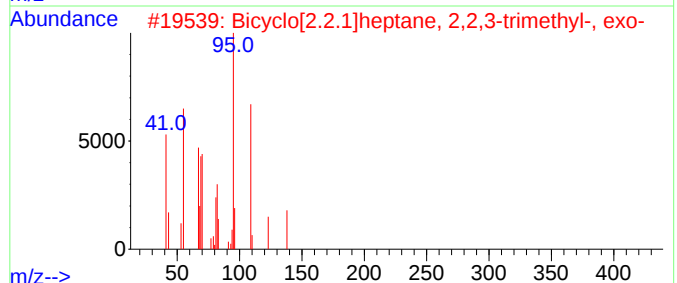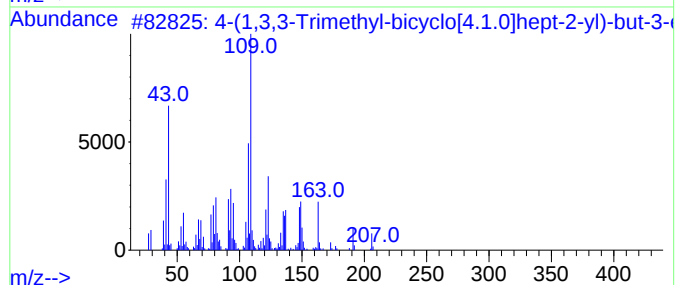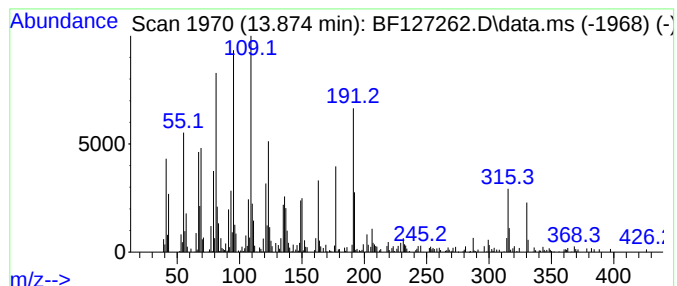

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030822\
Data File : BF127262.D
Acq On : 08 Mar 2022 17:01
Operator : CG\JU
Sample : N1763-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
31-32-SAMPLE-LOCATION-16

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown12.533	12.533	2.6	ng	67109	4	11.416	510493	20.0
unknown13.874	13.874	8.6	ng	155006	5	14.063	359176	20.0