

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030822\
 Data File : BF127270.D
 Acq On : 08 Mar 2022 20:55
 Operator : CG\JU
 Sample : N1832-01 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BU-02-03072022

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127270.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.498	542	546	557	rBV	555883	507245	2.23%	1.052%
2	6.510	714	718	731	rBV	542953	524107	2.30%	1.087%
3	6.881	777	781	784	rBV	843401	701227	3.08%	1.454%
4	7.439	872	876	879	rBV	416221	333492	1.46%	0.691%
5	8.163	995	999	1002	rBV	1078302	824554	3.62%	1.709%
6	9.233	1178	1181	1185	rBV	683673	555800	2.44%	1.152%
7	9.922	1292	1298	1301	rVV	1010833	775597	3.40%	1.608%
8	10.710	1430	1432	1437	rBV	257073	234216	1.03%	0.486%
9	11.416	1548	1552	1555	rBV	788568	670320	2.94%	1.390%
10	11.804	1613	1618	1621	rBV	6222925	6014896	26.39%	12.469%
11	12.510	1730	1738	1740	rBV	10687530	22792590	100.00%	47.250%
12	12.533	1740	1742	1746	rVV2	10355390	9630674	42.25%	19.965%
13	12.592	1749	1752	1756	rVB	3092326	2849395	12.50%	5.907%
14	13.004	1816	1822	1825	rBV	534392	467008	2.05%	0.968%
15	13.316	1872	1875	1880	rVB	308377	262774	1.15%	0.545%
16	13.980	1985	1988	1994	rBV	267935	249197	1.09%	0.517%
17	14.063	1999	2002	2006	rVB	541427	455592	2.00%	0.944%
18	15.557	2252	2256	2261	rVB	321484	389356	1.71%	0.807%




Sum of corrected areas: 48238040

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030822\
Data File : BF127270.D
Acq On : 08 Mar 2022 20:55
Operator : CG\JU
Sample : N1832-01 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-02-03072022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

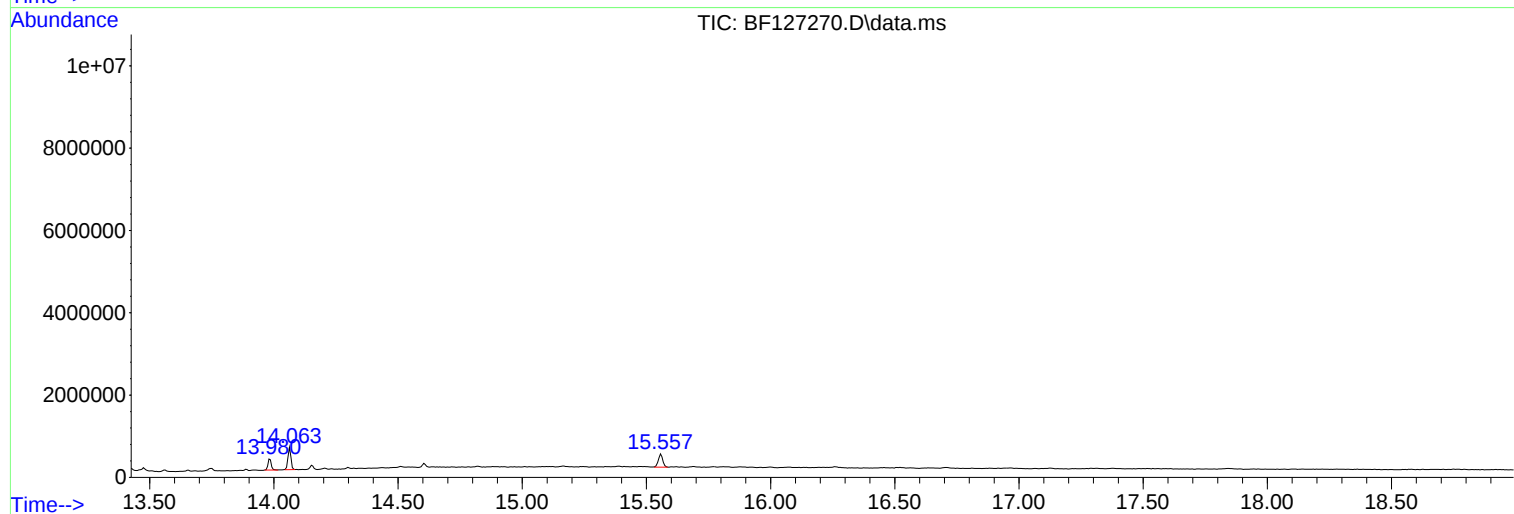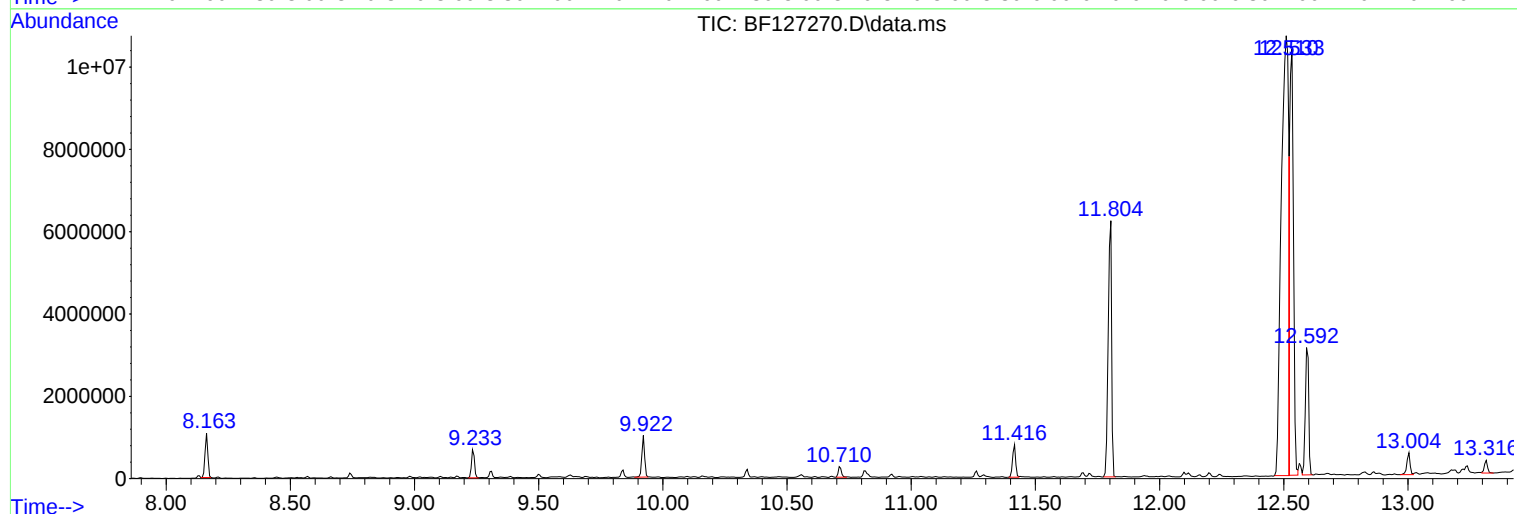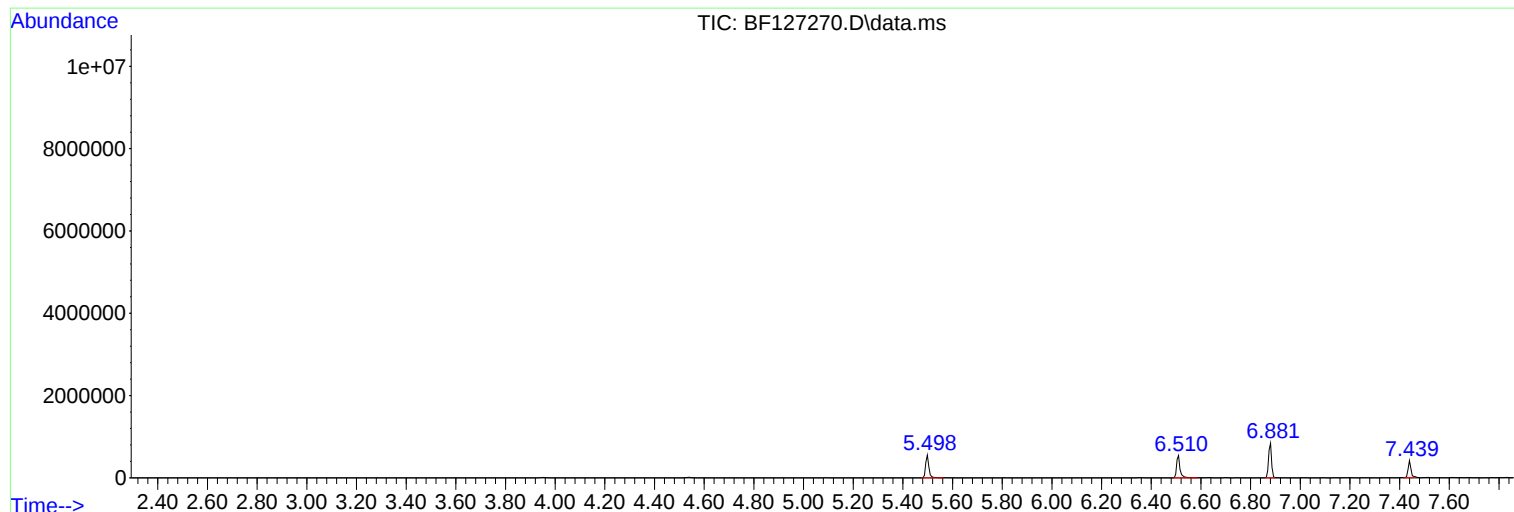

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030822\
Data File : BF127270.D
Acq On : 08 Mar 2022 20:55
Operator : CG\JU
Sample : N1832-01 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-02-03072022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030822\
Data File : BF127270.D
Acq On : 08 Mar 2022 20:55
Operator : CG\JU
Sample : N1832-01 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-02-03072022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc