

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030823\
 Data File : BF132696.D
 Acq On : 08 Mar 2023 18:24
 Operator : CG\JU
 Sample : 01825-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HH-TP2-0306

Quant Time: Mar 09 00:39:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 07 13:42:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.987	152	154572	20.000	ng	0.00
21) Naphthalene-d8	8.269	136	581701	20.000	ng	-0.01
39) Acenaphthene-d10	10.033	164	301769	20.000	ng	0.00
64) Phenanthrene-d10	11.527	188	534103	20.000	ng	0.00
76) Chrysene-d12	14.186	240	327388	20.000	ng	-0.01
86) Perylene-d12	15.727	264	384181	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.622	112	718003	75.389	ng	0.00
7) Phenol-d6	6.616	99	881740	70.938	ng	0.00
23) Nitrobenzene-d5	7.551	82	910492	74.261	ng	-0.01
42) 2,4,6-Tribromophenol	10.827	330	246099	75.514	ng	0.00
45) 2-Fluorobiphenyl	9.345	172	1463101	73.825	ng	-0.01
79) Terphenyl-d14	13.121	244	1547612	79.924	ng	0.00
Target Compounds						
						Qvalue
19) n-Nitroso-di-n-propyla...	7.551	70	119243	15.588	ng	# 76
25) Isophorone	7.551	82	910478	38.733	ng	# 67
27) 2,4-Dimethylphenol	7.998	122	24672	2.702	ng	# 1
32) Benzoic acid	7.998	122	24672	6.991	ng	# 88
51) 2,6-Dinitrotoluene	10.033	165	38488	7.691	ng	# 22
57) 2,4-Dinitrotoluene	10.033	165	38488	5.781	ng	# 21
67) 4-Bromophenyl-phenylether	10.827	248	15840	2.622	ng	# 1
77) Benzidine	12.868	184	189045	23.721	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030823\
Data File : BF132696.D
Acq On : 08 Mar 2023 18:24
Operator : CG\JU
Sample : 01825-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HH-TP2-0306

Quant Time: Mar 09 00:39:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 13:42:31 2023
Response via : Initial Calibration




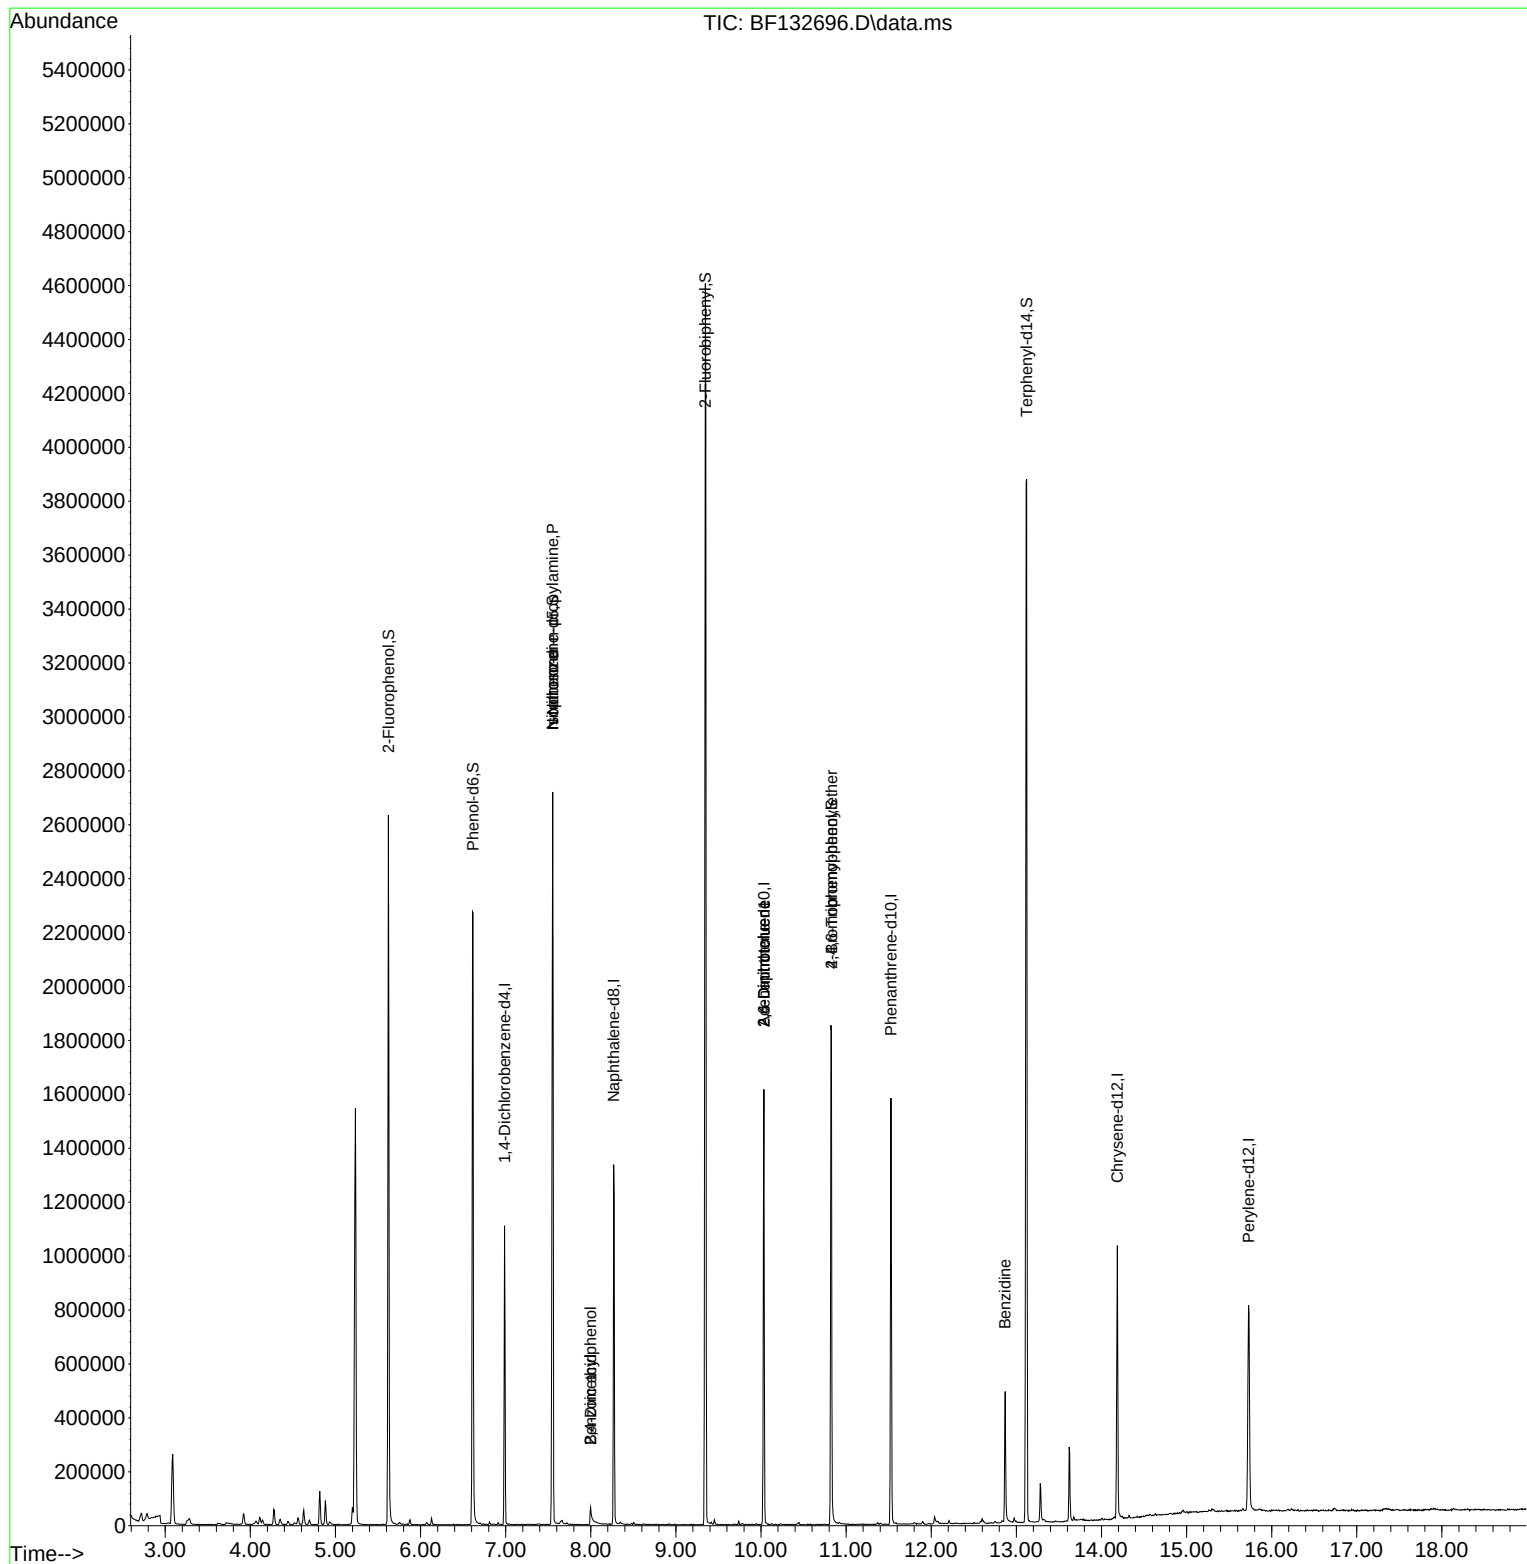




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.987 min Scan# 710
Delta R.T. -0.006 min
Lab File: BF132696.D
Acq: 08 Mar 2023 18:24




Instrument :
BNA_F
ClientSampleId :
HH-TP2-0306


Tgt Ion:152 Resp: 154572
Ion Ratio Lower Upper
152 100
150 154.5 125.4 188.2
115 61.4 47.8 71.6

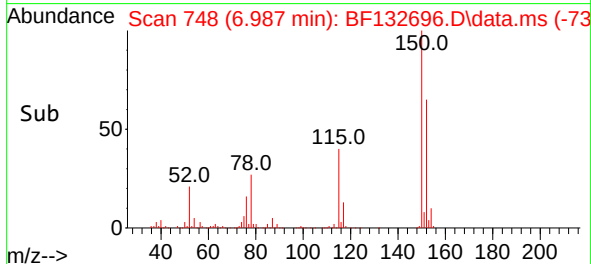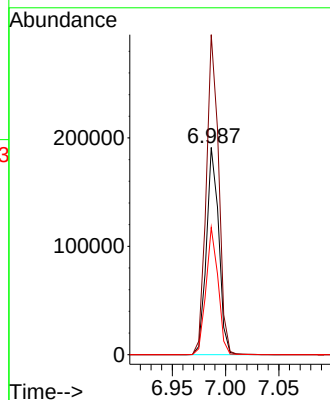

#5
2-Fluorophenol
Concen: 75.389 ng
RT: 5.622 min Scan# 516
Delta R.T. 0.006 min
Lab File: BF132696.D
Acq: 08 Mar 2023 18:24

Tgt Ion:112 Resp: 718003
Ion Ratio Lower Upper
112 100
64 60.1 51.6 77.4
63 30.2 27.4 41.2


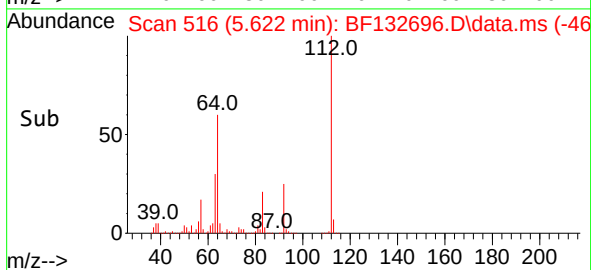
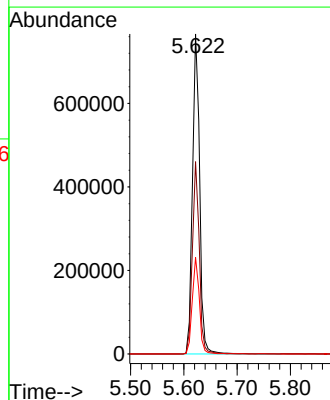
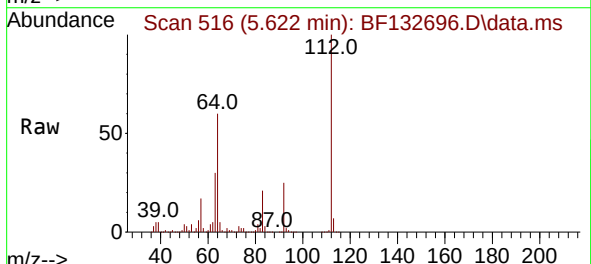




#7
Phenol-d6
Concen: 70.938 ng
RT: 6.616 min Scan# 61
Delta R.T. -0.006 min
Lab File: BF132696.D
Acq: 08 Mar 2023 18:24




Instrument :
BNA_F
ClientSampleId :
HH-TP2-0306


Tgt Ion: 99 Resp: 881740
Ion Ratio Lower Upper
99 100
42 14.6 13.9 20.9
71 31.7 28.5 42.7

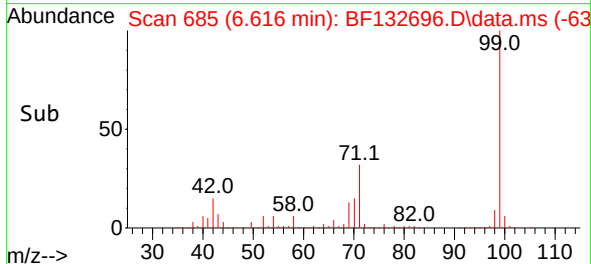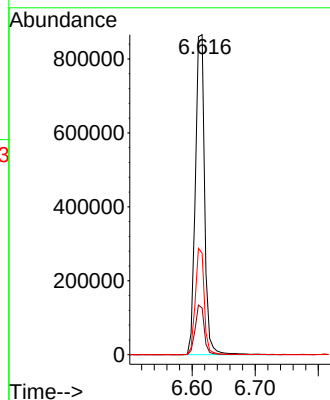

#19
n-Nitroso-di-n-propylamine
Concen: 15.588 ng
RT: 7.551 min Scan# 844
Delta R.T. 0.147 min
Lab File: BF132696.D
Acq: 08 Mar 2023 18:24

Tgt Ion: 70 Resp: 119243
Ion Ratio Lower Upper
70 100
42 40.2 44.1 66.1#
101 0.0 7.4 11.2#
130 2.2 14.2 21.4#



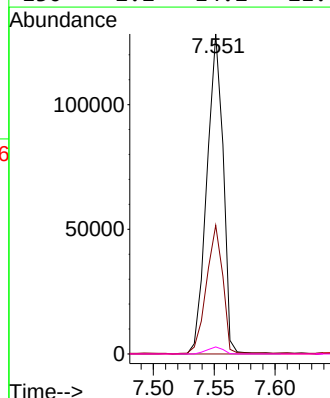
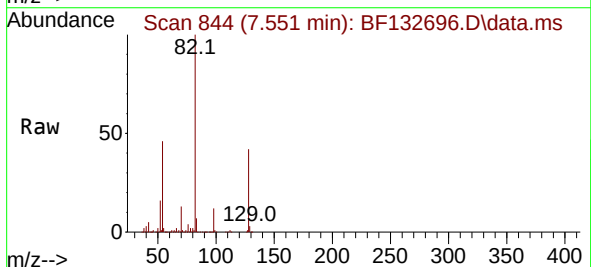




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.269 min Scan# 91
Delta R.T. -0.012 min
Lab File: BF132696.D
Acq: 08 Mar 2023 18:24




Instrument :
BNA_F
ClientSampleId :
HH-TP2-0306


Tgt Ion:136 Resp: 581701
Ion Ratio Lower Upper
136 100
137 11.0 8.9 13.3
54 8.0 6.2 9.4
68 7.2 5.2 7.8

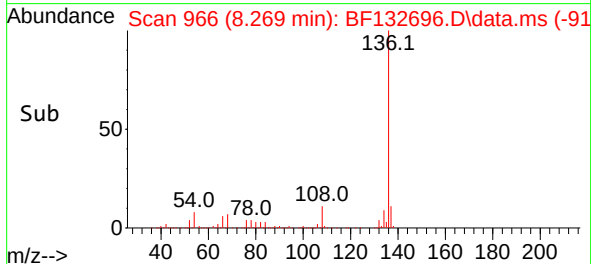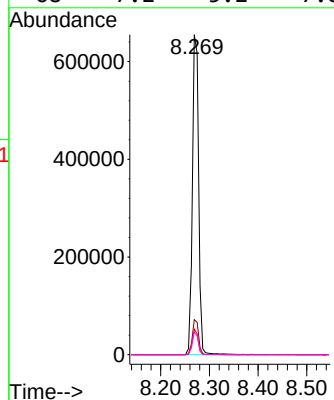

#23
Nitrobenzene-d5
Concen: 74.261 ng
RT: 7.551 min Scan# 844
Delta R.T. -0.012 min
Lab File: BF132696.D
Acq: 08 Mar 2023 18:24

Tgt Ion: 82 Resp: 910492
Ion Ratio Lower Upper
82 100
128 41.6 32.2 48.2
54 46.3 38.4 57.6


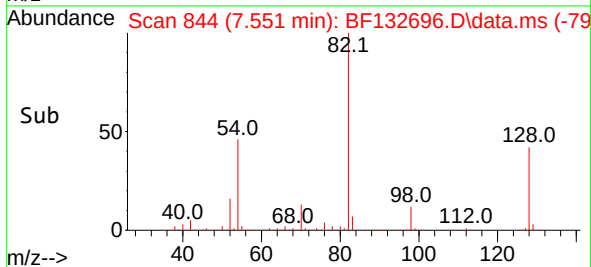
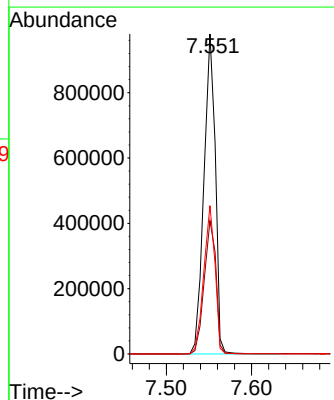
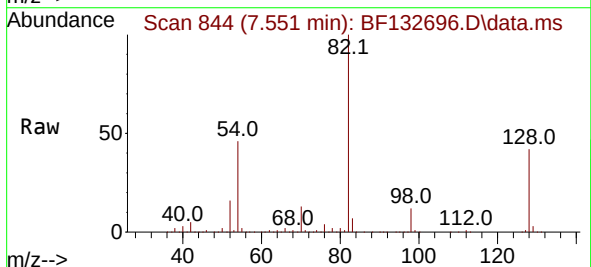




#25
Isophorone
Concen: 38.733 ng
RT: 7.551 min Scan# 84
Delta R.T. -0.265 min
Lab File: BF132696.D
Acq: 08 Mar 2023 18:24




Instrument :
BNA_F
ClientSampleId :
HH-TP2-0306


Tgt Ion: 82 Resp: 910478
Ion Ratio Lower Upper
82 100
95 0.0 5.7 8.5#
138 0.0 13.3 19.9#

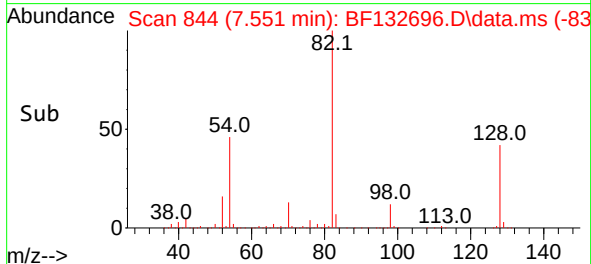

#27
2,4-Dimethylphenol
Concen: 2.702 ng
RT: 7.998 min Scan# 920
Delta R.T. 0.070 min
Lab File: BF132696.D
Acq: 08 Mar 2023 18:24

Tgt Ion: 122 Resp: 24672
Ion Ratio Lower Upper
122 100
107 0.0 98.7 148.1#
121 0.0 45.8 68.6#


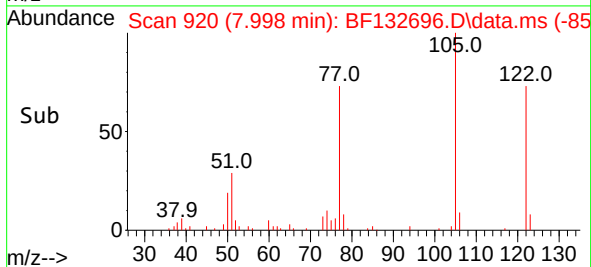

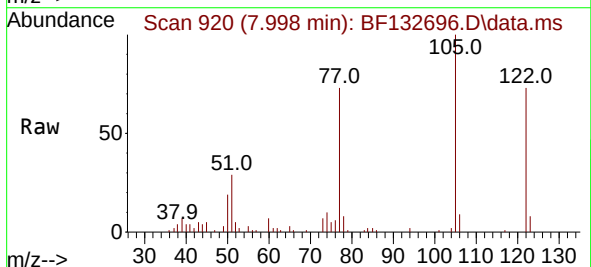




#32
Benzoic acid
Concen: 6.991 ng
RT: 7.998 min Scan# 91
Delta R.T. -0.059 min
Lab File: BF132696.D
Acq: 08 Mar 2023 18:24




Instrument :
BNA_F
ClientSampleId :
HH-TP2-0306


Tgt Ion:122 Resp: 24672
Ion Ratio Lower Upper
122 100
105 136.9 102.6 142.6
77 99.9 70.2 110.2

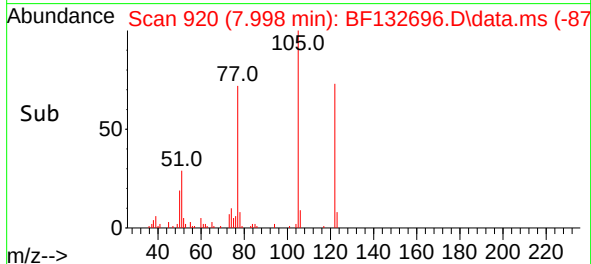

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.033 min Scan# 1266
Delta R.T. -0.006 min
Lab File: BF132696.D
Acq: 08 Mar 2023 18:24

Tgt Ion:164 Resp: 301769
Ion Ratio Lower Upper
164 100
162 101.6 79.8 119.8
160 44.8 35.8 53.6


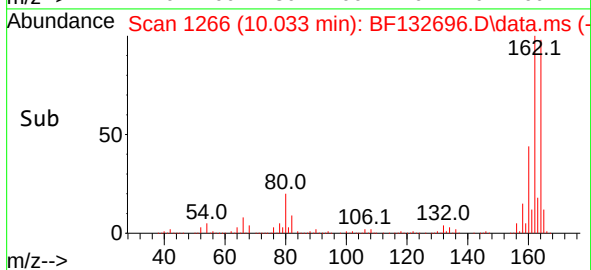

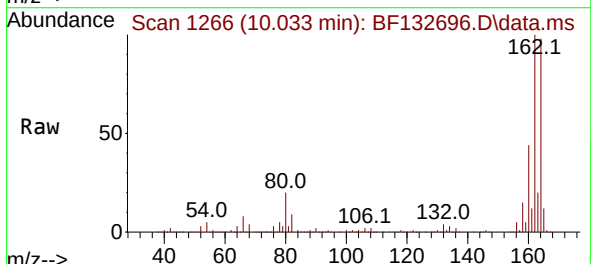




#42
2,4,6-Tribromophenol
Concen: 75.514 ng
RT: 10.827 min Scan# 1149
Delta R.T. -0.006 min
Lab File: BF132696.D
Acq: 08 Mar 2023 18:24




Instrument :
BNA_F
ClientSampleId :
HH-TP2-0306


Tgt Ion:330 Resp: 246099
Ion Ratio Lower Upper
330 100
332 94.9 76.2 114.4
141 33.5 28.4 42.6

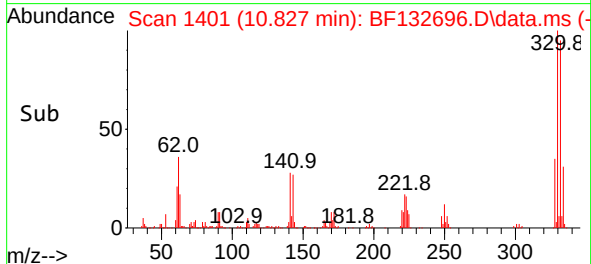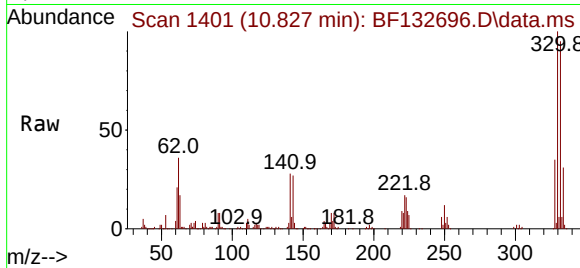

#45
2-Fluorobiphenyl
Concen: 73.825 ng
RT: 9.345 min Scan# 1149
Delta R.T. -0.012 min
Lab File: BF132696.D
Acq: 08 Mar 2023 18:24

Tgt Ion:172 Resp: 1463101
Ion Ratio Lower Upper
172 100
171 35.1 28.8 43.2
170 24.5 19.7 29.5


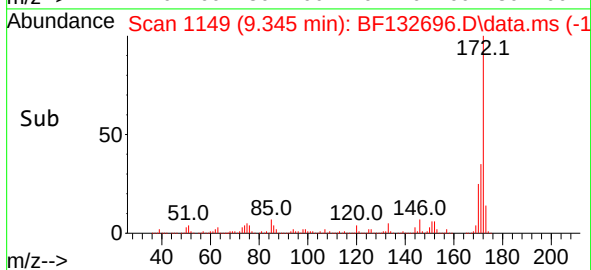

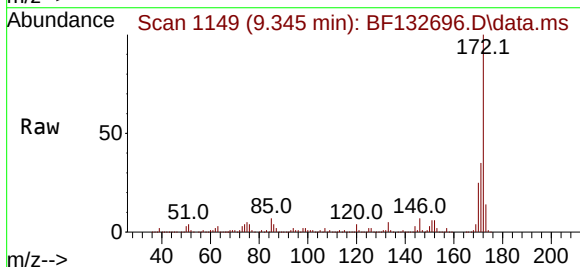




#51
2,6-Dinitrotoluene
Concen: 7.691 ng
RT: 10.033 min Scan# 1191
Delta R.T. 0.212 min
Lab File: BF132696.D
Acq: 08 Mar 2023 18:24




Instrument :
BNA_F
ClientSampleId :
HH-TP2-0306


Tgt Ion:165 Resp: 38488
Ion Ratio Lower Upper
165 100
63 0.8 47.3 70.9#
89 0.9 48.9 73.3#

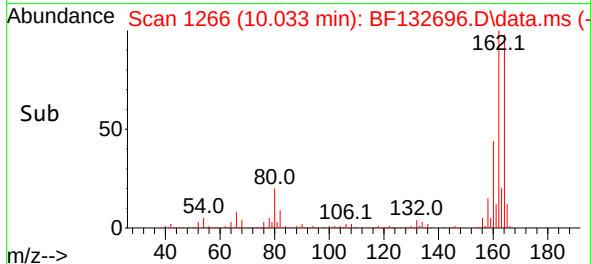

#57
2,4-Dinitrotoluene
Concen: 5.781 ng
RT: 10.033 min Scan# 1266
Delta R.T. -0.194 min
Lab File: BF132696.D
Acq: 08 Mar 2023 18:24

Tgt Ion:165 Resp: 38488
Ion Ratio Lower Upper
165 100
63 0.8 36.5 54.7#
89 0.9 62.4 93.6#
182 0.0 2.1 3.1#



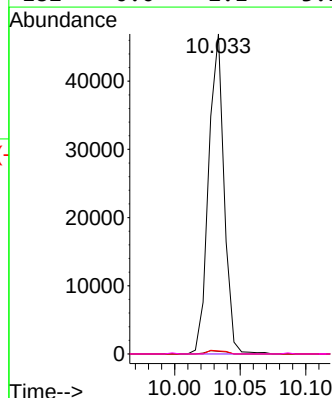
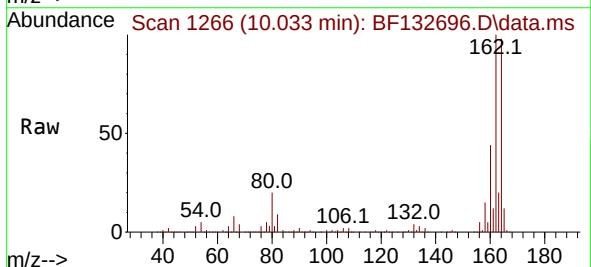


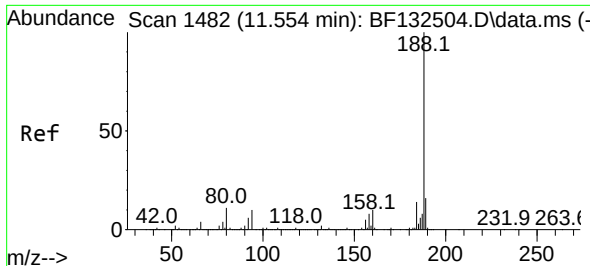

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.527 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF132696.D
Acq: 08 Mar 2023 18:24




Instrument :
BNA_F
ClientSampleId :
HH-TP2-0306


Tgt Ion:188 Resp: 534103
Ion Ratio Lower Upper
188 100
94 9.2 8.3 12.5
80 10.1 8.7 13.1

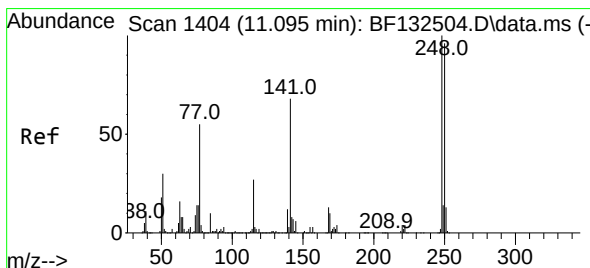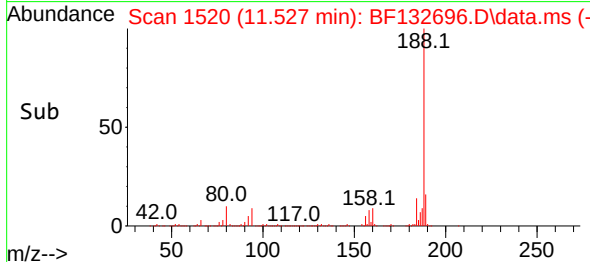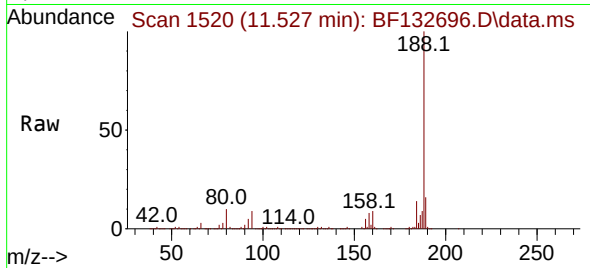

#67
4-Bromophenyl-phenylether
Concen: 2.622 ng
RT: 10.827 min Scan# 1401
Delta R.T. -0.247 min
Lab File: BF132696.D
Acq: 08 Mar 2023 18:24

Tgt Ion:248 Resp: 15840
Ion Ratio Lower Upper
248 100
250 198.0 77.0 115.4#
141 461.8 54.2 81.2#

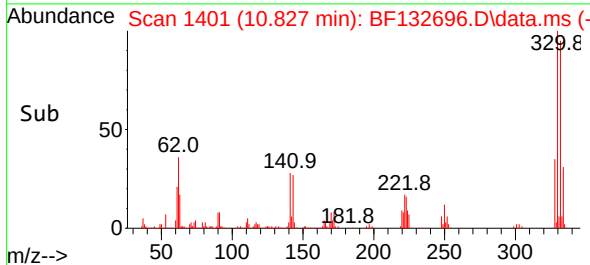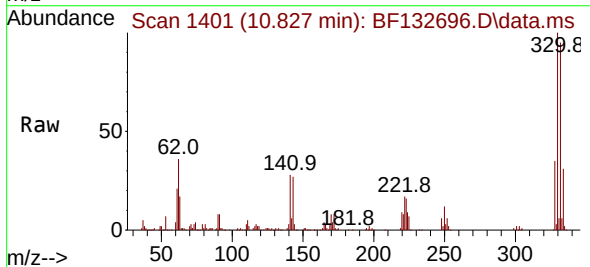



#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.186 min Scan# 1935

Delta R.T. -0.012 min

Lab File: BF132696.D

Acq: 08 Mar 2023 18:24

Instrument :

BNA_F

ClientSampleId :

HH-TP2-0306





Tgt Ion:240 Resp: 327388

Ion Ratio Lower Upper

240 100

120 10.4 7.2 10.8

236 26.9 21.8 32.6

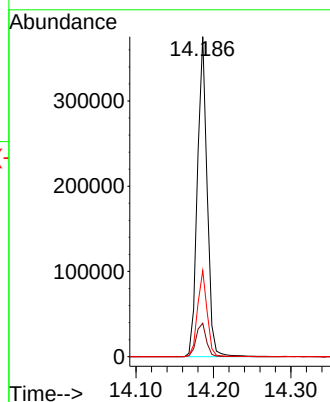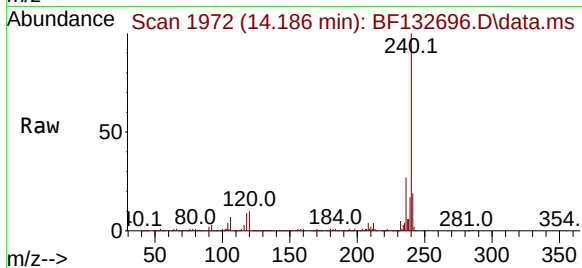

#77

Benzidine

Concen: 23.721 ng

RT: 12.868 min Scan# 1748

Delta R.T. -0.006 min

Lab File: BF132696.D

Acq: 08 Mar 2023 18:24




Tgt Ion:184 Resp: 189045


Ion Ratio Lower Upper

184 100

185 14.3 11.7 17.5

183 11.0 8.7 13.1


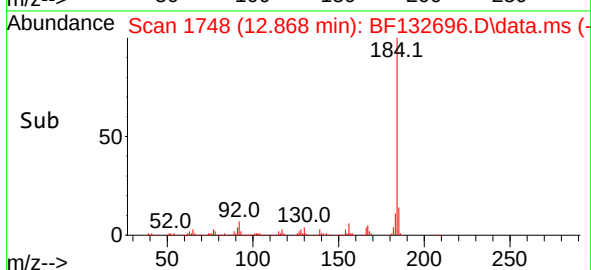
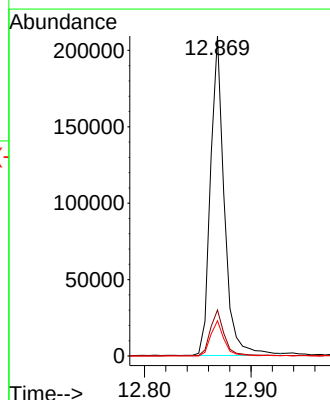
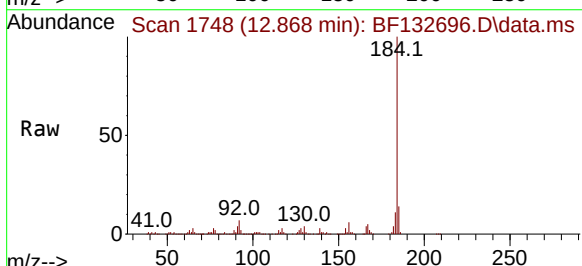




#79
 Terphenyl-d14
 Concen: 79.924 ng
 RT: 13.121 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BF132696.D
 Acq: 08 Mar 2023 18:24

Instrument :
 BNA_F
 ClientSampleId :
 HH-TP2-0306

Tgt Ion:244 Resp: 1547612
 Ion Ratio Lower Upper
 244 100
 212 7.5 6.5 9.7
 122 8.3 7.5 11.3

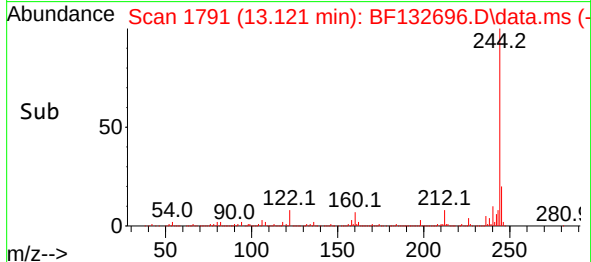

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.727 min Scan# 2234
 Delta R.T. -0.012 min
 Lab File: BF132696.D
 Acq: 08 Mar 2023 18:24

Tgt Ion:264 Resp: 384181
 Ion Ratio Lower Upper
 264 100
 260 23.7 18.8 28.2
 265 21.0 17.1 25.7

