
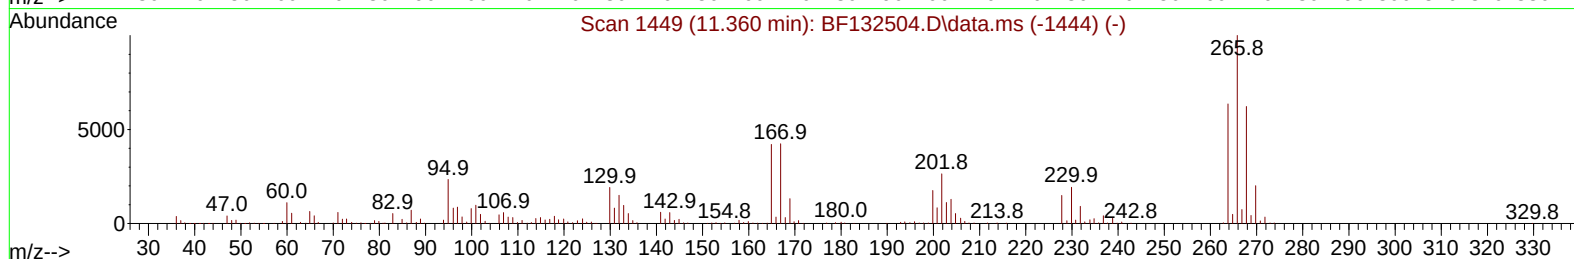
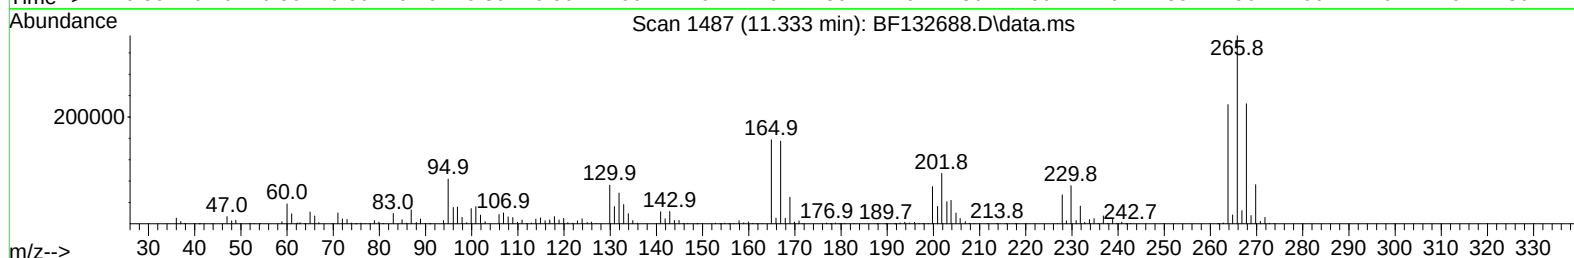


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030823\
Data File : BF132688.D
Acq On : 08 Mar 2023 13:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 09 04:57:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 13:42:31 2023
Response via : Initial Calibration

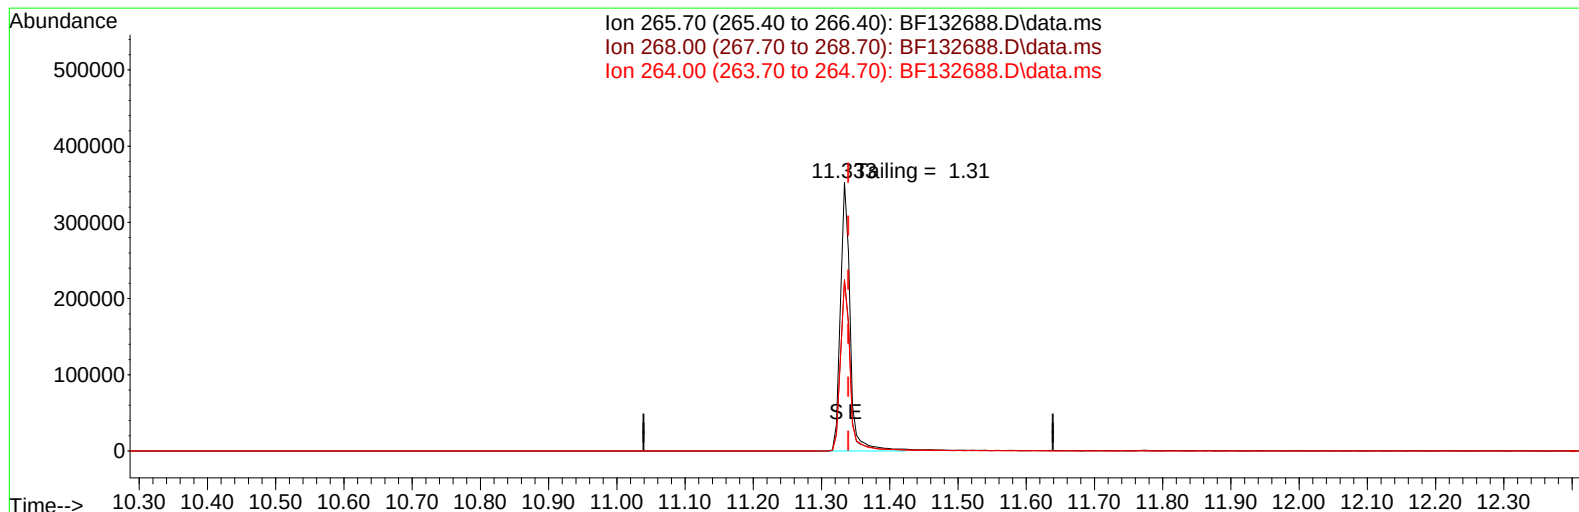

TIC: BF132688.D\data.ms

(70) Pentachlorophenol (C)




11.333min (-0.006) 304594.52 ng

response 347275

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.81
264.00	63.60	63.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030823\
 Data File : BF132688.D
 Acq On : 08 Mar 2023 13:23
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 09 04:57:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 07 13:42:31 2023
 Response via : Initial Calibration

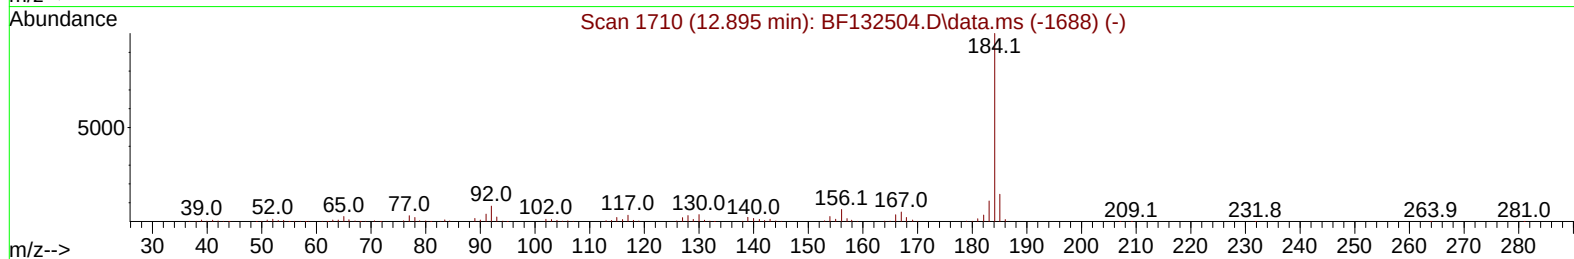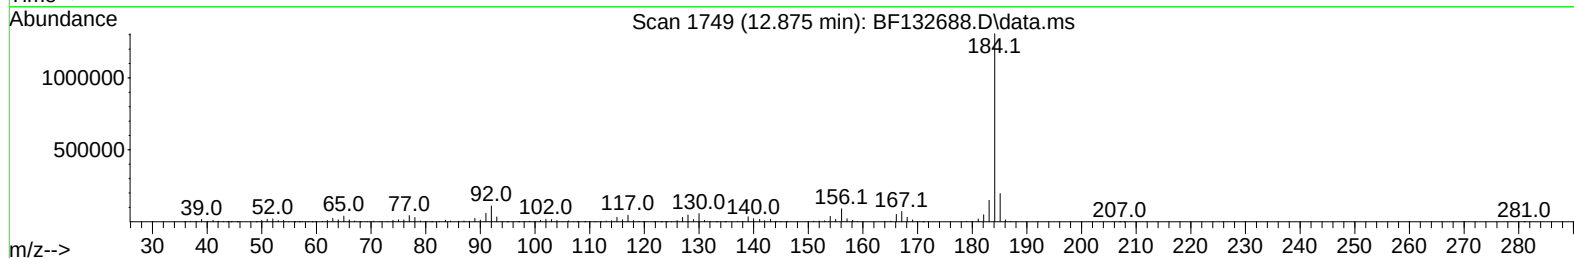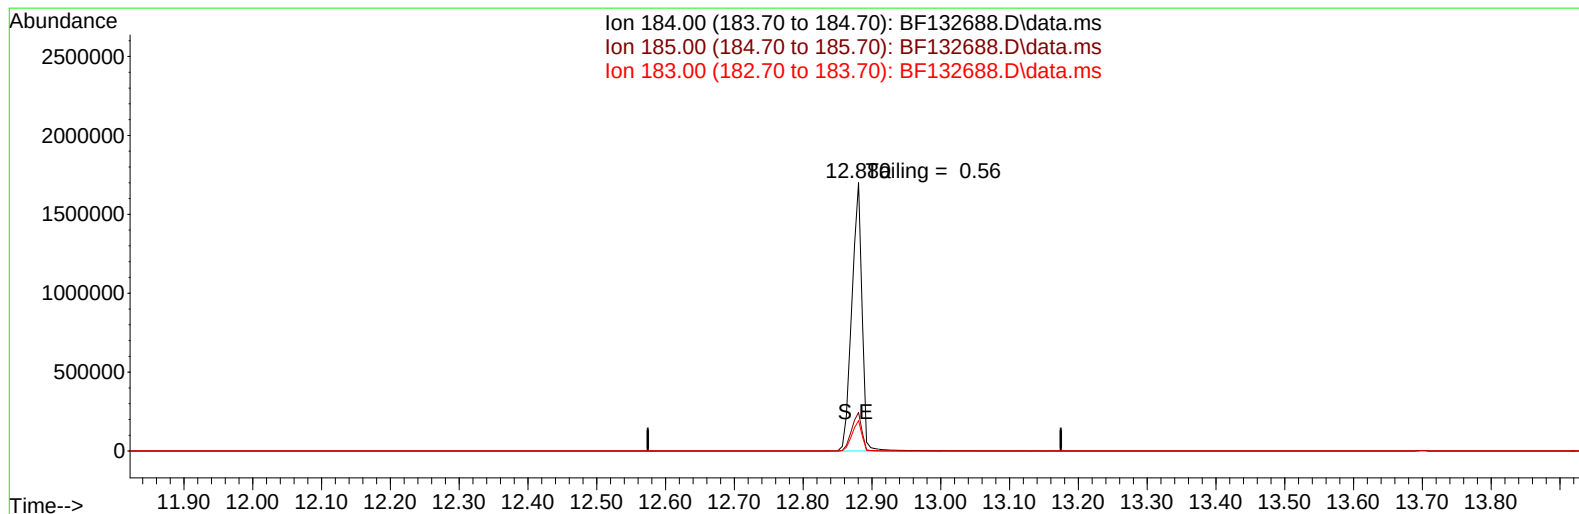

TIC: BF132688.D\data.ms

(77) Benzidine

12.875min (-12.875) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	14.60	0.00#
183.00	10.90	0.00#
0.00	0.00	0.00