

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030823\
 Data File : BF132690.D
 Acq On : 08 Mar 2023 15:01
 Operator : CG\JU
 Sample : PB151303BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB151303BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF132690.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.640	345	349	357	rVB	160094	185796	2.77%	0.443%
2	5.240	445	451	467	rVB	1717445	2457770	36.69%	5.859%
3	5.628	512	517	520	rBV	4669810	4932529	73.64%	11.758%
4	6.622	680	686	689	rBV	3901346	4893001	73.05%	11.664%
5	6.986	744	748	752	rBV	1379582	1103903	16.48%	2.632%
6	7.557	839	845	848	rBV	3266522	3323637	49.62%	7.923%
7	8.275	962	967	970	rBV	1619447	1454733	21.72%	3.468%
8	9.351	1143	1150	1153	rBV	6307234	5955971	88.92%	14.198%
9	10.033	1262	1266	1269	rBV	2112777	1765400	26.36%	4.208%
10	10.827	1397	1401	1405	rBV	3877255	4004768	59.79%	9.547%
11	11.527	1516	1520	1524	rBV	2198871	1873145	27.96%	4.465%
12	12.921	1754	1757	1761	rBV	92165	68426	1.02%	0.163%
13	13.121	1786	1791	1795	rBV	6090086	6698347	100.00%	15.968%
14	13.633	1873	1878	1882	rBV	83014	77701	1.16%	0.185%
15	14.186	1968	1972	1985	rBV	1609384	1473061	21.99%	3.512%
16	15.733	2229	2235	2245	rBV	740747	1079175	16.11%	2.573%
17	17.903	2589	2604	2616	rBV3	131428	602134	8.99%	1.435%




Sum of corrected areas: 41949497

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030823\
Data File : BF132690.D
Acq On : 08 Mar 2023 15:01
Operator : CG\JU
Sample : PB151303BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB151303BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: rteint.p

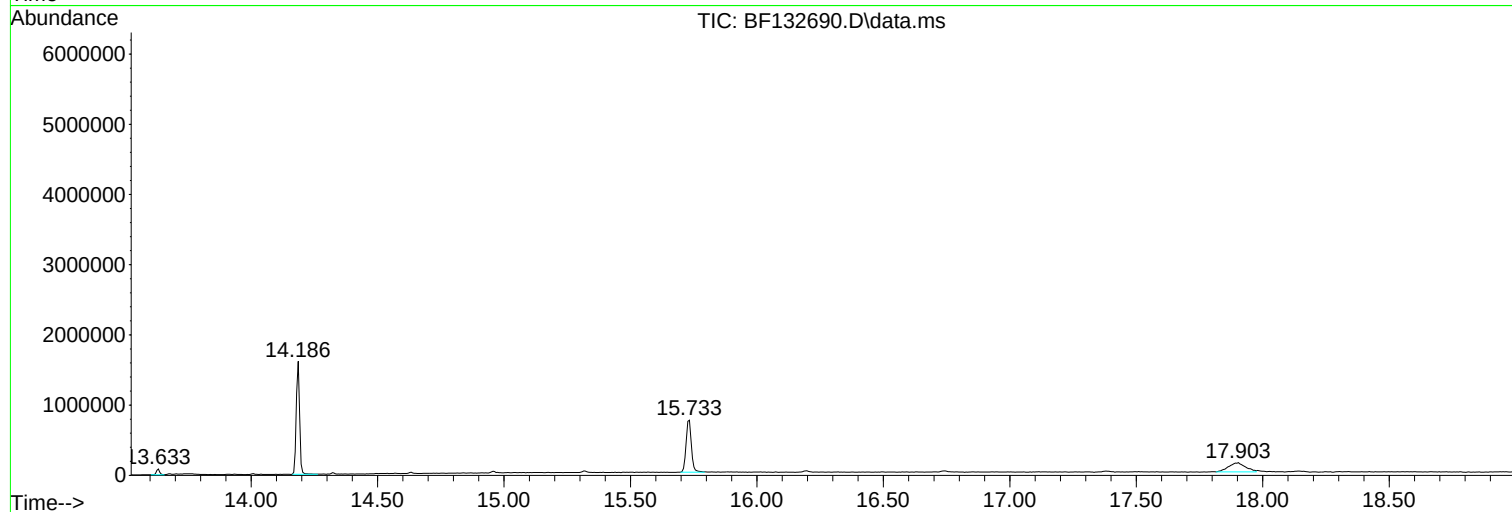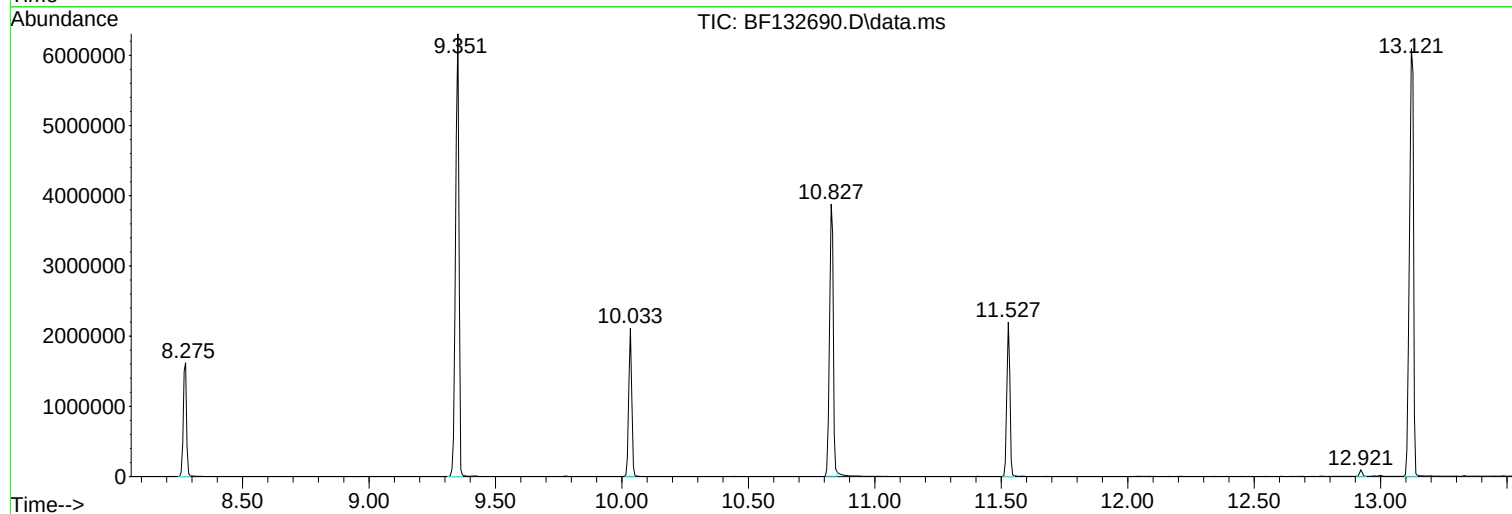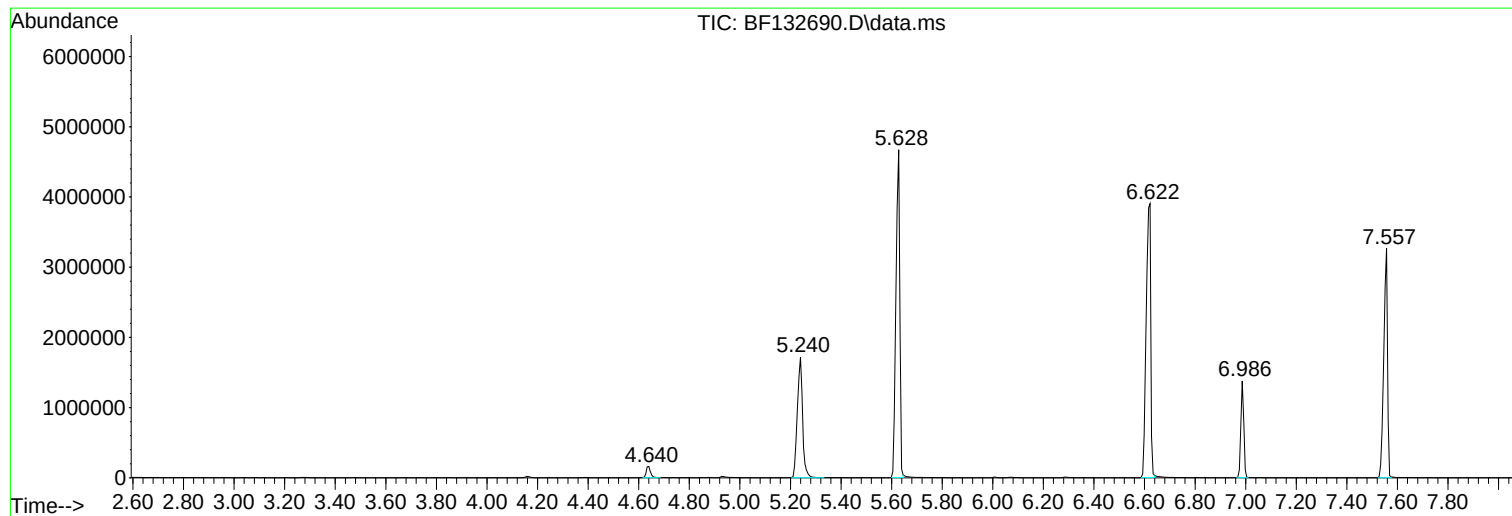

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030823\
Data File : BF132690.D
Acq On : 08 Mar 2023 15:01
Operator : CG\JU
Sample : PB151303BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB151303BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030823\
Data File : BF132690.D
Acq On : 08 Mar 2023 15:01
Operator : CG\JU
Sample : PB151303BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB151303BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------